

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
 Data File : PD076013.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 21:30
 Operator : AR\AJ
 Sample : 03101-04MS
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEL8MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/22/2023
 Supervised By :Ankita Jodhani 06/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:29:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	34562731	14794100	16.487	13.825
27)	SA Decachlor...	9.082	7.910	38297450	21536784	15.933	20.556 #
Target Compounds							
2)	A alpha-BHC	4.001	3.269	183.6E6	79876631	53.252m	51.754
3)	MA gamma-BHC...	4.335	3.599	161.2E6	72357289	49.888	49.757
4)	MA Heptachlor	4.926	3.939	170.1E6	73705233	50.484	49.655
5)	MB Aldrin	5.269	4.219	174.5E6	77256510	53.741	53.425
6)	B beta-BHC	4.531	3.895	67645446	30334256	46.559	44.443
7)	B delta-BHC	4.780	4.126	143.3E6	70538444	48.531	48.448
8)	B Heptachlo...	5.696	4.721	148.4E6	65683222	50.495	48.504
9)	A Endosulfan I	6.083	5.091	140.3E6	60656849	50.891	49.295
10)	B trans-Chl...	5.953	4.971	151.1E6	67987745	51.747	51.496
11)	B cis-Chlor...	6.032	5.036	158.2E6	68375011	52.187	49.798
12)	B 4,4'-DDE	6.204	5.224	314.5E6	132.5E6	112.948	114.965
13)	MA Dieldrin	6.358	5.356	330.0E6	144.3E6	107.114	103.500
14)	MA Endrin	6.589	5.631	280.8E6	127.8E6	107.679	103.327
15)	B Endosulfa...	6.808	5.925	272.9E6	120.8E6	106.581	102.478
16)	A 4,4'-DDD	6.722	5.779	240.9E6	102.4E6	111.666	111.869
17)	MA 4,4'-DDT	7.037	6.030	265.4E6	112.4E6	121.148	121.249
18)	B Endrin al...	6.938	6.105	183.9E6	81769218	96.120	94.522
19)	B Endosulfa...	7.173	6.328	244.0E6	111.2E6	101.154	101.224
20)	A Methoxychlor	7.512	6.606	684.0E6	281.7E6	517.930	522.735
21)	B Endrin ke...	7.660	6.834	279.6E6	128.9E6	103.403	103.031

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD076013.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 21:30
Operator : AR\AJ
Sample : 03101-04MS
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:29:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

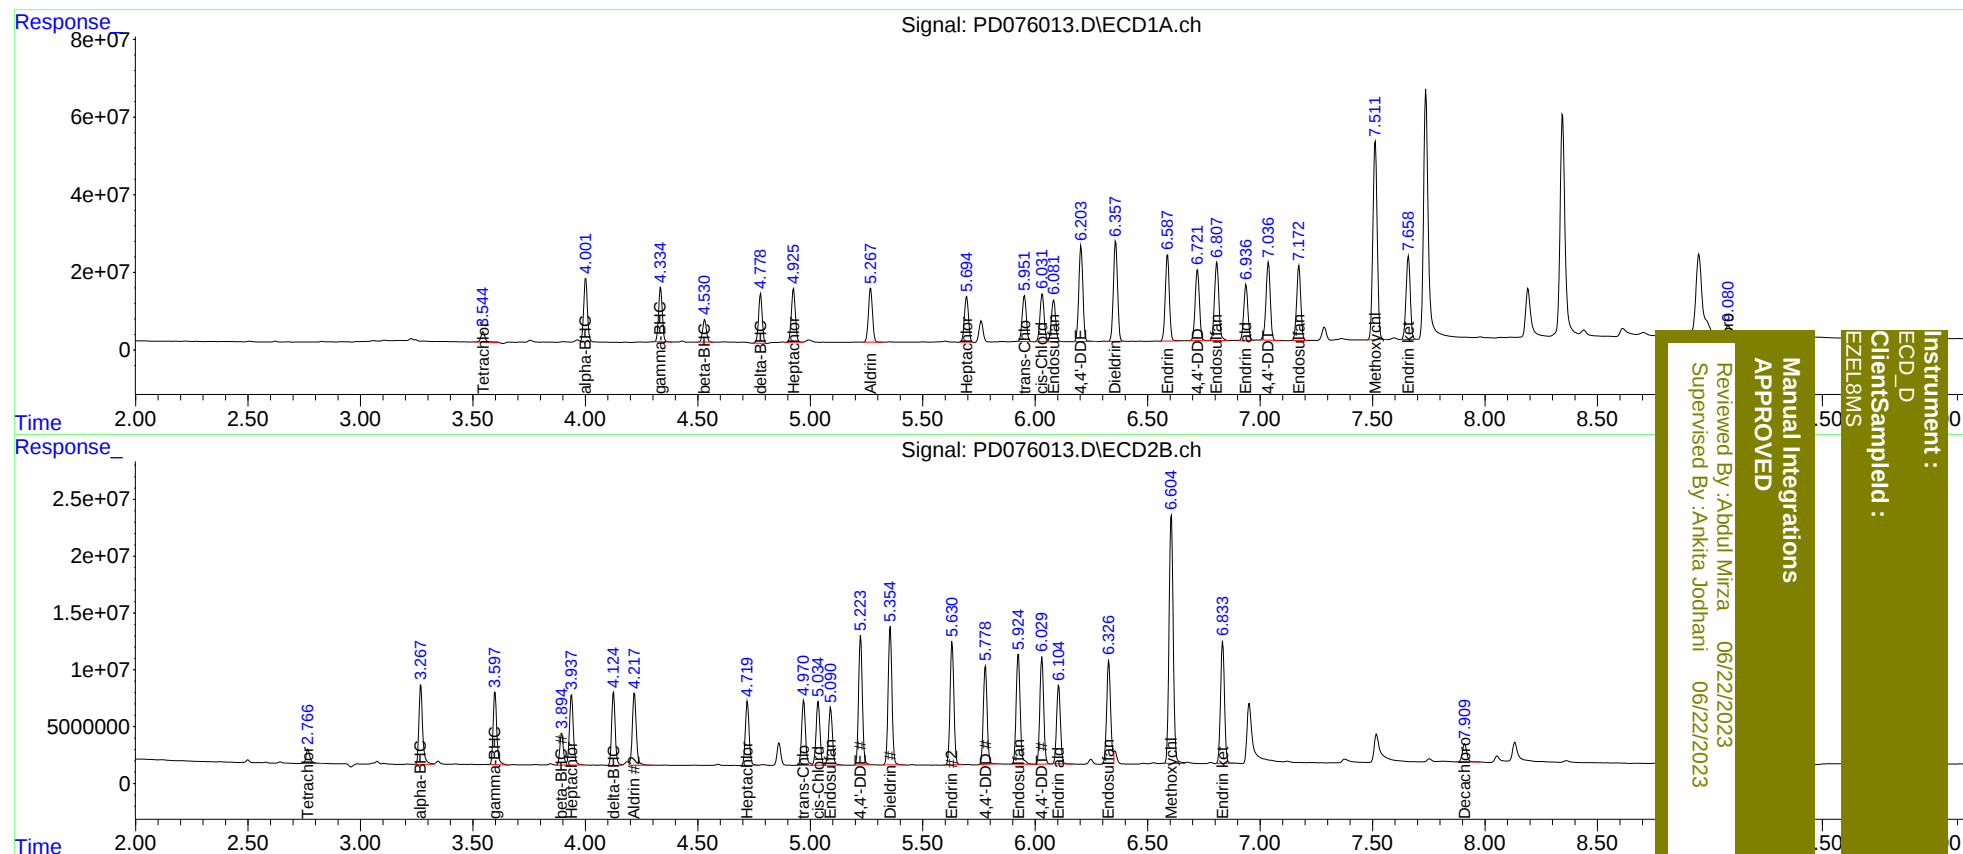

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/22/2023
Supervised By: Ankita Jodhani 06/22/2023

Instrument :
ECD_D
Client Sampled :
EZEL8MS