

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
 Data File : PD076017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 22:24
 Operator : AR\AJ
 Sample : 03101-08
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEM4

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/22/2023
 Supervised By : Ankita Jodhani 06/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 06:12:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.767	21087425	10320668	10.059m	9.645
2)	SA Decachlor...	9.083	7.910	34971630	16168083	14.549	15.432
Target Compounds							
10)	B trans-Chl...	5.951	4.972	4222904	2148676	1.446m	1.627
11)	B cis-Chlor...	6.034	5.035	6049399	1920978	1.996	1.399 #
12)	B 4,4'-DDE	6.204	5.224	2835690	1590763	1.018	1.381 #
16)	A 4,4'-DDD	6.721	5.779	3347678	2103330	1.552m	2.297 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD076017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 22:24
Operator : AR\AJ
Sample : 03101-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 06:12:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

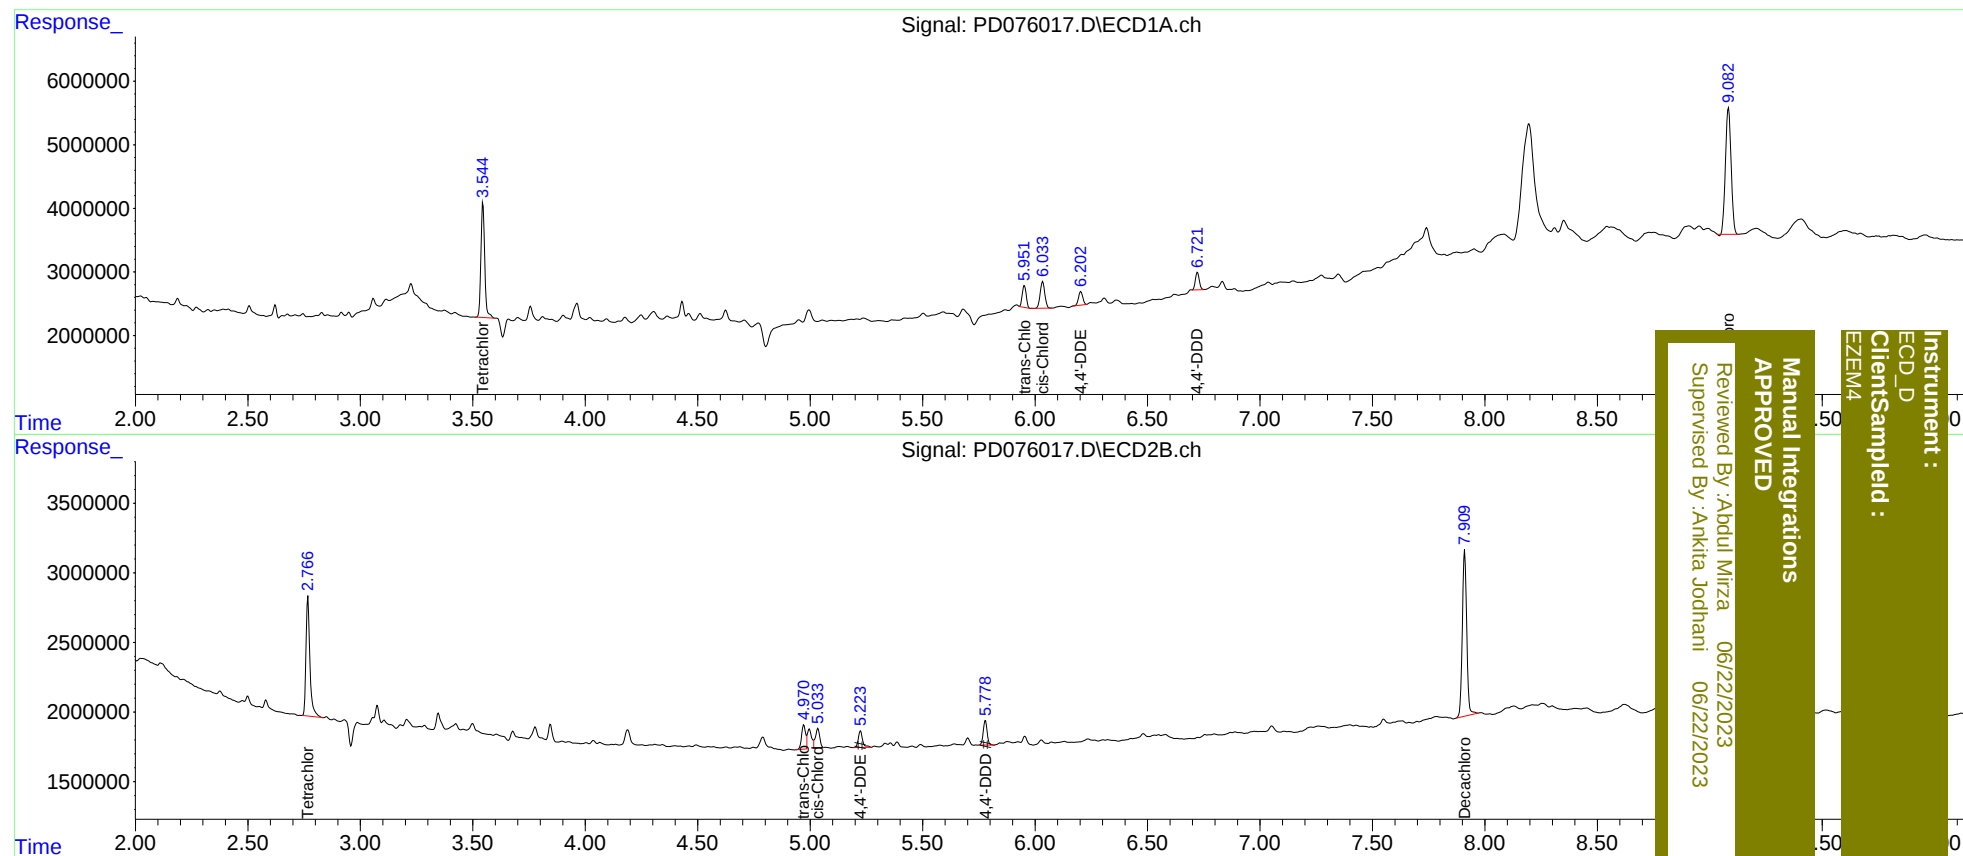

Instrument :
ECD_D
ClientSampled :
EZEM4
Manual Integrations
APPROVED
Reviewed By : Abdul Mirza 06/22/2023
Supervised By : Ankita Jodhani 06/22/2023