

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
 Data File : PD075973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 12:26
 Operator : AR\AJ
 Sample : RESC358
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC011

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:24:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.766	42496455	22210775	20.271	20.756
2)	SA Decachlor...	9.083	7.910	94738816	43135979	39.414	41.171
Target Compounds							
2)	A alpha-BHC	4.001	3.269	33191761	15344368	9.627	9.942
3)	MA gamma-BHC...	4.335	3.598	31491992	14699421	9.749	10.108
4)	MA Heptachlor	4.926	3.938	32983858	14974184	9.790	10.088
5)	MB Aldrin	5.269	4.219	32126238	14867234	9.894	10.281
6)	B beta-BHC	4.531	3.895	14899786	6793432	10.255	9.953
7)	B delta-BHC	4.779	4.125	28087807	14189997	9.511	9.746
8)	B Heptachlo...	5.696	4.721	29329491	13574588	9.979	10.024
9)	A Endosulfan I	6.083	5.091	27659702	12374368	10.031	10.056
10)	B trans-Chl...	5.952	4.972	28190017	13187584	9.653	9.989
11)	B cis-Chlor...	6.032	5.035	29388294	13592368	9.697	9.899
12)	B 4,4'-DDE	6.204	5.224	52124964	22489266	18.718	19.517
13)	MA Dieldrin	6.358	5.356	59301931	27782600	19.248	19.929
14)	MA Endrin	6.589	5.632	53092608	24828999	20.362	20.082
15)	B Endosulfa...	6.808	5.925	49142704	23424834	19.194	19.865
16)	A 4,4'-DDD	6.722	5.780	41157057	18293982	19.078	19.981
17)	MA 4,4'-DDT	7.037	6.030	40643304	17288322	18.551	18.657
18)	B Endrin al...	6.938	6.105	36198286	17421960	18.915	20.139
19)	B Endosulfa...	7.173	6.328	46847917	22065120	19.425	20.094
20)	A Methoxychlor	7.513	6.606	131.1E6	55336986	99.279	102.678
21)	B Endrin ke...	7.659	6.834	53309118	26208812	19.713	20.944

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD075973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 12:26
Operator : AR\AJ
Sample : RESC358
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:24:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

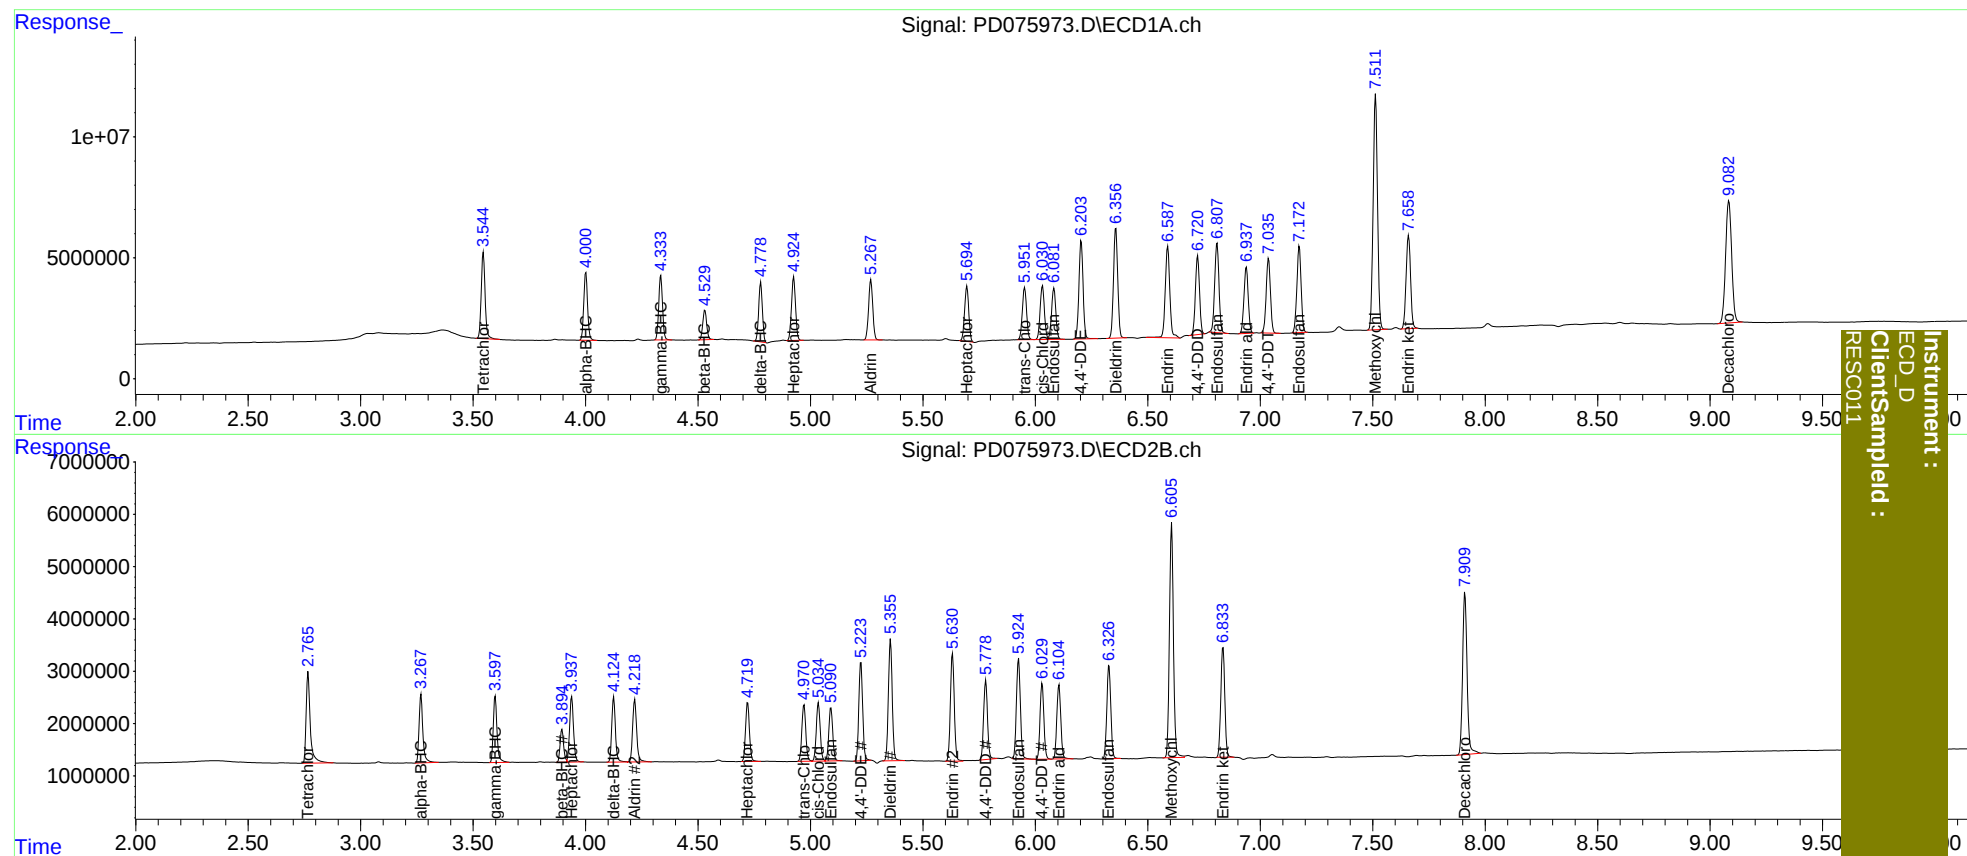

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD075973.D
Acq On : 21 Jun 2023 12:26
Operator : AR\AJ
Sample : RESC358
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC011

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Title : GC Extractables
Last Update : Wed Jun 21 16:21:29 2023
Integrator: ChemStation

RT#1	RT#2	Resolution
3.545	4.001	100.00%
4.001	4.335	100.00%
4.335	4.531	100.00%
4.531	4.779	100.00%
4.779	4.926	100.00%
4.926	5.269	100.00%
5.269	5.696	100.00%
5.696	5.952	100.00%
5.952	6.032	100.00%
6.032	6.083	97.87%
6.083	6.204	100.00%
6.204	6.358	100.00%
6.358	6.589	100.00%
6.589	6.722	100.00%
6.722	6.808	100.00%
6.808	6.938	100.00%
6.938	7.037	100.00%
7.037	7.173	100.00%
7.173	7.513	100.00%
7.513	7.659	100.00%
7.659	9.083	100.00%

Signal #2


2.766	3.269	100.00%
3.269	3.598	100.00%
3.598	3.895	100.00%
3.895	3.939	93.65%
3.939	4.125	100.00%
4.125	4.219	100.00%
4.219	4.721	100.00%
4.721	4.972	100.00%
4.972	5.035	99.40%
5.035	5.091	97.83%
5.091	5.224	100.00%
5.224	5.356	100.00%
5.356	5.632	100.00%
5.632	5.780	100.00%
5.780	5.925	100.00%
5.925	6.030	100.00%
6.030	6.105	100.00%
6.105	6.328	100.00%
6.328	6.606	100.00%
6.606	6.834	100.00%
6.834	7.910	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD075973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 12:26
Operator : AR\AJ
Sample : RESC358
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC011

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:24:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

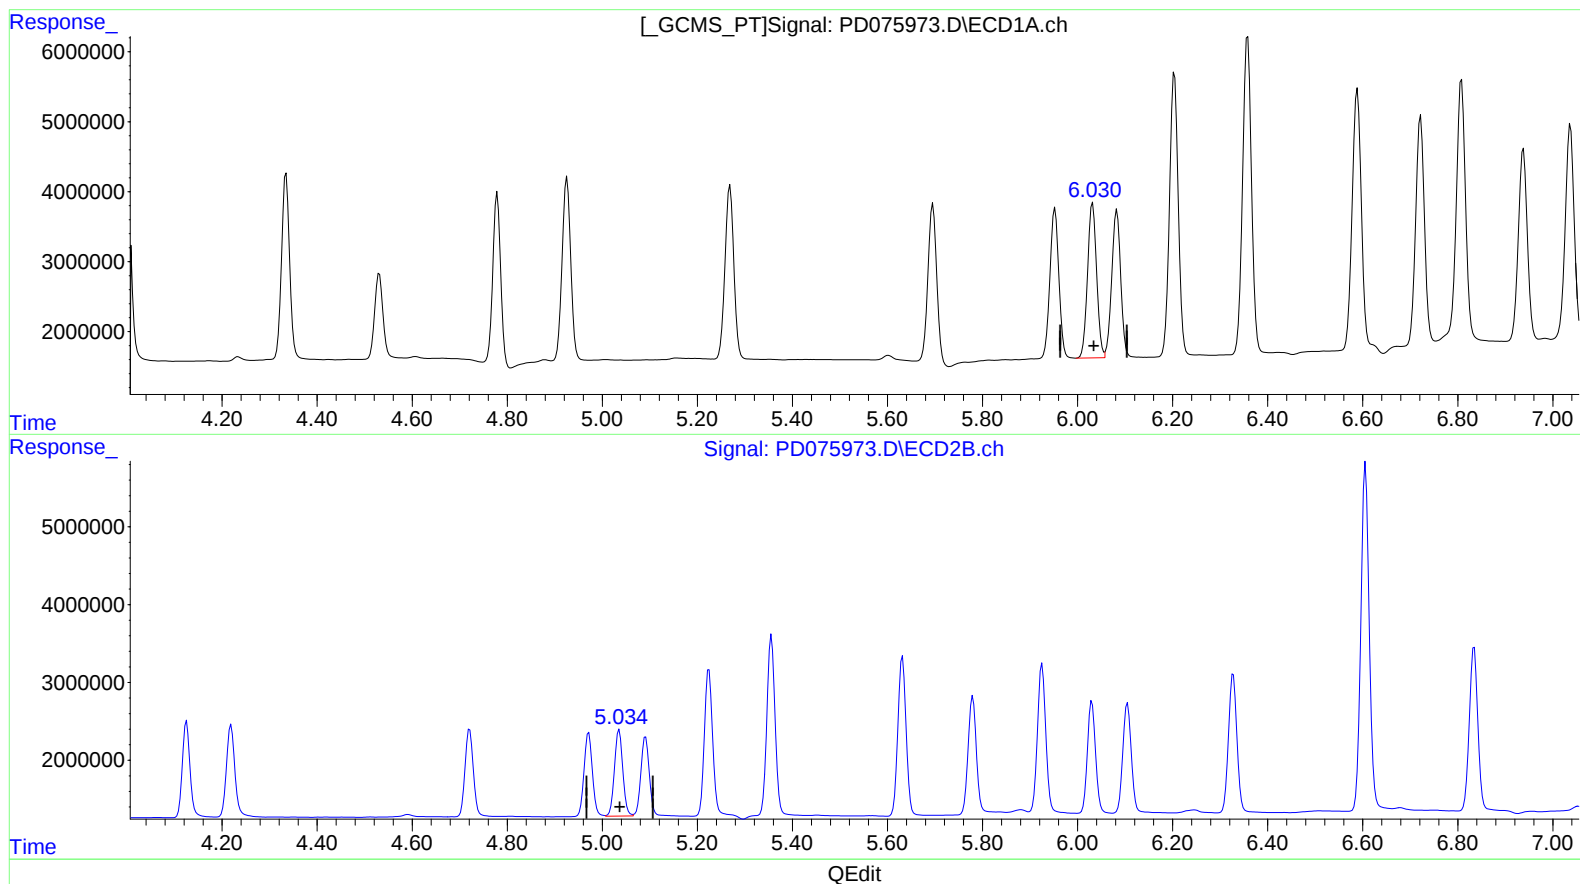

(11) cis-Chlordane (B)

6.032min 9.697 ng/ml

response 29388294

(11) cis-Chlordane #2 (B)

5.035min 9.899 ng/ml


response 13592368

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD075973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 12:26
Operator : AR\AJ
Sample : RESC358
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC011

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:24:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

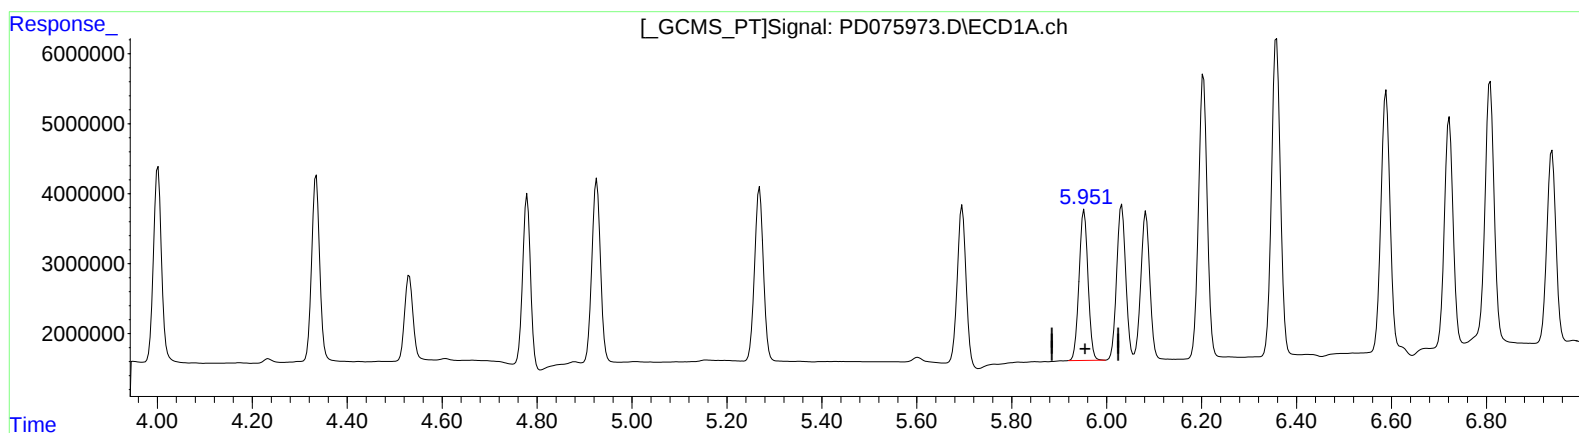

(10) trans-Chlordane (B)

5.952min 9.653 ng/ml

response 28190017

(10) trans-Chlordane #2 (B)

4.972min 9.989 ng/ml



response 13187584

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD075973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 12:26
Operator : AR\AJ
Sample : RESC358
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC011

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:24:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

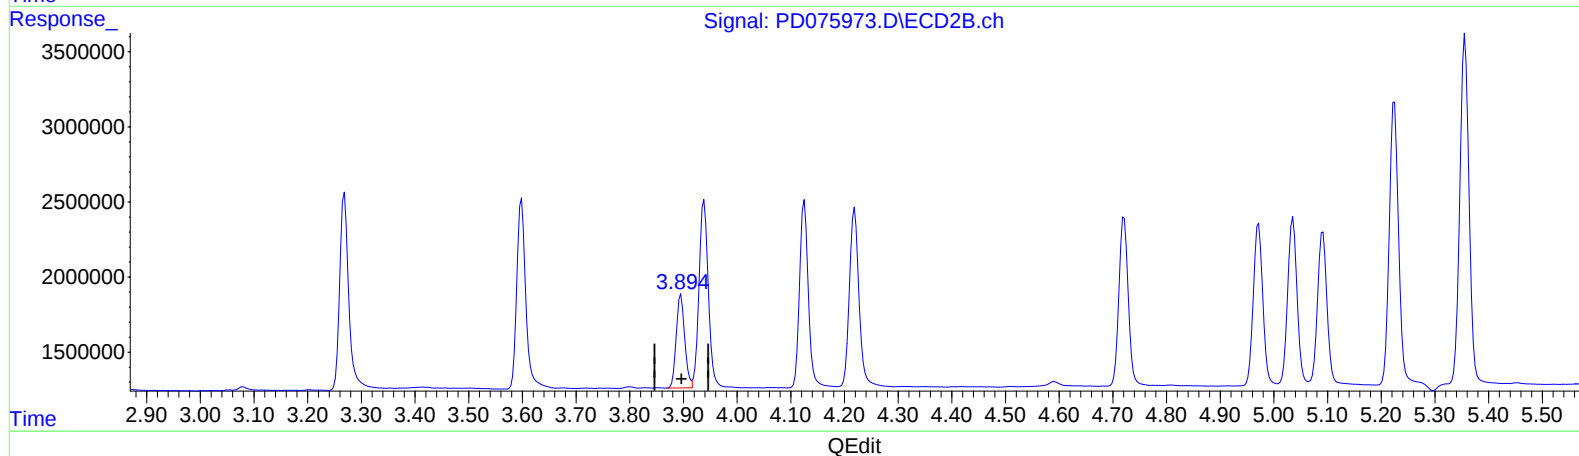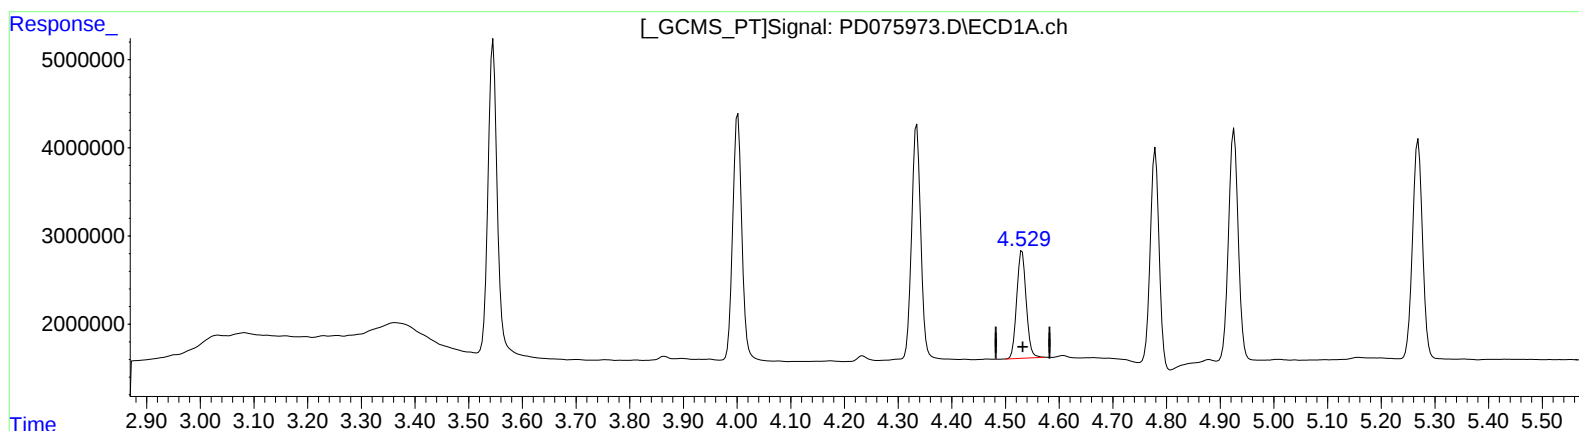

(6) beta-BHC (B)

4.531min 10.255 ng/ml

response 14899786

(6) beta-BHC #2 (B)

3.895min 9.953 ng/ml

response 6793432