

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
 Data File : PD076014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 21:44
 Operator : AR\AJ
 Sample : 03101-05MSD
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEL8MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/22/2023
 Supervised By :Ankita Jodhani 06/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:30:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.767	35495234	14688739	16.932	13.727
2)	SA Decachlor...	9.083	7.910	39567548	21632673	16.461	20.647 #
Target Compounds							
2)	A alpha-BHC	4.001	3.269	184.5E6	80690385	53.521m	52.281
3)	MA gamma-BHC...	4.335	3.599	161.8E6	72863838	50.086	50.105
4)	MA Heptachlor	4.926	3.939	171.0E6	74577837	50.743	50.243
5)	MB Aldrin	5.269	4.219	175.4E6	78286068	54.026	54.137
6)	B beta-BHC	4.531	3.895	67578992	30574537	46.513	44.795
7)	B delta-BHC	4.779	4.125	143.2E6	71073122	48.491	48.816
8)	B Heptachlo...	5.696	4.721	151.5E6	66418408	51.530	49.047
9)	A Endosulfan I	6.083	5.091	142.4E6	61257088	51.648	49.782
10)	B trans-Chl...	5.952	4.971	153.3E6	68666801	52.485	52.010
11)	B cis-Chlor...	6.032	5.035	160.4E6	69056127	52.927	50.294
12)	B 4,4'-DDE	6.204	5.225	320.5E6	134.2E6	115.090	116.500
13)	MA Dieldrin	6.358	5.356	336.0E6	145.9E6	109.052	104.638
14)	MA Endrin	6.588	5.632	285.4E6	129.6E6	109.466	104.839
15)	B Endosulfa...	6.808	5.925	278.9E6	122.2E6	108.942	103.625
16)	A 4,4'-DDD	6.722	5.779	246.2E6	103.6E6	114.138	113.125
17)	MA 4,4'-DDT	7.037	6.030	272.0E6	113.5E6	124.153	122.534
18)	B Endrin al...	6.938	6.105	188.5E6	82765453	98.480	95.674
19)	B Endosulfa...	7.173	6.327	250.9E6	123.4E6	104.051	112.416
20)	A Methoxychlor	7.513	6.606	706.0E6	284.8E6	534.576	528.468
21)	B Endrin ke...	7.659	6.834	288.7E6	129.4E6	106.762	103.440

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD076014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 21:44
Operator : AR\AJ
Sample : 03101-05MSD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:30:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

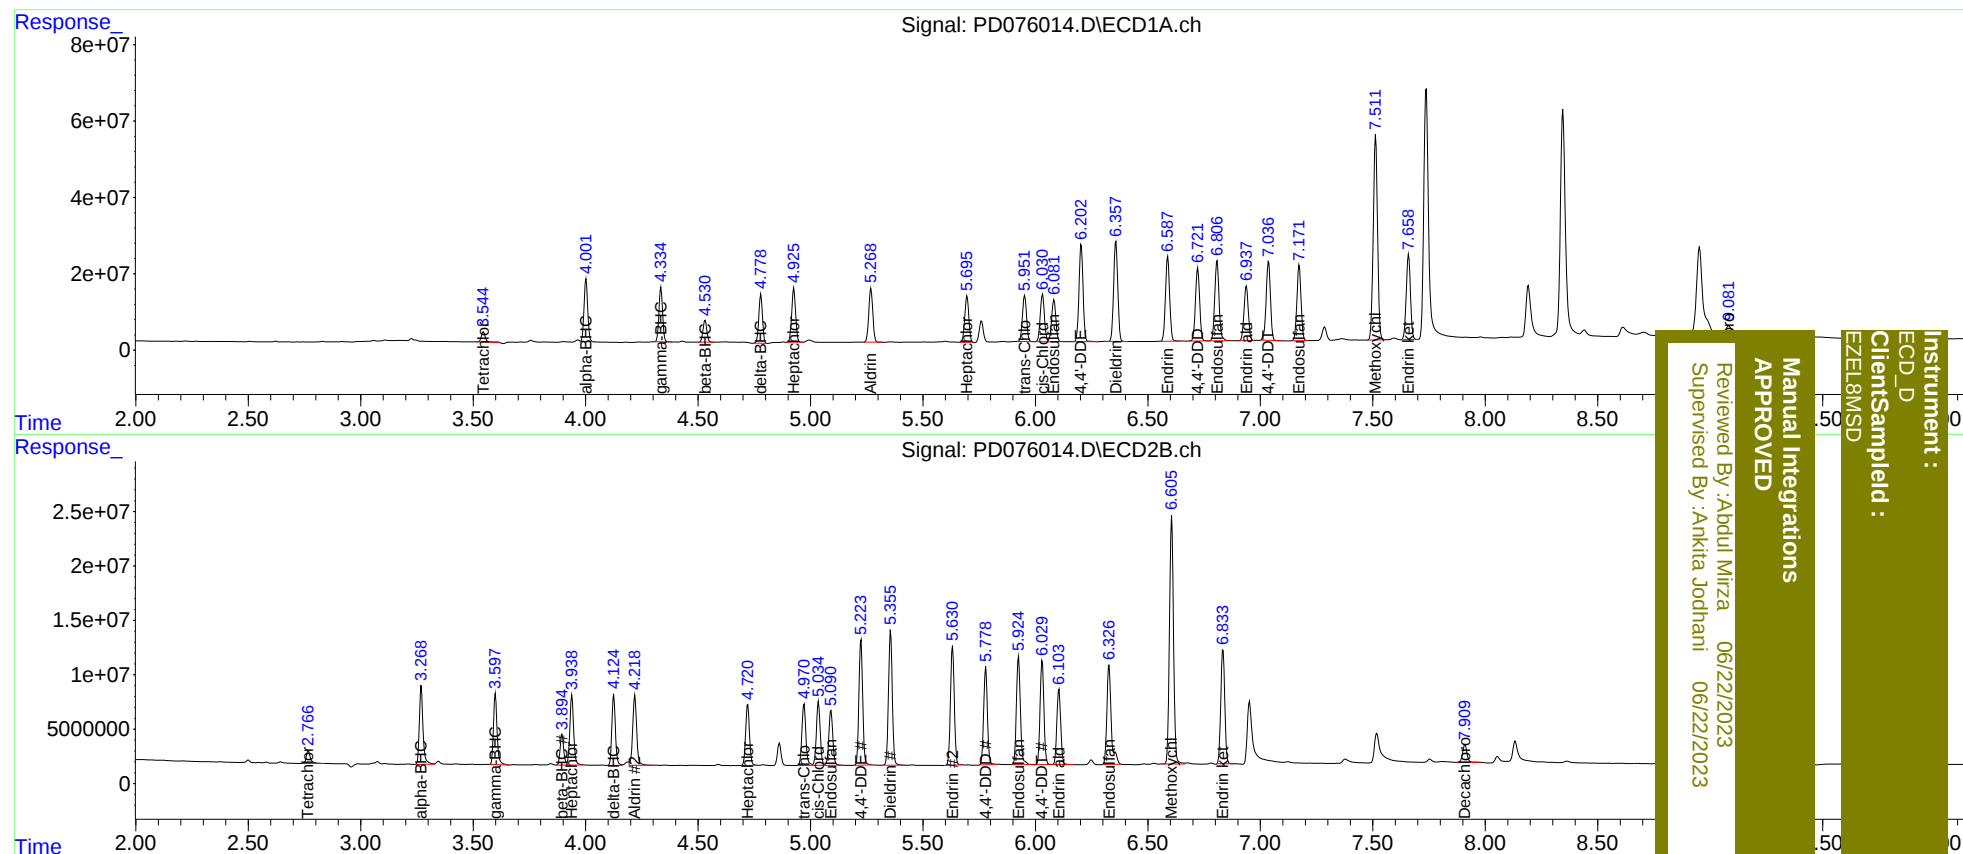

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/22/2023
Supervised By: Ankita Jodhani 06/22/2023

Instrument :
ECD_D
Client Sampled :
EZEL8MSD