

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 08:38
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 04:06:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	8.161	9.034	1055025	4047151	0.610	0.292 #
Target Compounds							
2)	A alpha-BHC	0.000	4.396f	0	19160144	N.D.	0.771
3)	MA gamma-BHC...	4.162	0.000	1581222	0	0.695	N.D. #
4)	MA Heptachlor	4.420f	0.000	3089396	0	1.415	N.D. #
6)	B beta-BHC	4.420	4.853f	3089396	22437180	3.182	2.301 #
7)	B delta-BHC	0.000	5.020	0	47804035	N.D.	2.040
8)	B Heptachlo...	0.000	5.847	0	13684532	N.D.	0.665
9)	A Endosulfan I	0.000	6.210	0	9783957	N.D.	0.494
11)	B cis-Chlor...	0.000	6.210f	0	9783957	N.D.	0.486
14)	MA Endrin	5.992	0.000	2113958	0	1.169	N.D. #
20)	A Methoxychlor	0.000	7.489f	0	6163138	N.D.	0.797


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 08:38
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 04:06:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

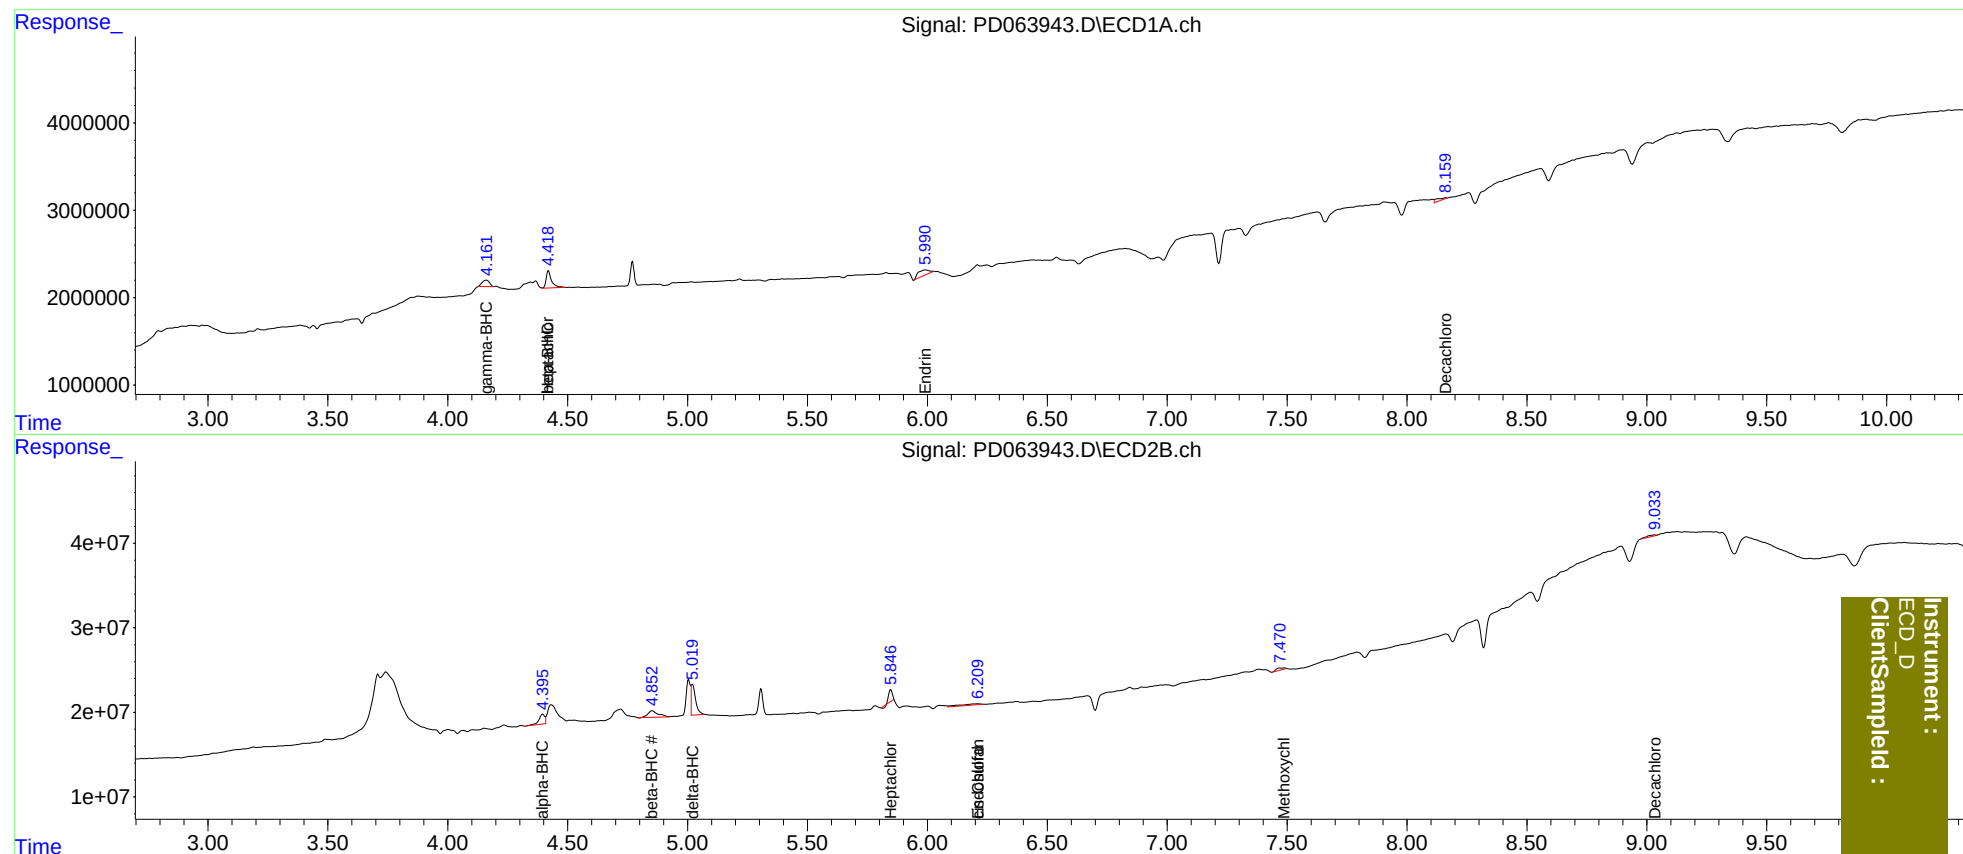


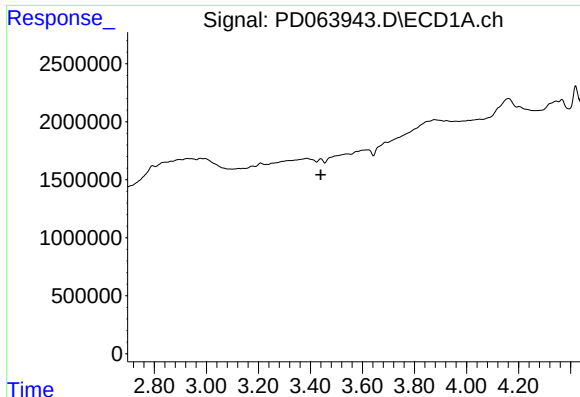

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

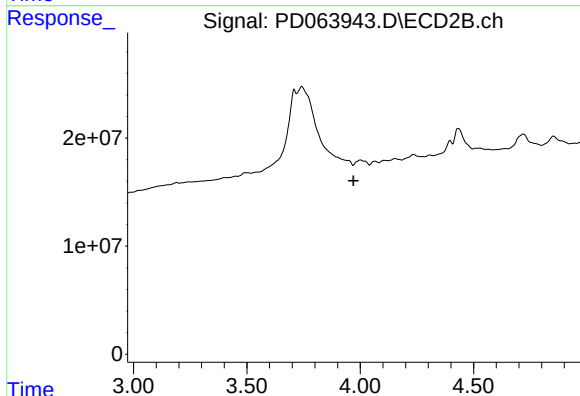


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.971 min
Response: 0
Conc: N.D.

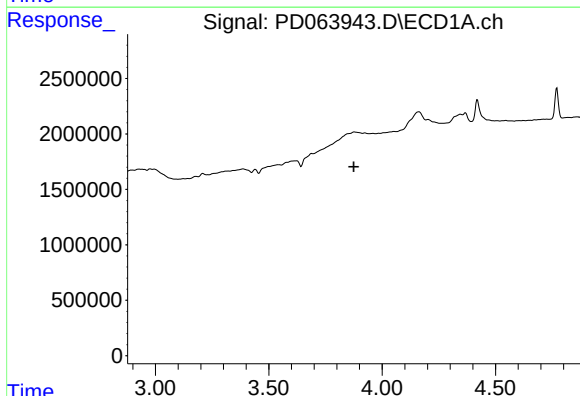


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.874 min
Response: 0
Conc: N.D.

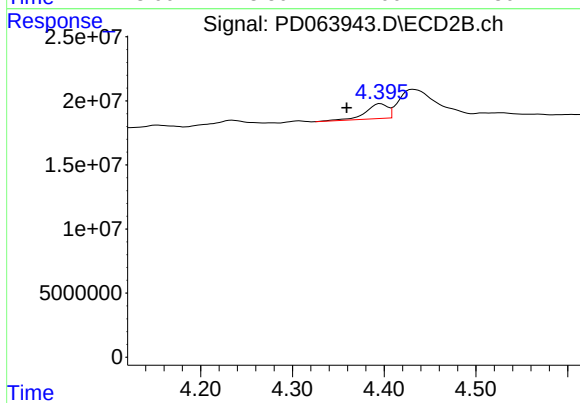

#2 alpha-BHC


R.T.: 4.396 min
Delta R.T.: 0.037 min
Response: 19160144
Conc: 0.77 ng/ml

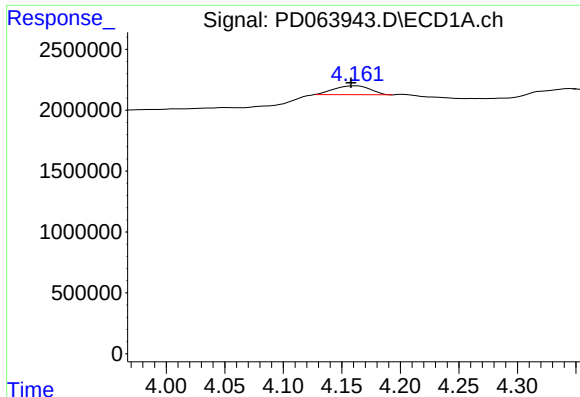

#3 gamma-BHC (Lindane)


R.T.: 4.162 min
Delta R.T.: 0.004 min
Response: 1581222
Conc: 0.69 ng/ml

Instrument :
ECD_D
ClientSampleId :

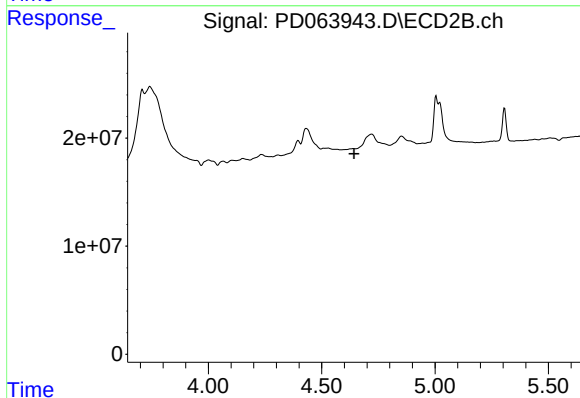


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.644 min
Response: 0
Conc: N.D.

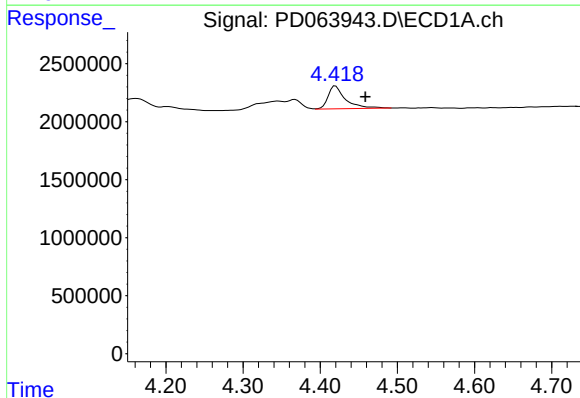


#4 Heptachlor

R.T.: 4.420 min
Delta R.T.: -0.039 min
Response: 3089396
Conc: 1.42 ng/ml

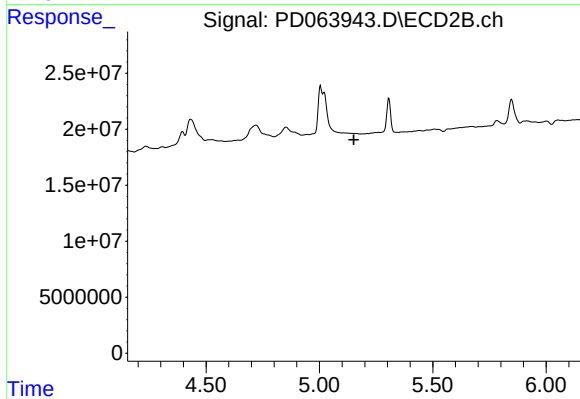

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.151 min
Response: 0
Conc: N.D.

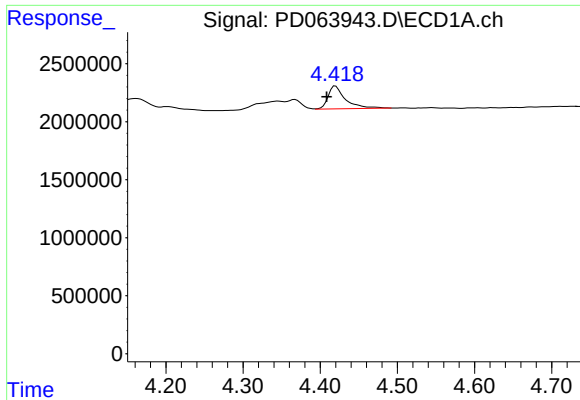

#6 beta-BHC


R.T.: 4.420 min
Delta R.T.: 0.011 min
Response: 3089396
Conc: 3.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

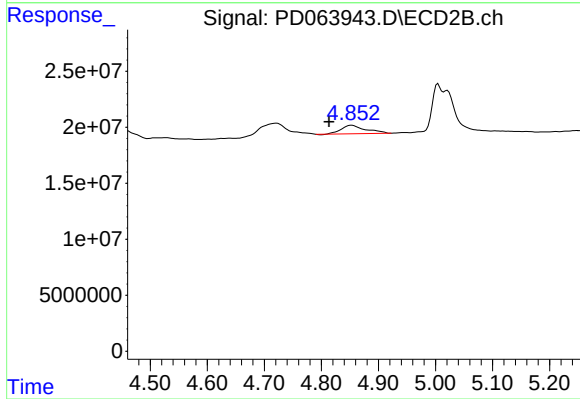


#6 beta-BHC

R.T.: 4.853 min
Delta R.T.: 0.039 min
Response: 22437180
Conc: 2.30 ng/ml

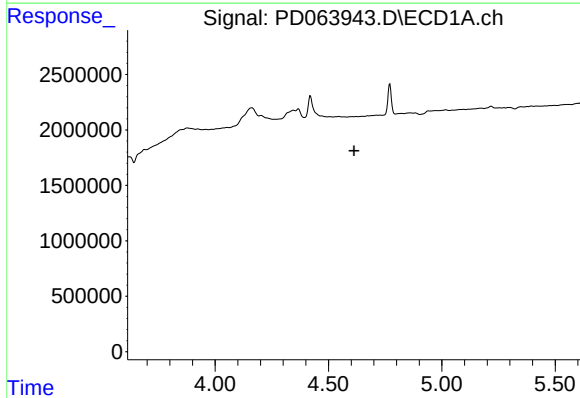


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

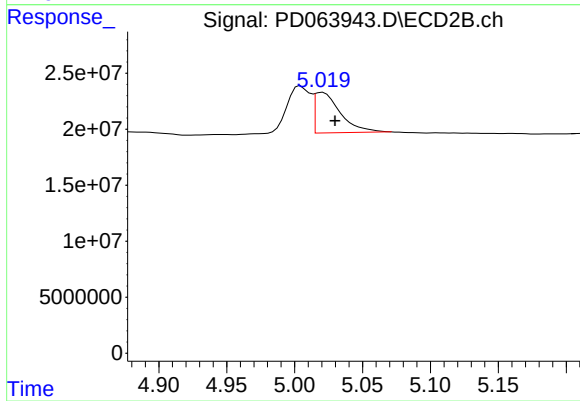

#7 delta-BHC


R.T.: 5.020 min
Delta R.T.: -0.009 min
Response: 47804035
Conc: 2.04 ng/ml

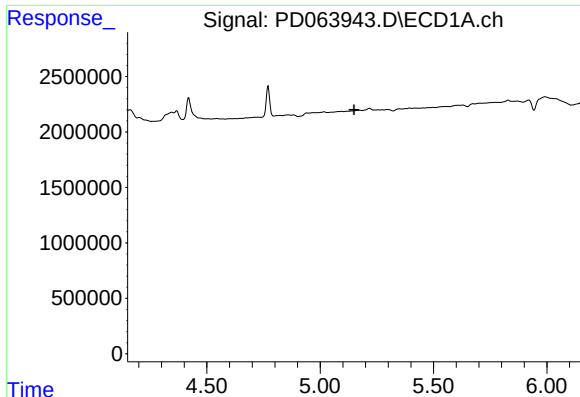

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

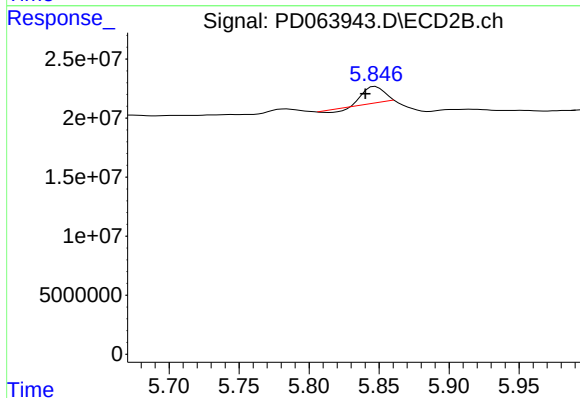


#8 Heptachlor epoxide

R.T.: 5.847 min
Delta R.T.: 0.007 min
Response: 13684532
Conc: 0.67 ng/ml

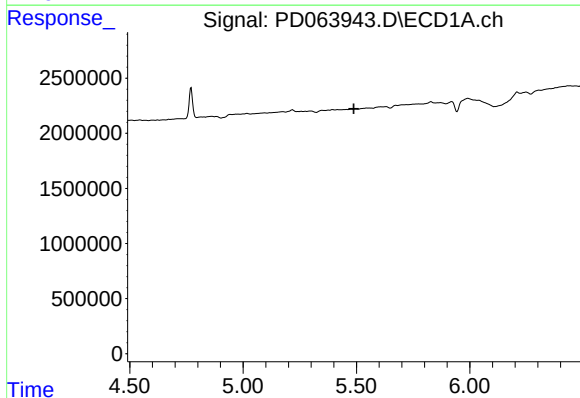


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.488 min
Response: 0
Conc: N.D.

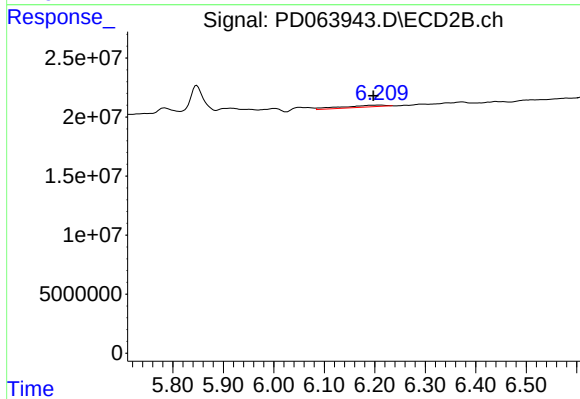

#9 Endosulfan I


R.T.: 6.210 min
Delta R.T.: 0.013 min
Response: 9783957
Conc: 0.49 ng/ml

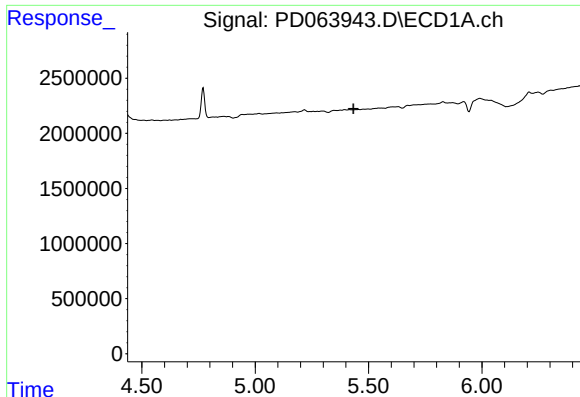

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

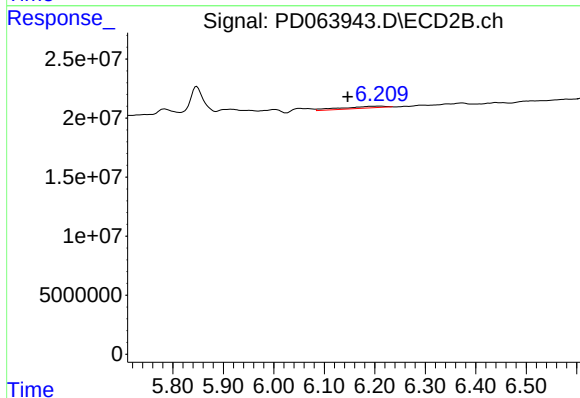


#11 cis-Chlordane

R.T.: 6.210 min
Delta R.T.: 0.064 min
Response: 9783957
Conc: 0.49 ng/ml

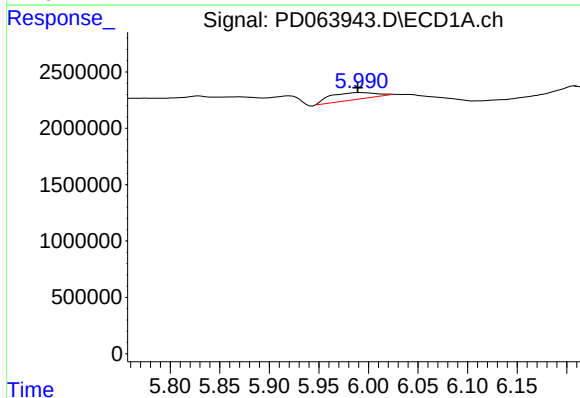


#14 Endrin

R.T.: 5.992 min
Delta R.T.: 0.002 min
Response: 2113958
Conc: 1.17 ng/ml

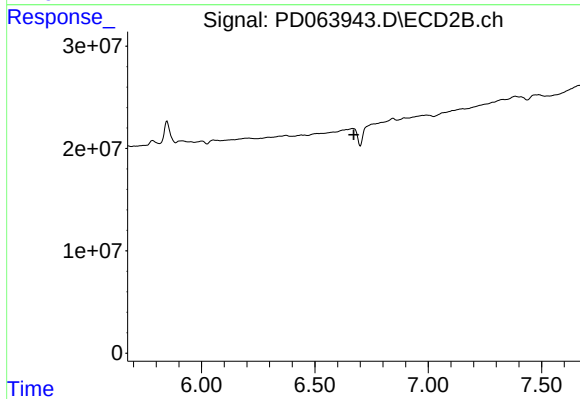

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.672 min
Response: 0
Conc: N.D.

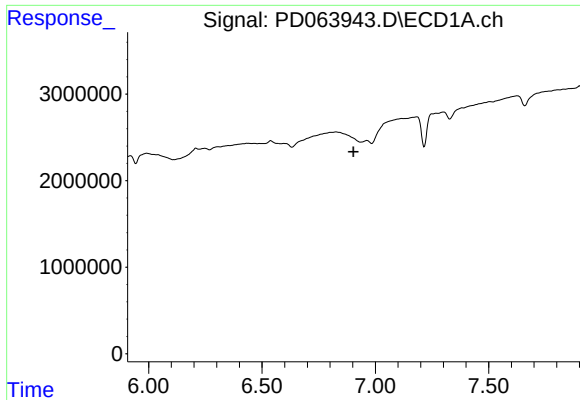

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

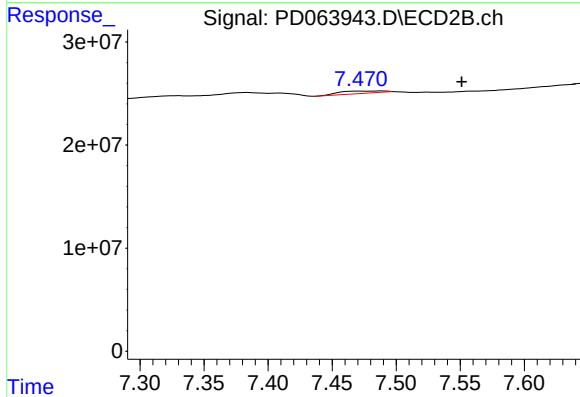


#20 Methoxychlor

R.T.: 7.489 min
Delta R.T.: -0.062 min
Response: 6163138
Conc: 0.80 ng/ml

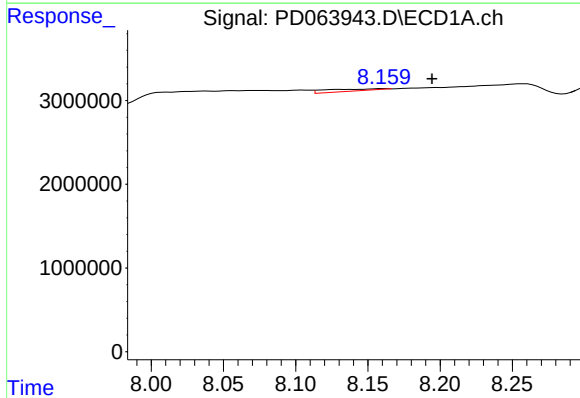

#27 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: -0.034 min
Response: 1055025
Conc: 0.61 ng/ml

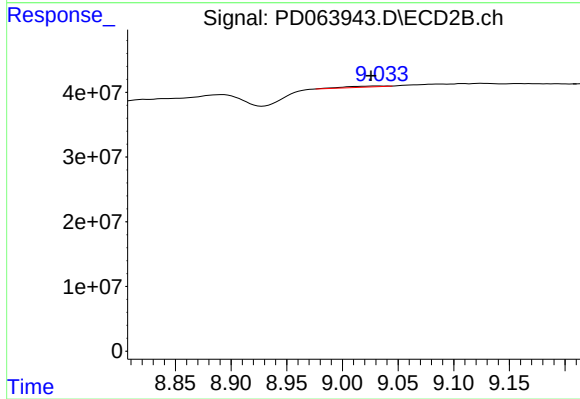

#27 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: 0.008 min
Response: 4047151
Conc: 0.29 ng/ml