

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 09:20
 Operator : AR\AJ
 Sample : PB137217BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 04:07:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.969	30770296	315.7E6	19.794	19.933
27)	SA Decachlor...	8.191	9.022	71795696	579.5E6	41.477	41.784
Target Compounds							
6)	B beta-BHC	4.372f	0.000	5943484	0	6.121	N.D. #
7)	B delta-BHC	0.000	5.005	0	102.5E6	N.D.	4.376
8)	B Heptachlo...	0.000	5.849	0	6640360	N.D.	0.323
15)	B Endosulfa...	0.000	6.897	0	5838878	N.D.	0.361
16)	A 4,4'-DDD	0.000	6.816	0	13522326	N.D.	0.803
19)	B Endosulfa...	0.000	7.226	0	6476905	N.D.	0.394
20)	A Methoxychlor	0.000	7.488f	0	5063494	N.D.	0.654
21)	B Endrin ke...	0.000	7.728	0	3183217	N.D.	0.201


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 09:20
Operator : AR\AJ
Sample : PB137217BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 04:07:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

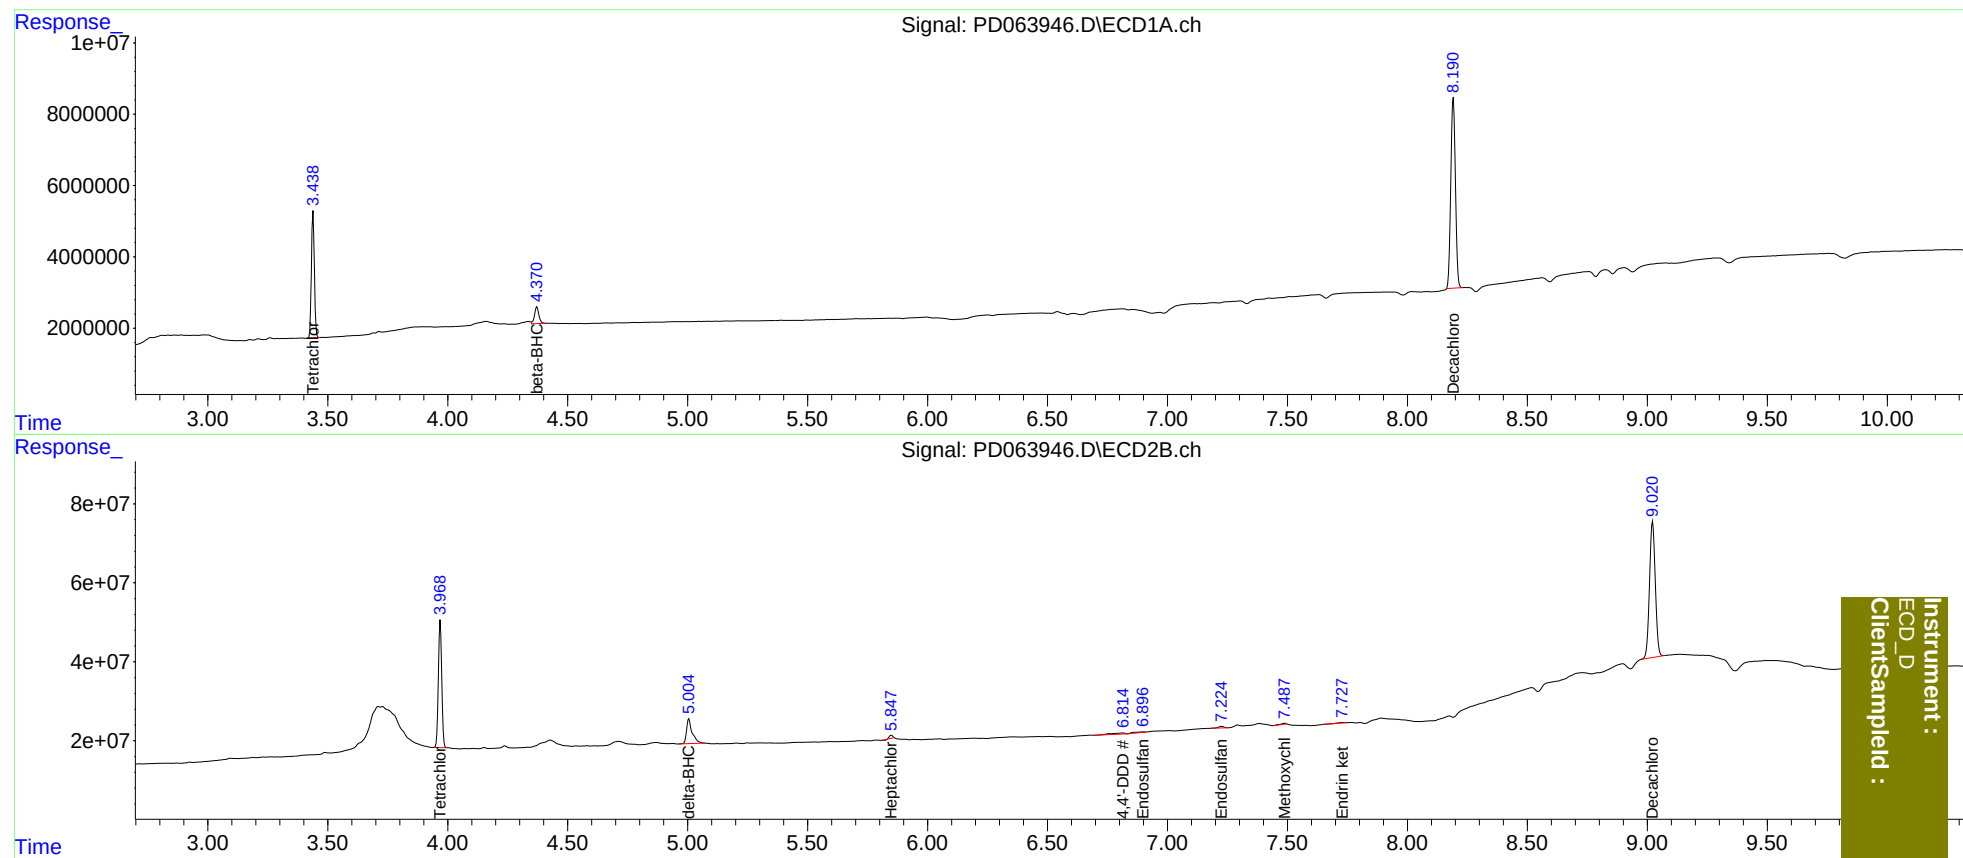


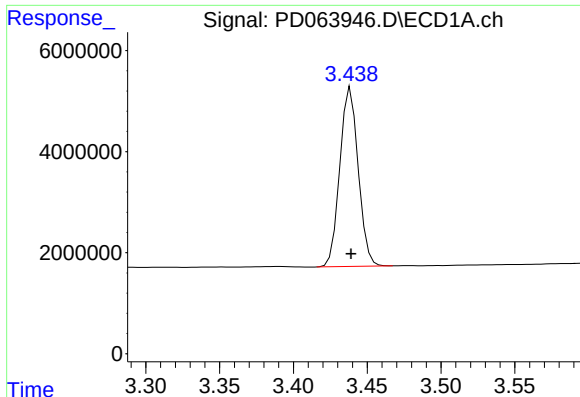

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 30770296
Conc: 19.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

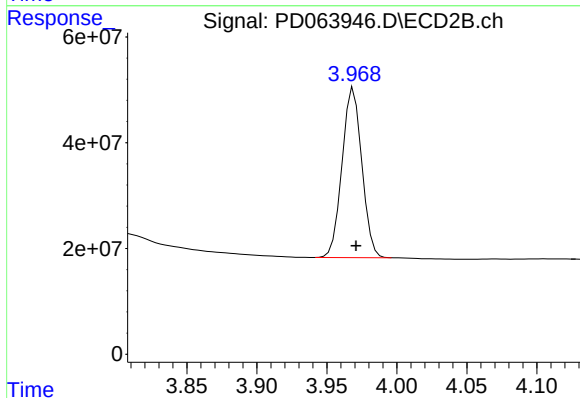


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.002 min
Response: 315698666
Conc: 19.93 ng/ml

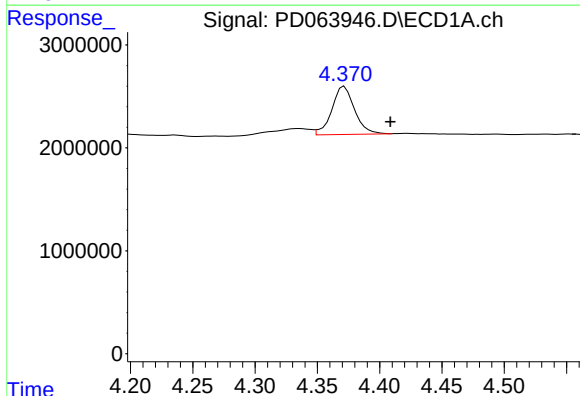


#6 beta-BHC

R.T.: 4.372 min
Delta R.T.: -0.037 min
Response: 5943484
Conc: 6.12 ng/ml

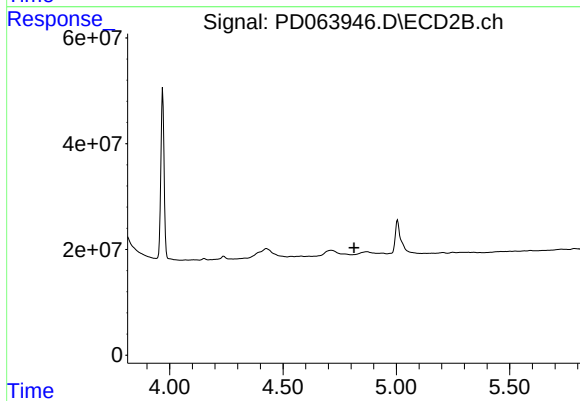

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.814 min
Response: 0
Conc: N.D.

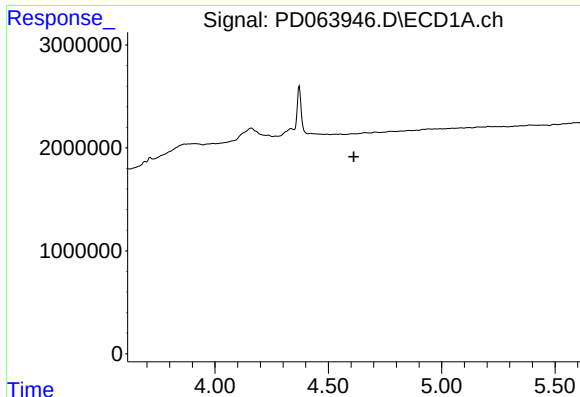

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

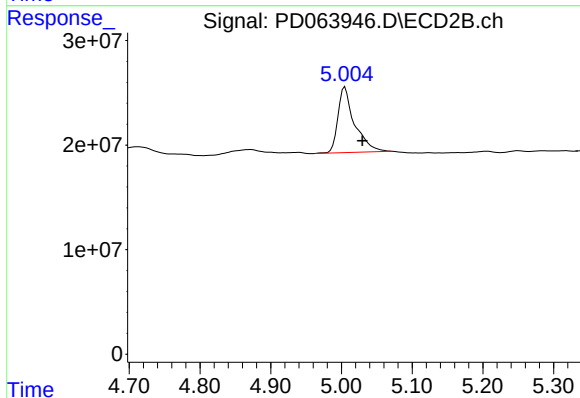


#7 delta-BHC

R.T.: 5.005 min
Delta R.T.: -0.025 min
Response: 102522706
Conc: 4.38 ng/ml

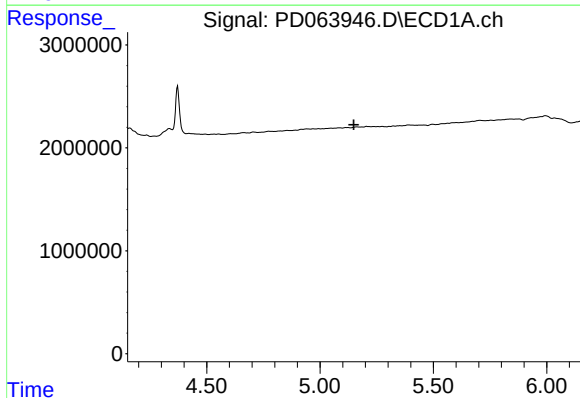


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

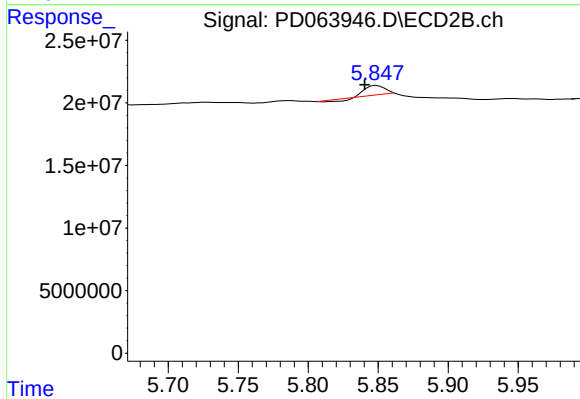

#8 Heptachlor epoxide


R.T.: 5.849 min
Delta R.T.: 0.009 min
Response: 6640360
Conc: 0.32 ng/ml

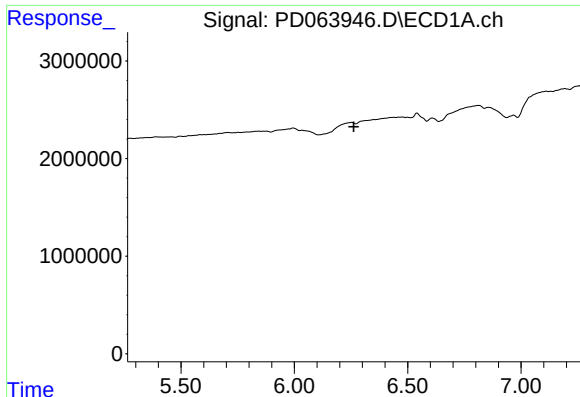

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

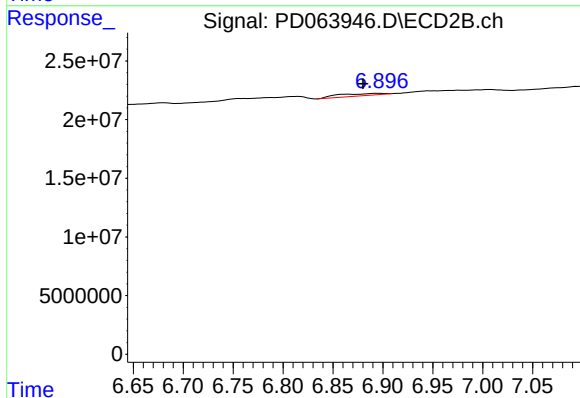


#15 Endosulfan II

R.T.: 6.897 min
Delta R.T.: 0.017 min
Response: 5838878
Conc: 0.36 ng/ml

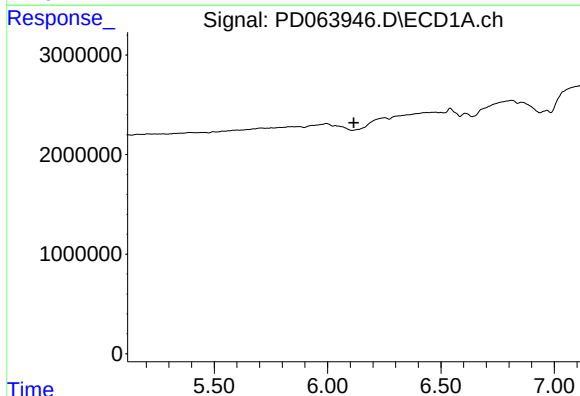


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.115 min
Response: 0
Conc: N.D.

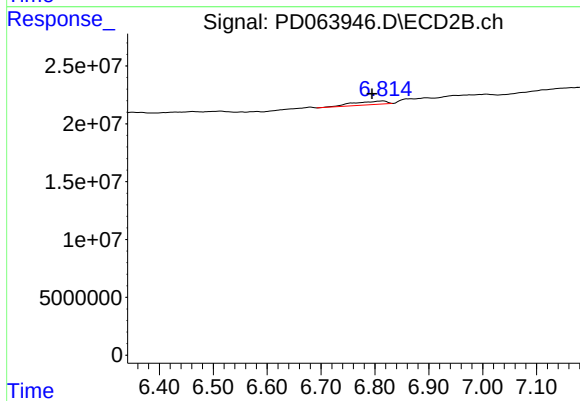

#16 4,4'-DDD


R.T.: 6.816 min
Delta R.T.: 0.021 min
Response: 13522326
Conc: 0.80 ng/ml

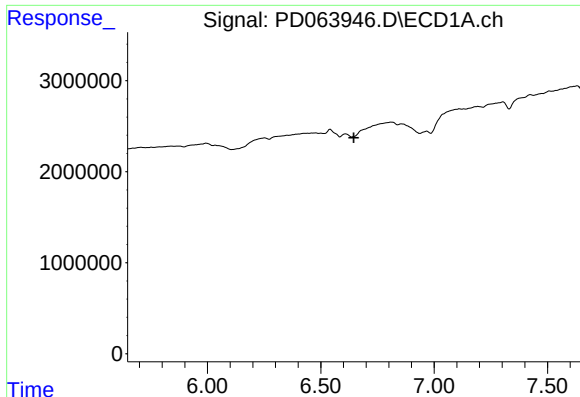

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

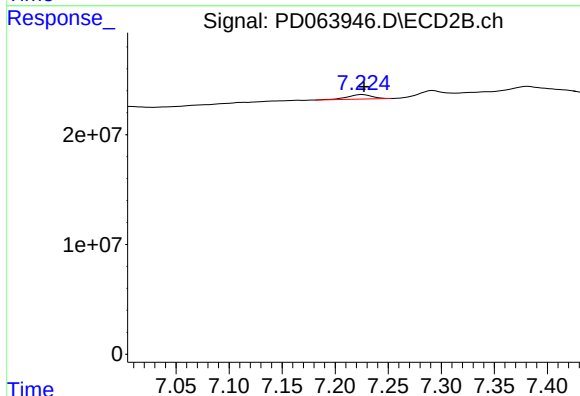


#19 Endosulfan Sulfate

R.T.: 7.226 min
Delta R.T.: -0.001 min
Response: 6476905
Conc: 0.39 ng/ml

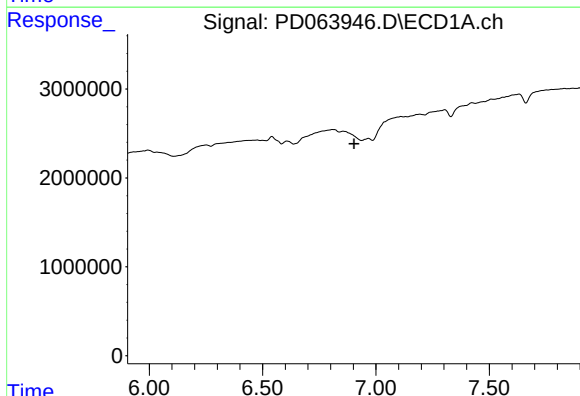


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.904 min
Response: 0
Conc: N.D.

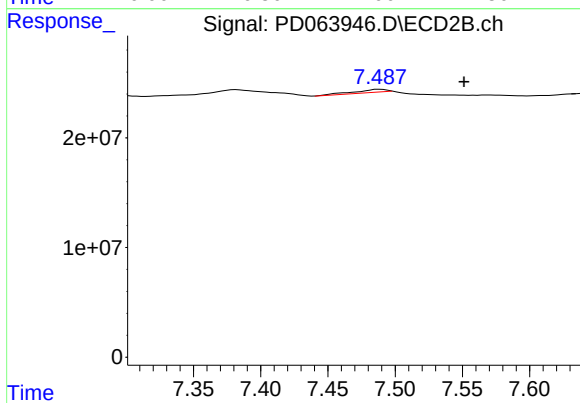

#20 Methoxychlor


R.T.: 7.488 min
Delta R.T.: -0.063 min
Response: 5063494
Conc: 0.65 ng/ml

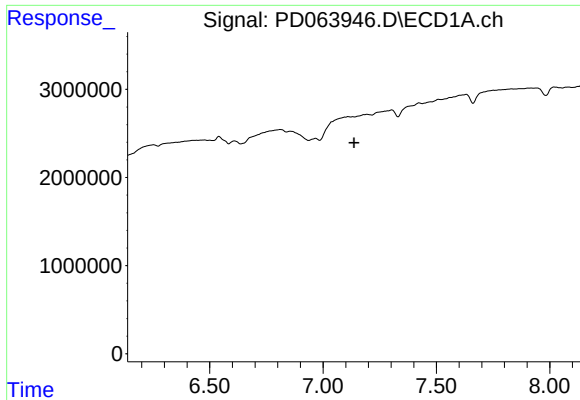

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.137 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

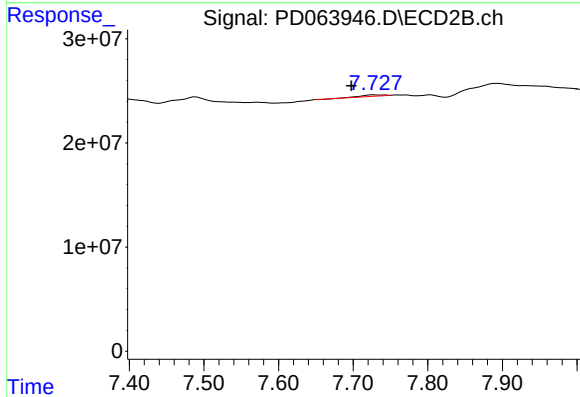


#21 Endrin ketone

R.T.: 7.728 min
Delta R.T.: 0.030 min
Response: 3183217
Conc: 0.20 ng/ml

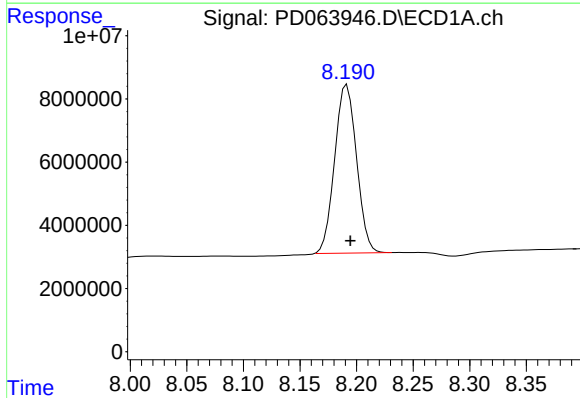

#27 Decachlorobiphenyl

R.T.: 8.191 min
Delta R.T.: -0.003 min
Response: 71795696
Conc: 41.48 ng/ml

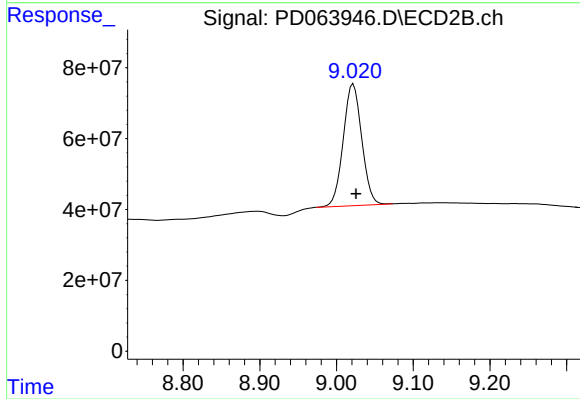

#27 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.004 min
Response: 579474096
Conc: 41.78 ng/ml