

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 09:34
 Operator : AR\AJ
 Sample : PB137217BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleID :
 PLCS217

Manual Integrations
 APPROVED

Ankita
 6/25/2021 8:51:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 04:54:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.969	30506784	306.8E6	19.625	19.371
27)	SA Decachlor...	8.191	9.022	70027431	558.4E6	40.456	40.263
Target Compounds							
2)	A alpha-BHC	3.873	4.357	10626715	124.5E6	4.543	5.013
3)	MA gamma-BHC...	4.156	4.642	11007123	113.0E6	4.837	4.951
4)	MA Heptachlor	4.457	5.148	10027058	117.5E6	4.593	5.043
5)	MB Aldrin	4.704	5.453	9665039	115.5E6	4.769	5.242
6)	B beta-BHC	4.408	4.813	5026759	48028258	5.177	4.924
7)	B delta-BHC	4.611	5.029	9905236	158.3E6	4.589	6.756 #
8)	B Heptachlo...	5.148	5.838	9410659	121.5E6	4.963	5.907m
9)	A Endosulfan I	5.486	6.195	8919258	96303250	4.874	4.861
10)	B trans-Chl...	5.374	6.073	9422532	105.5E6	4.845	5.014
11)	B cis-Chlor...	5.432	6.145	9575066	100.1E6	5.040	4.972
12)	B 4,4'-DDE	5.596	6.302	18751522	201.6E6	9.497	9.977
13)	MA Dieldrin	5.729	6.450	18773360	209.2E6	8.971	9.999m
14)	MA Endrin	5.987	6.669	15748970	159.4E6	8.708	9.111
15)	B Endosulfa...	6.260	6.878	15052706	174.8E6	9.212	10.805
16)	A 4,4'-DDD	6.112	6.790	15197500	178.5E6	9.205	10.602m
17)	MA 4,4'-DDT	6.353	7.090	13133665	144.0E6	7.804	8.745
18)	B Endrin al...	6.427	7.002	14800463	152.5E6	10.367m	10.839
19)	B Endosulfa...	6.643	7.226	11790805	165.5E6	7.595	10.055 #
20)	A Methoxychlor	6.900	7.549	41935398	366.6E6	45.486	47.379
21)	B Endrin ke...	7.133	7.694	20017973	170.5E6	10.552m	10.746m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 09:34
Operator : AR\AJ
Sample : PB137217BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 04:54:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

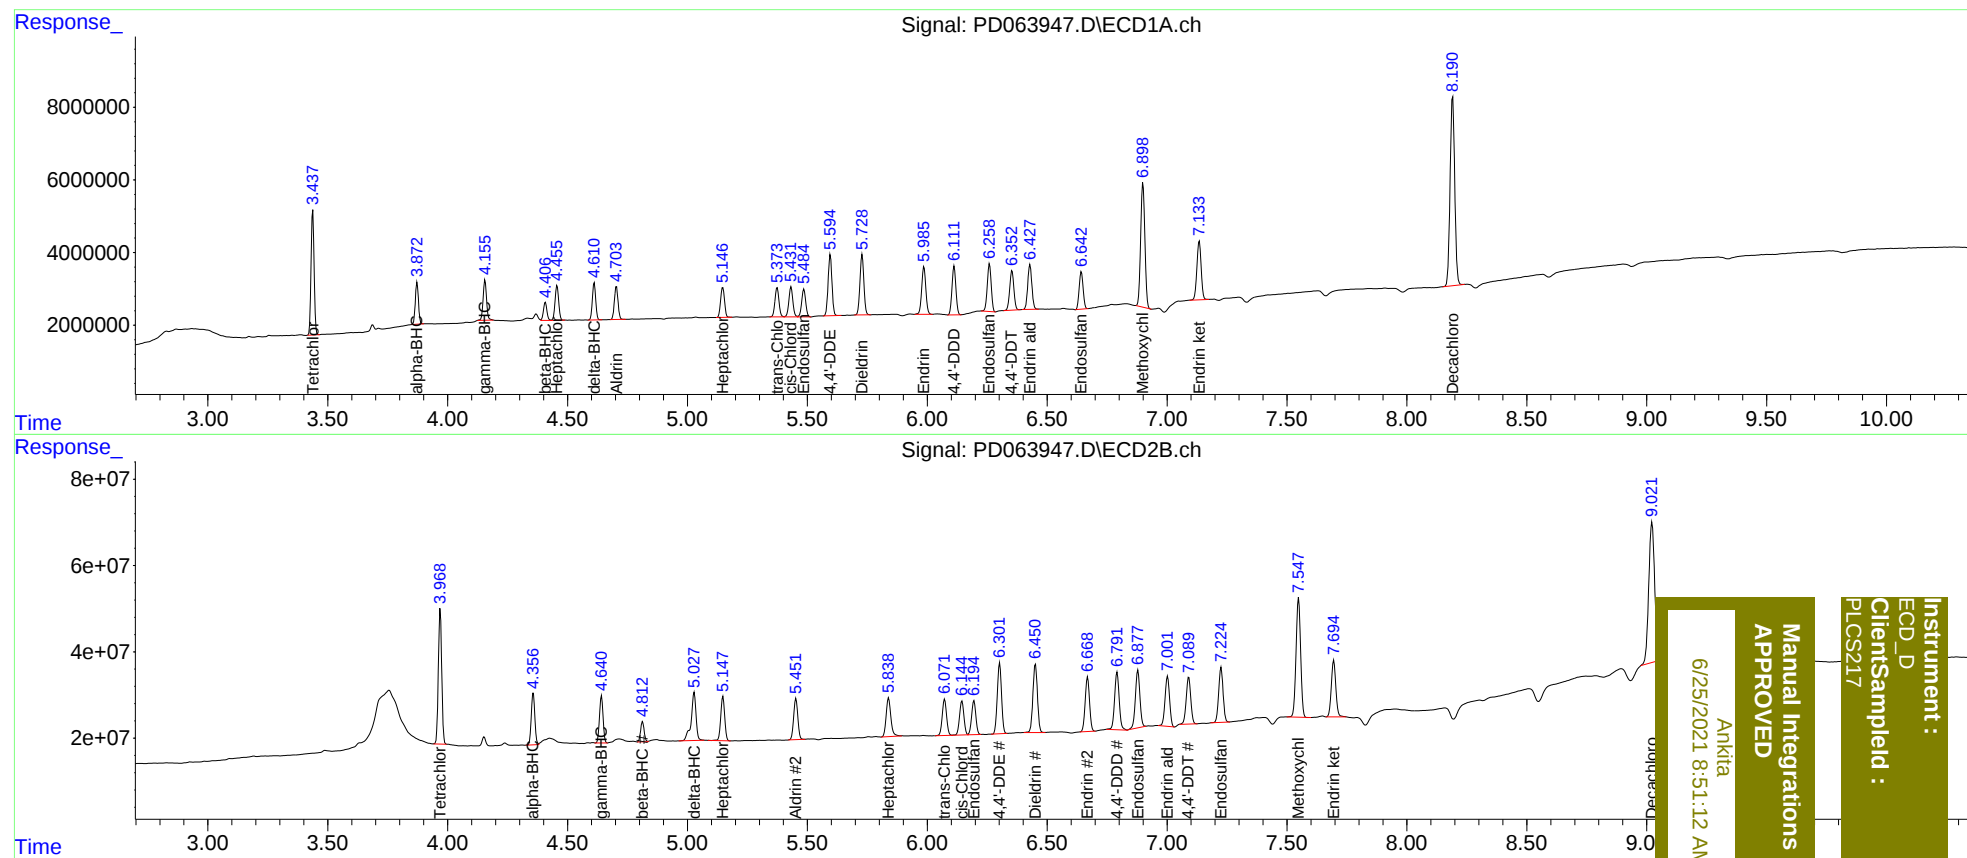

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:12 AM

Instrument :
ECD_D
ClientSampled :
PLCS217