

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 11:42
 Operator : AR\AJ
 Sample : M2682-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGDM4

Manual Integrations
 APPROVED

Ankita
 6/25/2021 8:51:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 04:09:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.436	3.969	15666584	137.2E6	10.078	8.660
2)	SA Decachlor...	8.184	9.020	51856738	379.4E6	29.958m	27.360m
Target Compounds							
3)	MA gamma-BHC...	4.160	4.621	37567583	183.8E6	16.507	8.053m#
12)	B 4,4'-DDE	5.616	6.291	8577246	55834632	4.344m	2.763m#
15)	B Endosulfa...	6.260	6.865	10236795	62196426	6.264	3.844m#
16)	A 4,4'-DDD	6.112	6.787	3239305	143.0E6	1.962m	8.496 #
19)	B Endosulfa...	6.657	7.223	13473757	50533254	8.679	3.070m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 11:42
Operator : AR\AJ
Sample : M2682-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 04:09:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

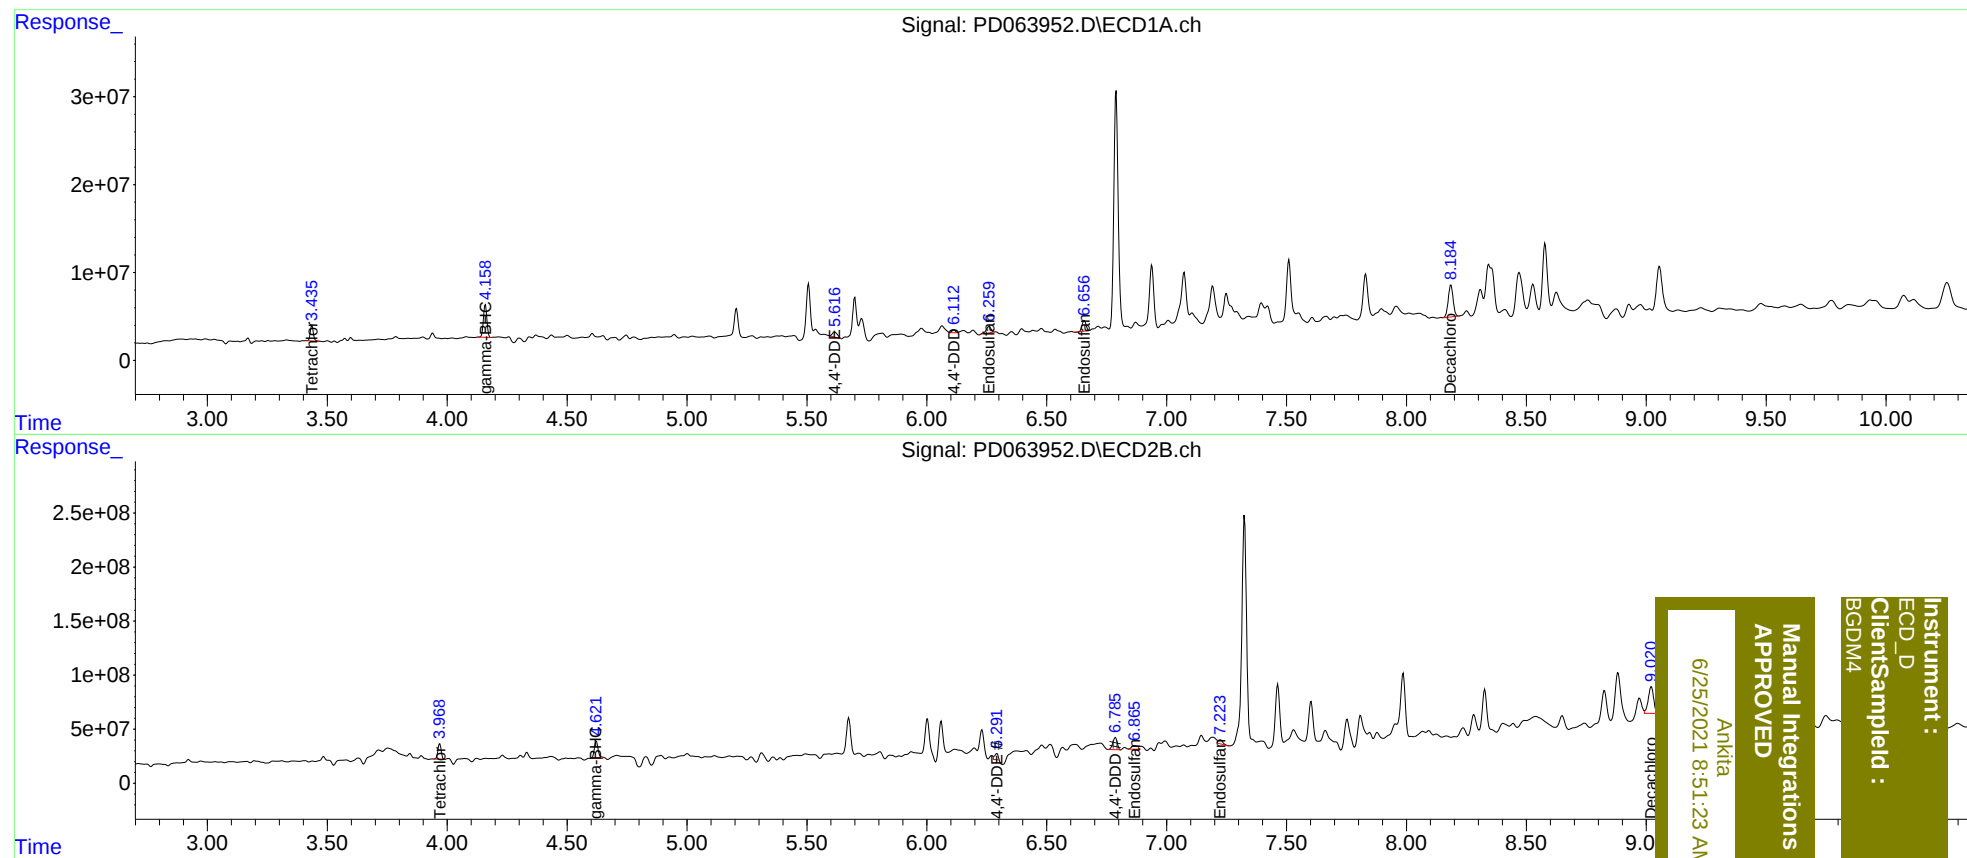

Manual Integrations
APPROVED

6/25/2021 8:51:23 AM

Ankita

Instrument :
ECD_D
Client Sample :
BGDM4