

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063967.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 18:52
 Operator : AR\AJ
 Sample : M2682-09
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGDA0

Manual Integrations
 APPROVED

Ankita
 6/25/2021 8:51:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 04:14:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.437	3.970	24165818	234.8E6	15.546	14.827
27) SA Decachlor...	8.187	9.020	32817576	273.2E6	18.959m	19.698m
Target Compounds						
10) B trans-Chl...	5.386	6.060	1490963	42149395	0.767m	2.004m#
15) B Endosulfa...	6.258	6.861	1403219	85666582	0.859m	5.294m#
17) MA 4,4'-DDT	6.351	7.102	824543	22909095	0.490m	1.392 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063967.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:52
Operator : AR\AJ
Sample : M2682-09
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 04:14:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

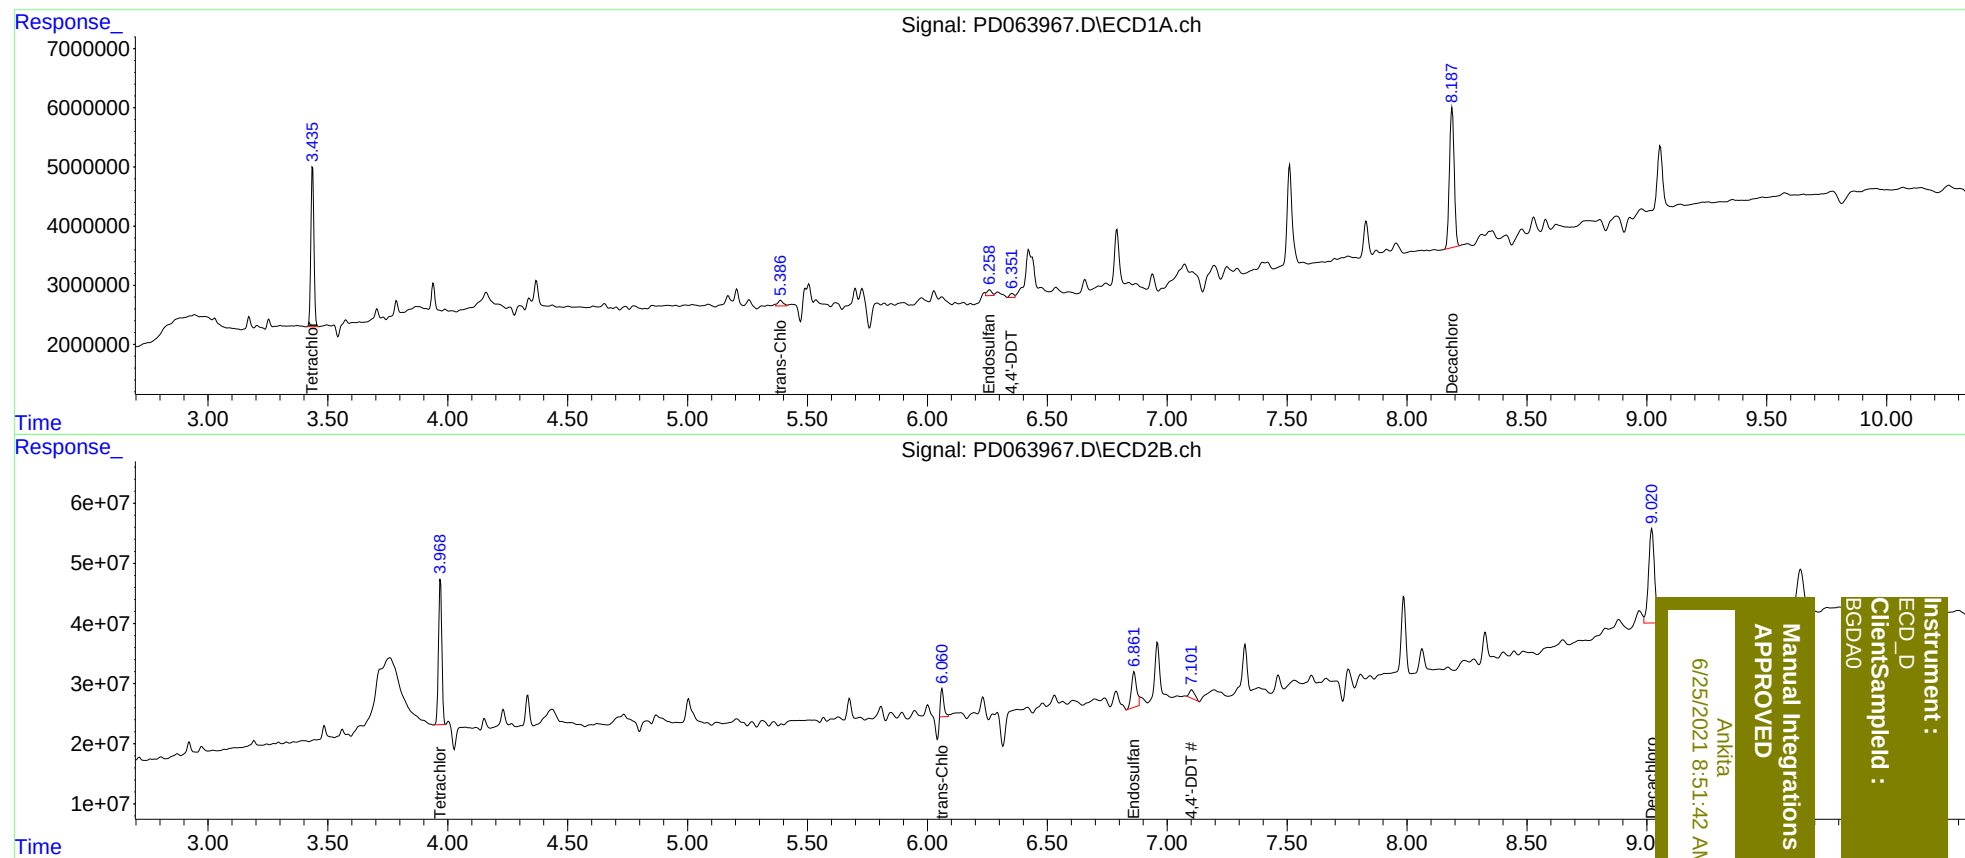

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:42 AM

Instrument :
ECD_D
ClientSampled :
BGDA0