

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 20:03
 Operator : AR\AJ
 Sample : M2682-19MS
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGDB5MS

Manual Integrations
 APPROVED

Ankita
 6/25/2021 8:51:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 06:35:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.970	14342775	139.0E6	9.227	8.779
27)	SA Decachlor...	8.190	9.021	27775943	214.7E6	16.047	15.483
Target Compounds							
2)	A alpha-BHC	3.873	4.356	123.4E6	1164.0E6	52.739	46.849m
3)	MA gamma-BHC...	4.155	4.642	117.6E6	1052.1E6	51.668	46.108
4)	MA Heptachlor	4.456	5.148	115.1E6	1073.4E6	52.725	46.077
5)	MB Aldrin	4.703	5.453	107.9E6	1032.4E6	53.244	46.864
6)	B beta-BHC	4.407	4.812	47283194	425.9E6	48.696	43.672
7)	B delta-BHC	4.611	5.029	115.7E6	964.7E6	53.581	41.173
8)	B Heptachlo...	5.146	5.838	104.0E6	818.7E6	54.870	39.792 #
9)	A Endosulfan I	5.484	6.194	91405542	866.6E6	49.952	43.743
10)	B trans-Chl...	5.372	6.072	103.1E6	927.9E6	52.996	44.111
11)	B cis-Chlor...	5.431	6.144	99664876	940.1E6	52.456	46.680
12)	B 4,4'-DDE	5.594	6.302	219.5E6	1829.2E6	111.172	90.532
13)	MA Dieldrin	5.727	6.451	216.5E6	1885.9E6	103.432	90.149
14)	MA Endrin	5.986	6.669	190.3E6	1532.4E6	105.246	87.584
15)	B Endosulfa...	6.259	6.878	179.2E6	1554.2E6	109.660	96.049
16)	A 4,4'-DDD	6.111	6.791	173.2E6	1560.9E6	104.906	92.724
17)	MA 4,4'-DDT	6.352	7.090	180.2E6	1508.6E6	107.056	91.637
18)	B Endrin al...	6.426	7.002	154.6E6	1321.9E6	108.258m	93.962
19)	B Endosulfa...	6.641	7.224	164.5E6	1510.6E6	105.980	91.784
20)	A Methoxychlor	6.898	7.548	456.2E6	3360.2E6	494.863	434.325
21)	B Endrin ke...	7.132	7.694	215.1E6	1522.6E6	113.405m	95.945

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 20:03
Operator : AR\AJ
Sample : M2682-19MS
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:35:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

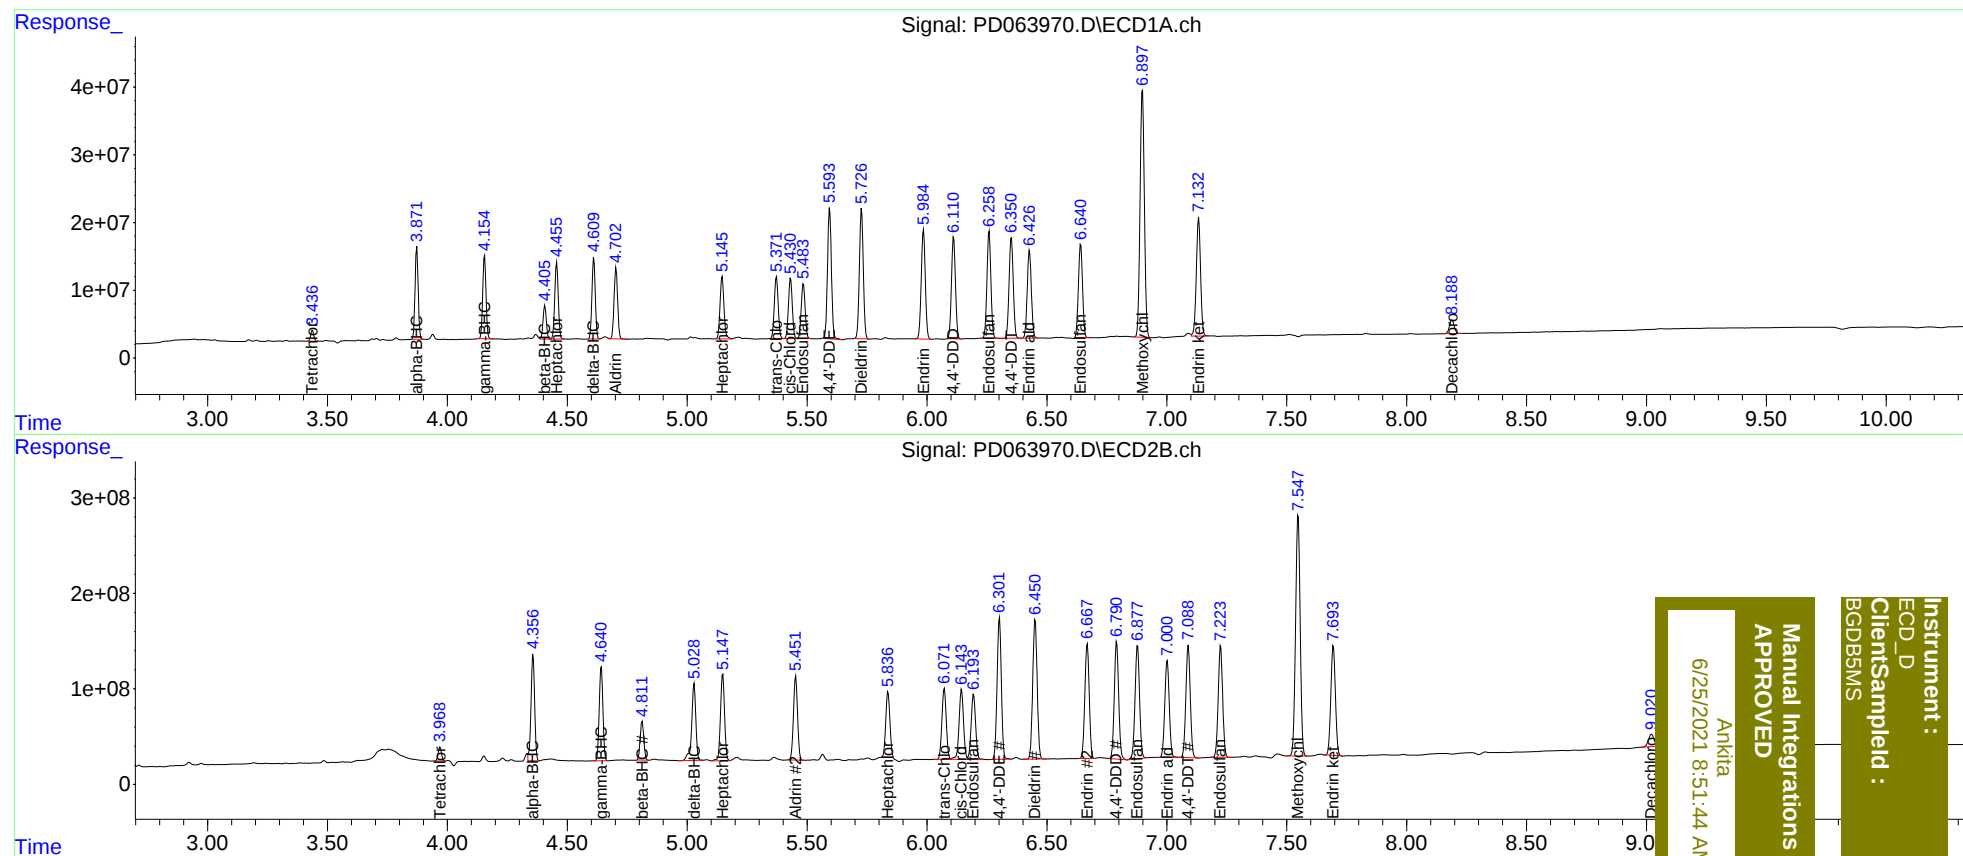

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:44 AM

Instrument :
ECD_D
Client Sampled :
BGDB5MS