

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:23
Operator : AR\AJ
Sample : M2682-08
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BGD95

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

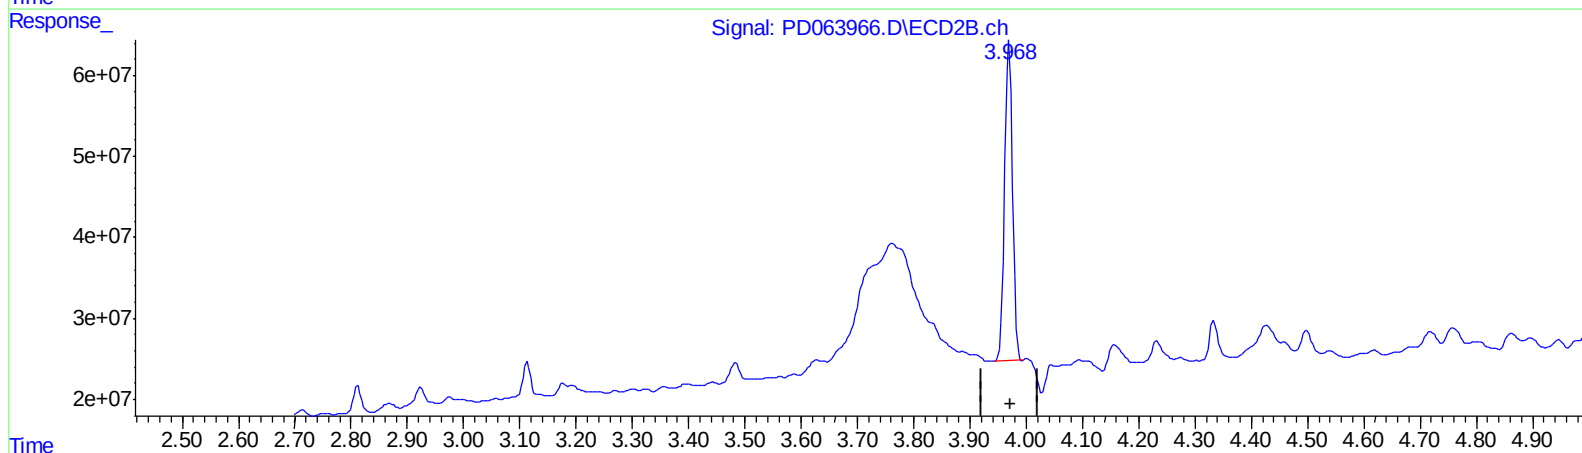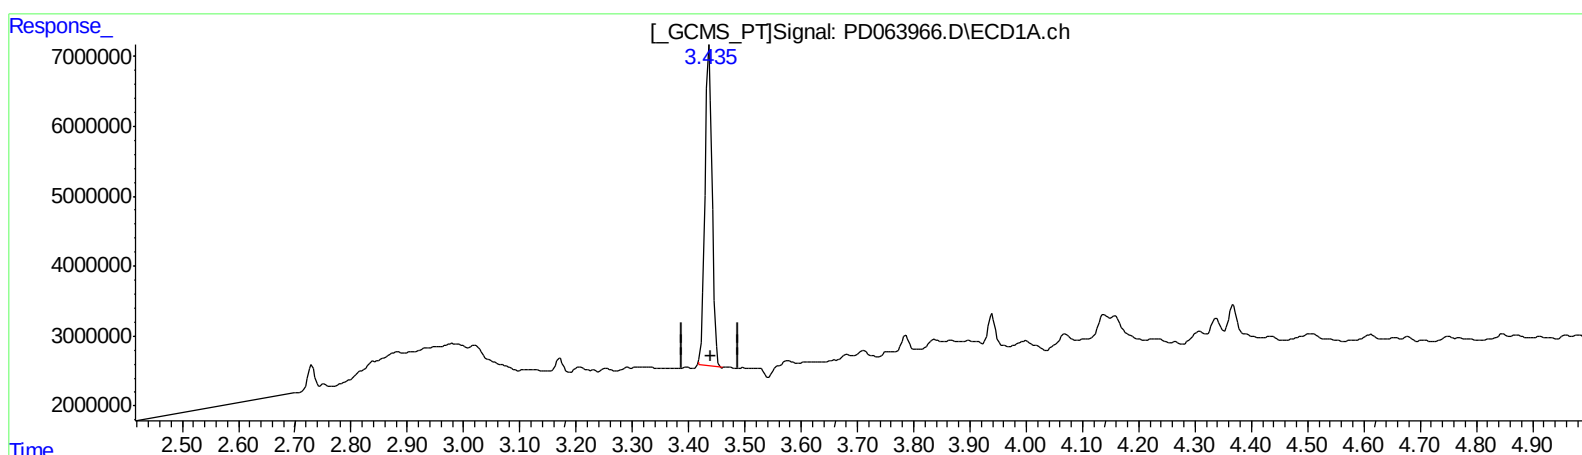

QEdit

(1) Tetrachloro-m-xylene (SA)

3.436min 25.427 ng/ml

response 39526807

(1) Tetrachloro-m-xylene #2 (SA)

3.970min 23.781 ng/ml

response 376636293

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:23
Operator : AR\AJ
Sample : M2682-08
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BGD95

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

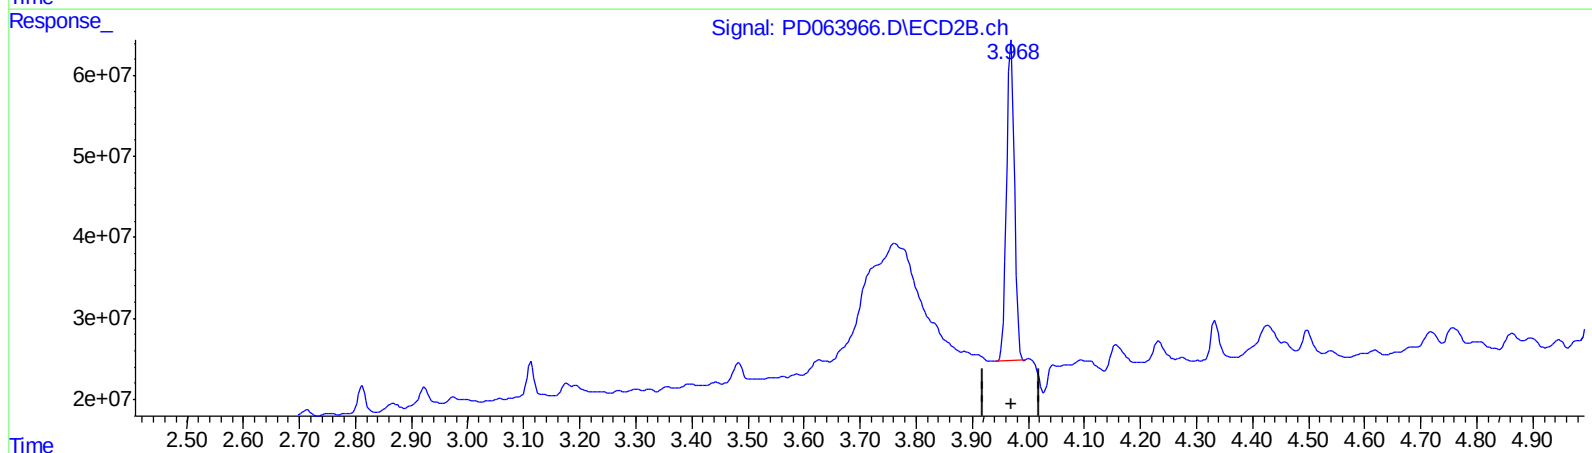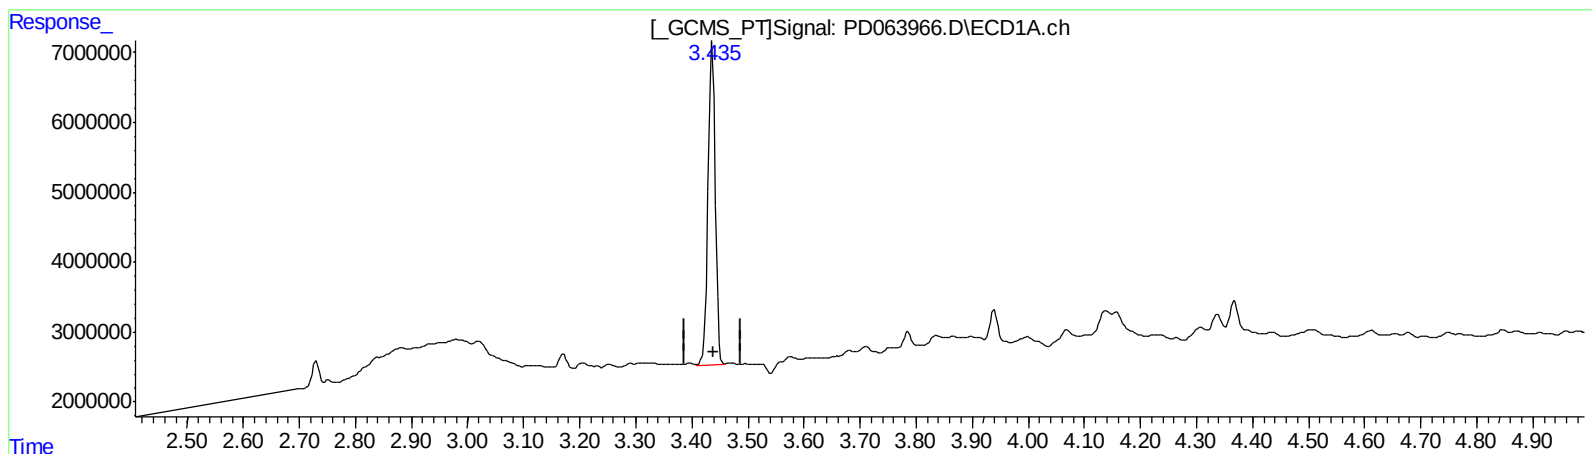

QEdit

(1) Tetrachloro-m-xylene (SA)

3.435min 26.027 ng/ml m

response 40458797

(1) Tetrachloro-m-xylene #2 (SA)

3.970min 23.781 ng/ml

response 376636293

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:23
Operator : AR\AJ
Sample : M2682-08
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampled :
BGD95

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

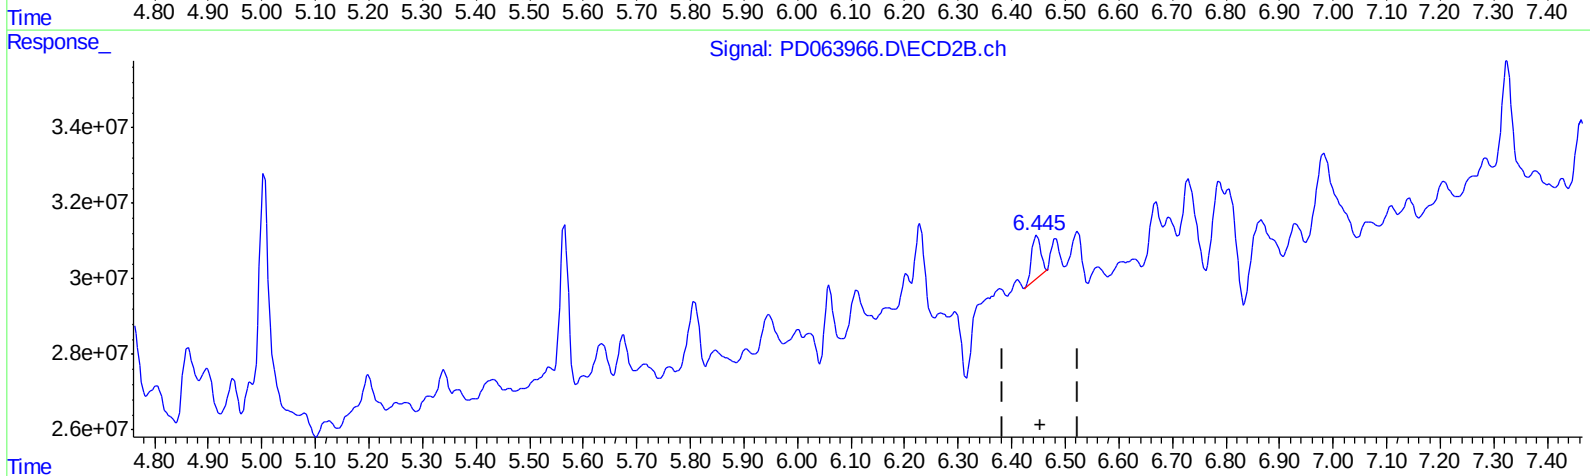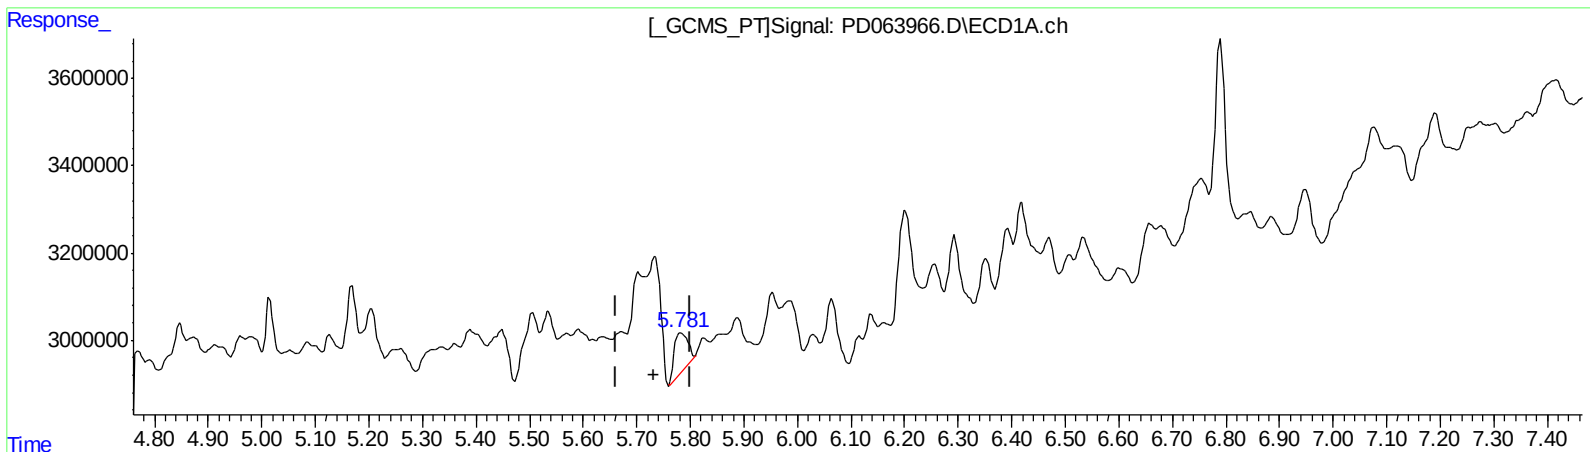

QEdit

(13) Dieldrin (MA)
5.783min 0.737 ng/ml
response 1542378

(13) Dieldrin #2 (MA)
6.447min 0.621 ng/ml
response 12996708

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:23
Operator : AR\AJ
Sample : M2682-08
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampled :
BGD95

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

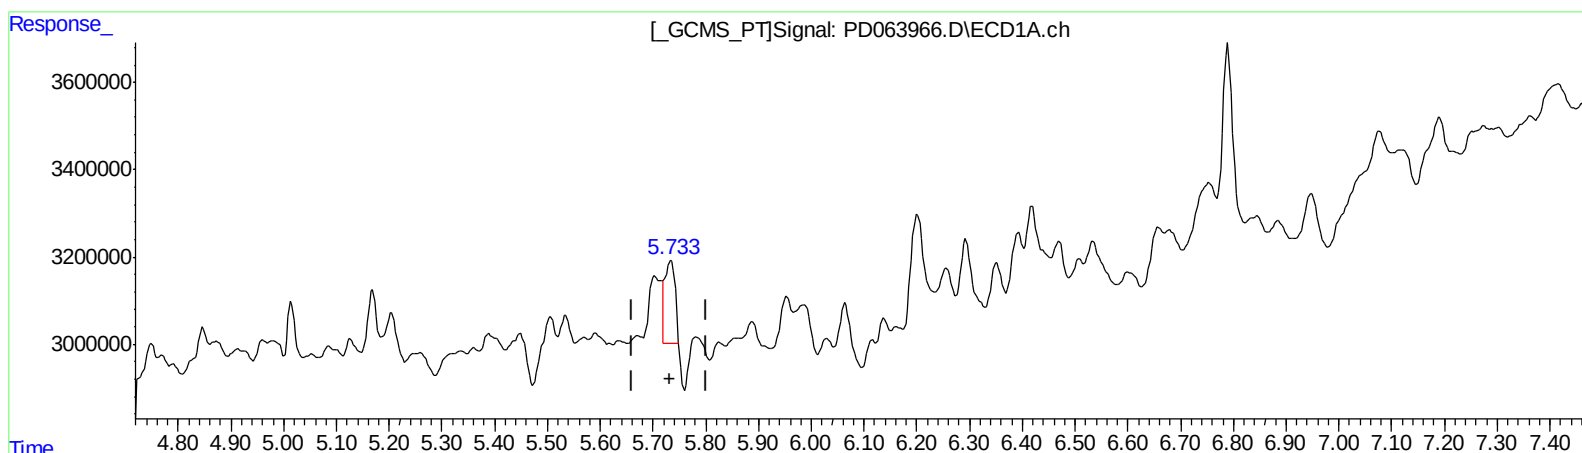

(13) Dieldrin (MA)
5.733min 1.220 ng/ml m
response 2553525

(13) Dieldrin #2 (MA)
6.447min 0.621 ng/ml
response 12996708

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:23
Operator : AR\AJ
Sample : M2682-08
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
BGD95

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

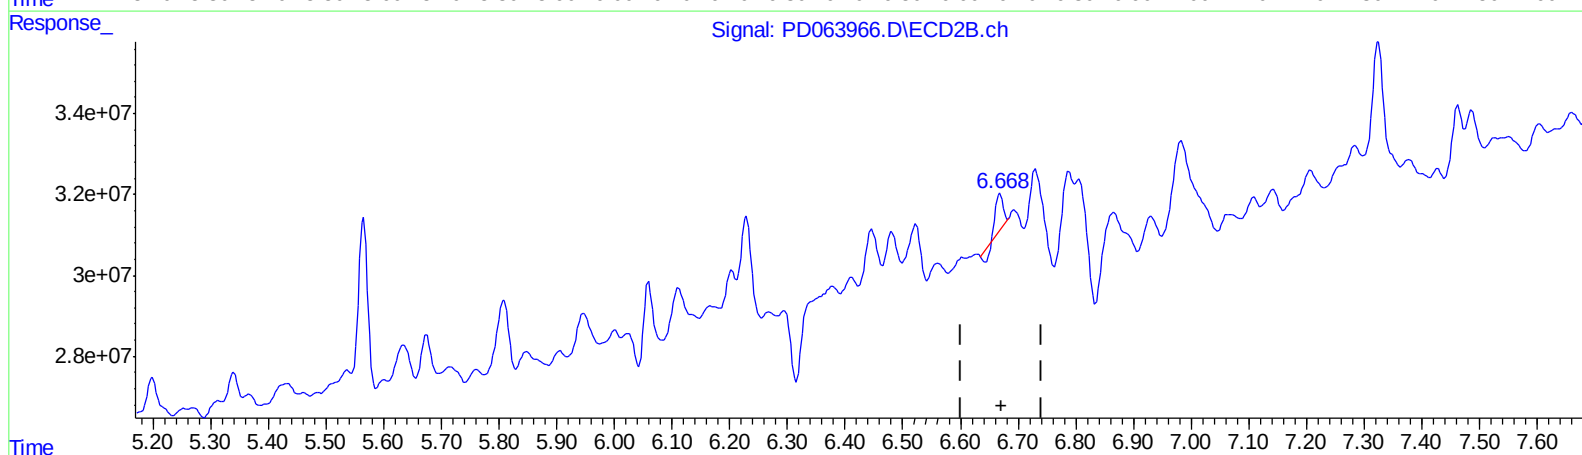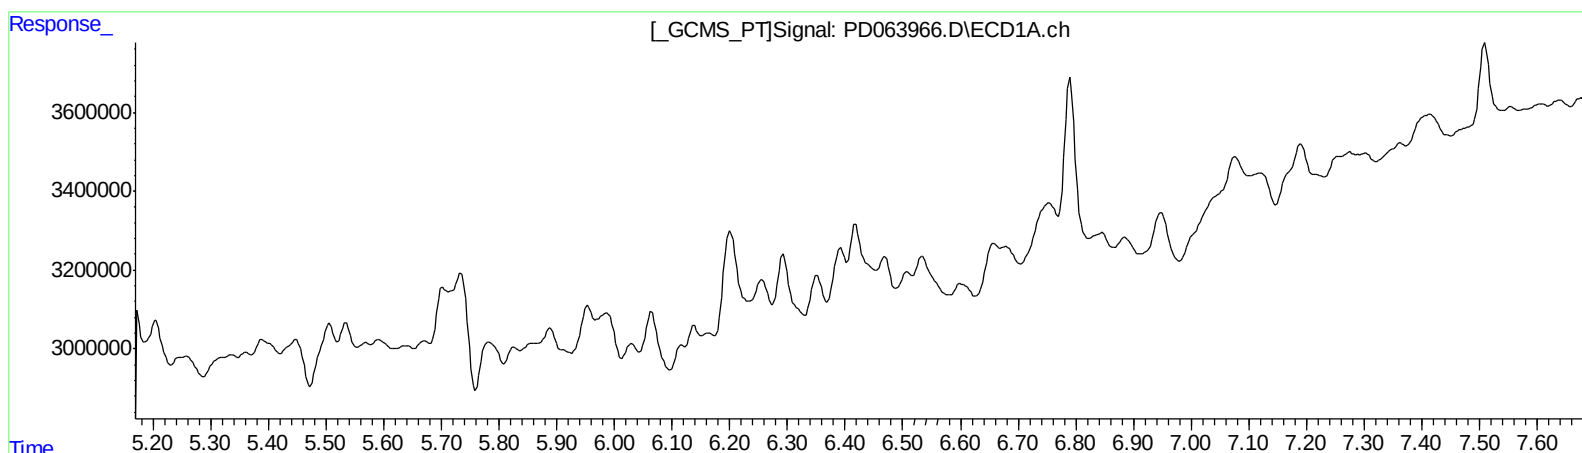

QEdit

(14) Endrin (MA)
0.000min 0.000 ng/ml
response 0

(14) Endrin #2 (MA)
6.669min 0.328 ng/ml
response 5732142

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 18:23
Operator : AR\AJ
Sample : M2682-08
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
BGD95

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:29:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

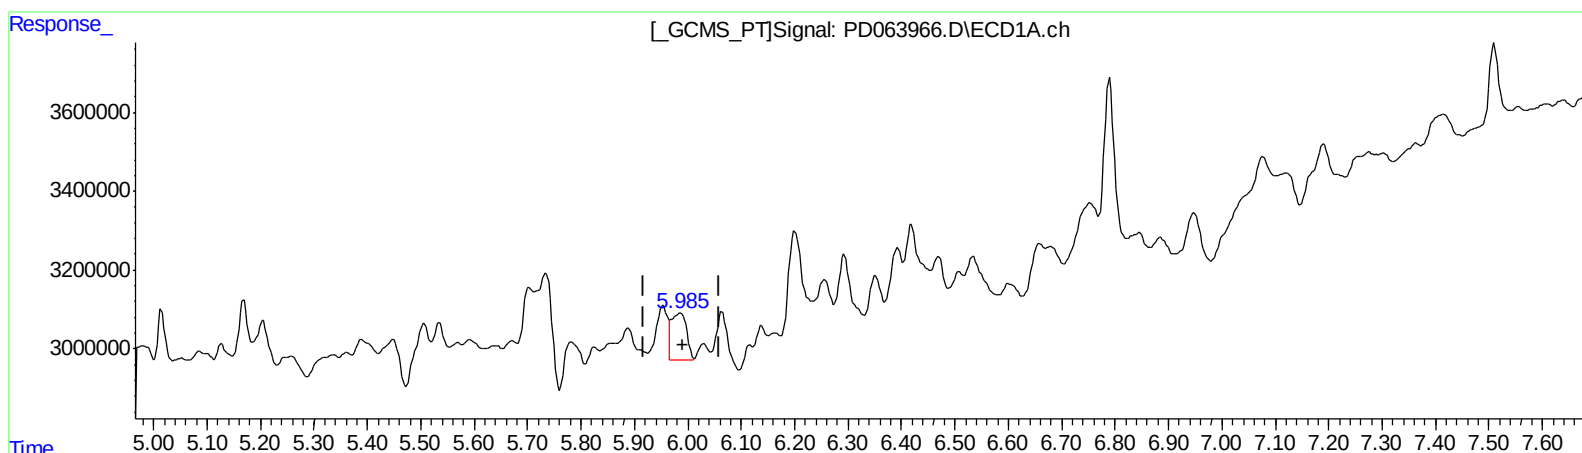

QEdit

(14) Endrin (MA)

5.985min 1.308 ng/ml m

response 2364781

(14) Endrin #2 (MA)

6.668min 1.211 ng/ml m

response 21179315

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 18:23
 Operator : AR\AJ
 Sample : M2682-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGD95

Manual Integrations
 APPROVED

Ankita
 6/25/2021 8:51:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 06:29:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.435	3.970	40458797	376.6E6	26.027m	23.781
27) SA Decachlor...	8.188	9.020	61462671	490.9E6	35.508	35.396
Target Compounds						
13) MA Dieldrin	5.733	6.447	2553525	12996708	1.220m	0.621 #
14) MA Endrin	5.985	6.668	2364781	21179315	1.308m	1.211m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 06/28/21