

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
 Data File : PD063971.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2021 20:17
 Operator : AR\AJ
 Sample : M2682-20MSD
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGDB5MSD

Manual Integrations
 APPROVED

Ankita
 6/25/2021 8:51:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 24 06:35:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.969	14514721	138.5E6	9.337	8.743
27)	SA Decachlor...	8.190	9.022	27309604	217.3E6	15.777	15.669
Target Compounds							
2)	A alpha-BHC	3.873	4.356	123.3E6	1172.8E6	52.729	47.204m
3)	MA gamma-BHC...	4.156	4.641	117.5E6	1047.5E6	51.611	45.909
4)	MA Heptachlor	4.456	5.148	115.2E6	1078.4E6	52.773	46.290
5)	MB Aldrin	4.703	5.452	107.3E6	1031.1E6	52.960	46.804
6)	B beta-BHC	4.407	4.812	47282853	426.3E6	48.695	43.706
7)	B delta-BHC	4.611	5.029	115.9E6	923.9E6	53.675	39.433 #
8)	B Heptachlo...	5.146	5.838	104.2E6	818.6E6	54.964	39.789 #
9)	A Endosulfan I	5.485	6.194	91179261	858.3E6	49.829	43.324
10)	B trans-Chl...	5.373	6.072	102.7E6	922.0E6	52.814	43.833
11)	B cis-Chlor...	5.431	6.144	99591380	932.2E6	52.418	46.288
12)	B 4,4'-DDE	5.595	6.302	215.7E6	1842.6E6	109.274	91.195
13)	MA Dieldrin	5.728	6.451	214.7E6	1878.6E6	102.578	89.800
14)	MA Endrin	5.986	6.667	187.2E6	1557.6E6	103.507	89.027m
15)	B Endosulfa...	6.260	6.878	177.4E6	1554.0E6	108.535	96.040
16)	A 4,4'-DDD	6.112	6.792	172.6E6	1565.2E6	104.541	92.980
17)	MA 4,4'-DDT	6.353	7.090	178.3E6	1498.4E6	105.917	91.022
18)	B Endrin al...	6.428	7.002	150.0E6	1300.5E6	105.088	92.441
19)	B Endosulfa...	6.642	7.225	165.5E6	1506.6E6	106.587	91.545
20)	A Methoxychlor	6.900	7.548	453.1E6	3358.1E6	491.495	434.048
21)	B Endrin ke...	7.132	7.695	209.8E6	1513.8E6	110.600m	95.390

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062321\
Data File : PD063971.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2021 20:17
Operator : AR\AJ
Sample : M2682-20MSD
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 24 06:35:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

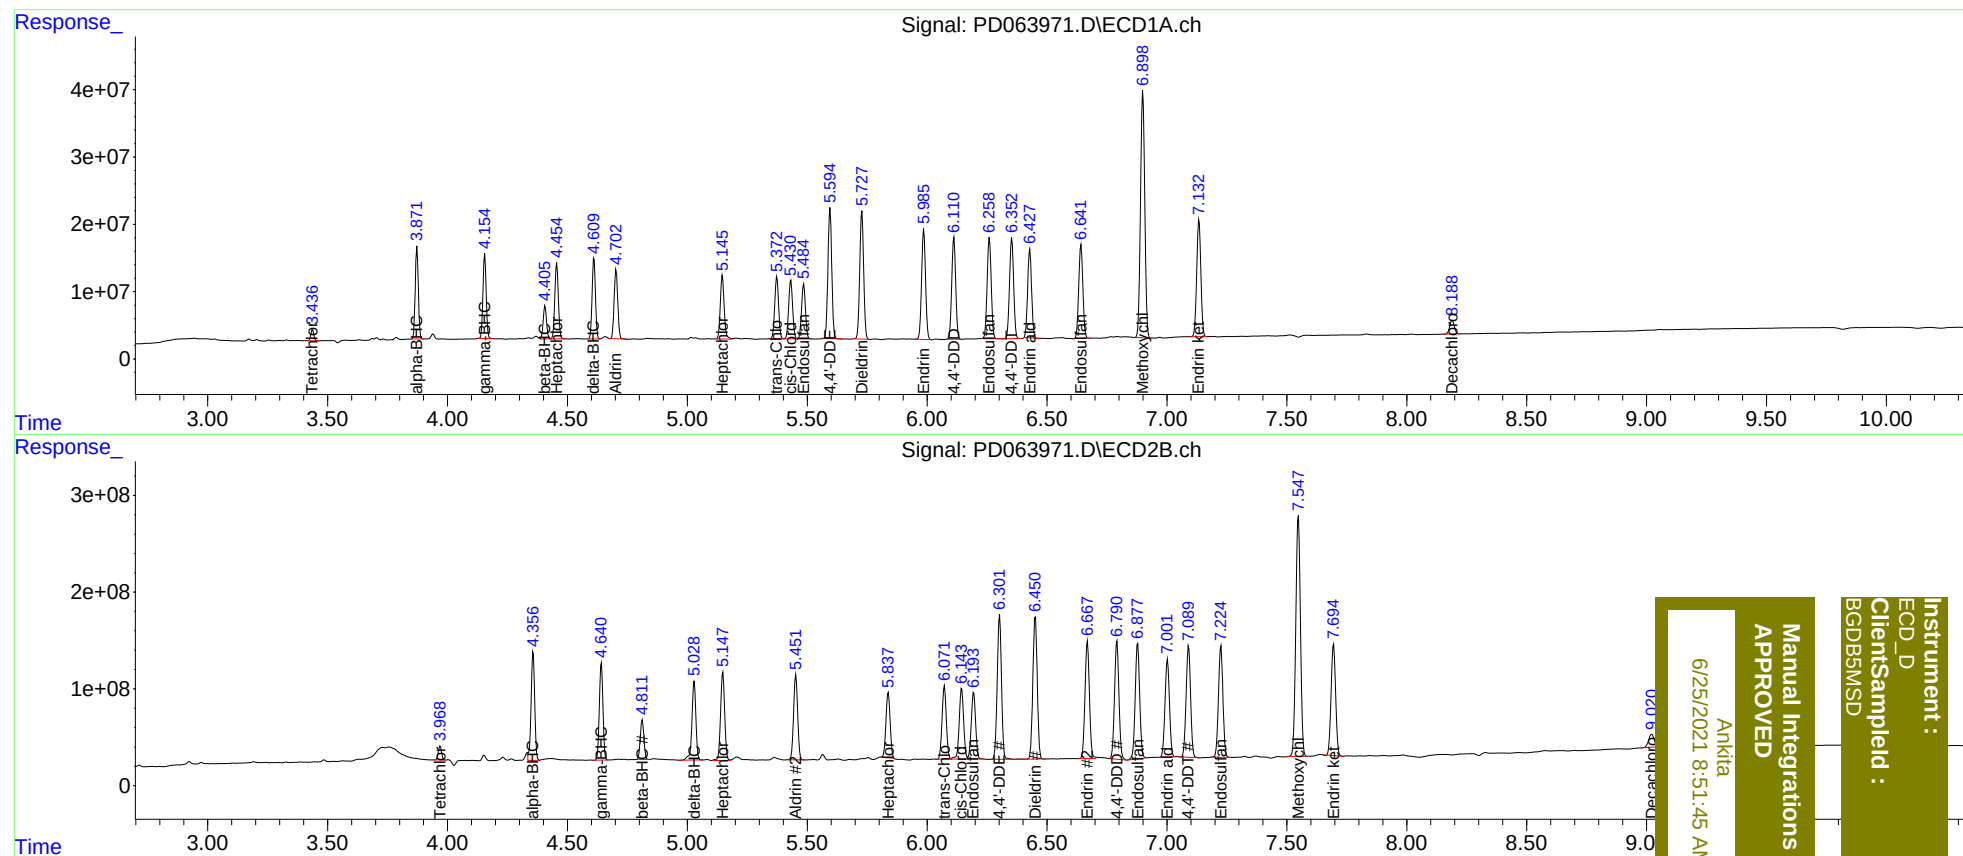

Manual Integrations
APPROVED

Ankita
6/25/2021 8:51:45 AM

Instrument :
ECD_D
ClientSampled :
BGDB5MSD