

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062322\
 Data File : PD070478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 22:16
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDB4001

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/23/2022
 Supervised By : Ankita Jodhani 06/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 10:52:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 23 10:52:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.121	60383723	537.8E6	39.739	37.308
27)	SA Decachlor...	8.126	9.277	131.5E6	581.9E6	76.382	70.444
Target Compounds							
5)	MB Aldrin	4.654	5.636	88475582	669.3E6	41.249	36.851
6)	B beta-BHC	4.365	4.966	39655195	335.0E6	38.408	37.003
7)	B delta-BHC	4.566	5.189	96037236	471.1E6	42.259	49.990m
8)	B Heptachlo...	5.095	6.023	81446494	414.2E6	40.407	52.995 #
10)	B trans-Chl...	5.319	6.259	83924865	591.4E6	40.853	37.087
11)	B cis-Chlor...	5.378	6.333	81587054	569.5E6	39.975	36.518
12)	B 4,4'-DDE	5.543	6.485	165.5E6	1084.6E6	84.788	74.860
15)	B Endosulfa...	6.203	7.067	140.6E6	849.1E6	82.189	73.497
18)	B Endrin al...	6.372	7.191	122.3E6	732.1E6	79.280	71.935
19)	B Endosulfa...	6.584	7.416	146.1E6	834.4E6	80.986	72.805
21)	B Endrin ke...	7.075	7.889	165.3E6	847.7E6	81.832	72.120

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062322\
Data File : PD070478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 22:16
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 10:52:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 23 10:52:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

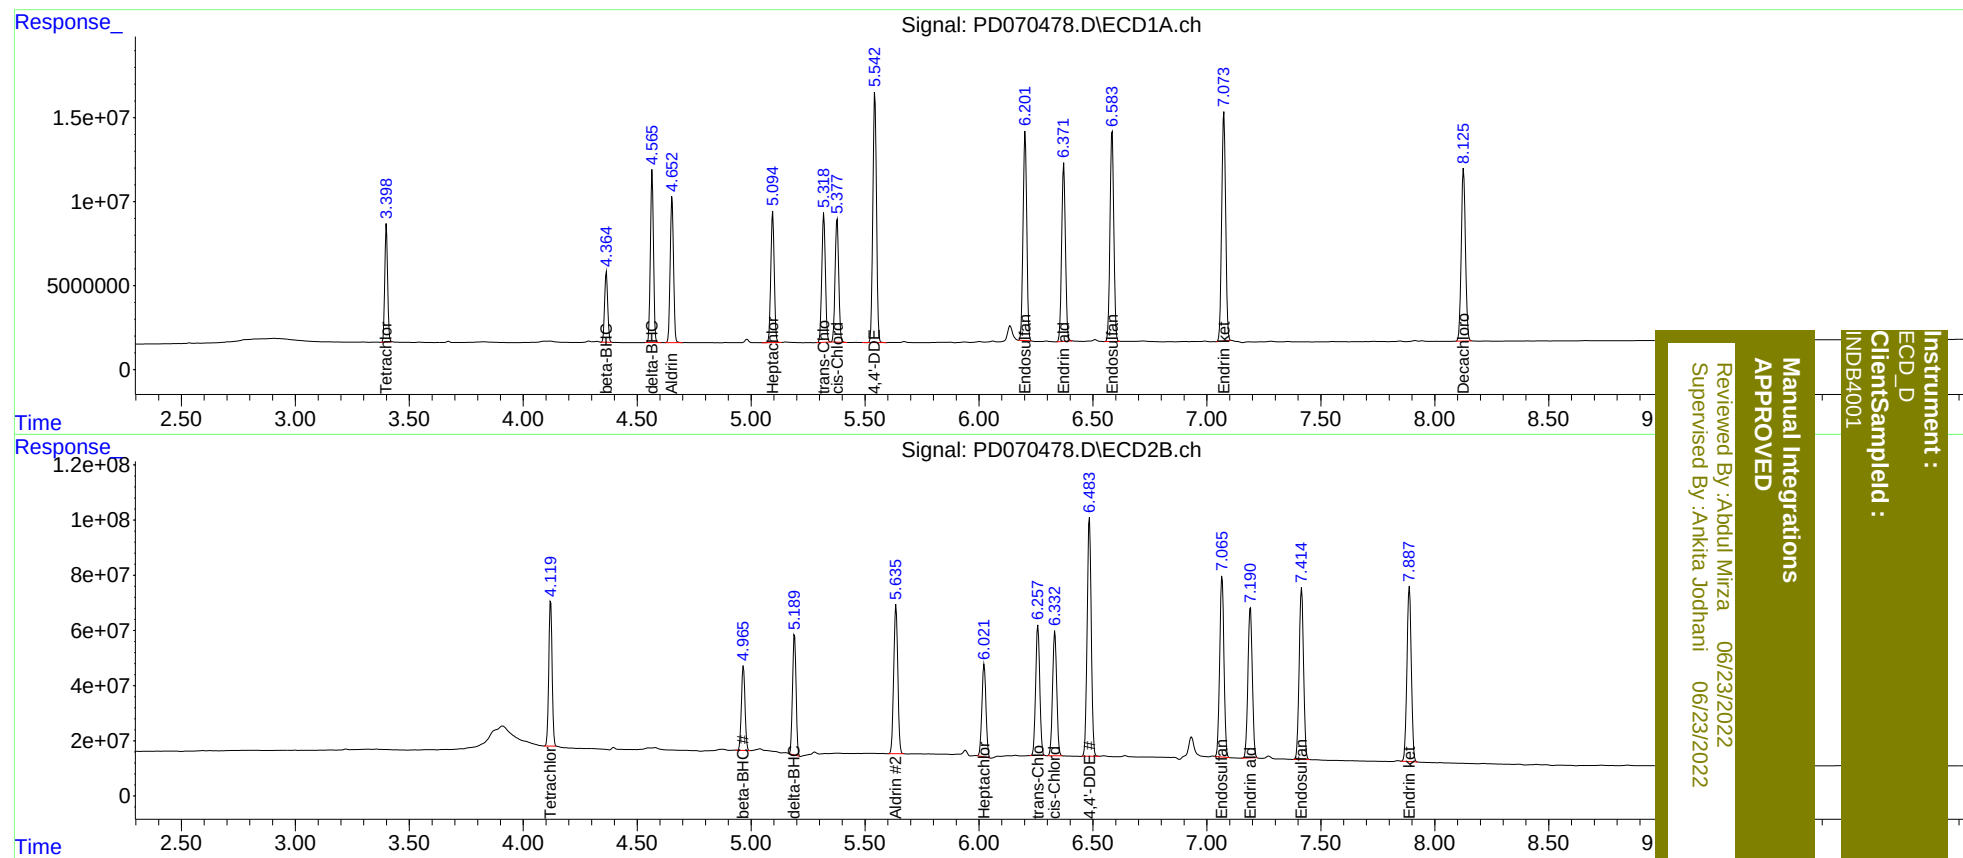

Reviewed By: Abdul Mirza 06/23/2022
Supervised By: Ankita Jodhani 06/23/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
INDB4001