

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062322\
 Data File : PD070463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 18:44
 Operator : AR\AJ
 Sample : RESC028
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC030

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/23/2022
 Supervised By :Ankita Jodhani 06/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 12:12:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062322CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 23 12:10:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.121	29240953	278.8E6	19.181	19.567
27)	SA Decachlor...	8.127	9.278	62730559	298.3E6	39.016	40.842
Target Compounds							
2)	A alpha-BHC	3.835	4.512	19253337	186.2E6	8.435	9.040m
3)	MA gamma-BHC...	4.115	4.802	18928345	176.3E6	8.680	9.463
4)	MA Heptachlor	4.407	5.326	18645541	161.3E6	8.646m	9.247
5)	MB Aldrin	4.654	5.636	21299023	180.8E6	9.821	10.548
6)	B beta-BHC	4.365	4.966	9888096	88377903	9.857	10.398
7)	B delta-BHC	4.566	5.189	22055455	75109568	9.449	7.261m
8)	B Heptachlo...	5.095	6.023	18973921	47137478	9.436	5.461m#
9)	A Endosulfan I	5.431	6.384	15653566	131.1E6	8.614	9.783
10)	B trans-Chl...	5.319	6.260	19806093	151.7E6	9.562	10.046
11)	B cis-Chlor...	5.378	6.334	19681643	161.5E6	9.680	11.024
12)	B 4,4'-DDE	5.543	6.486	37166932	297.9E6	18.642	21.597
13)	MA Dieldrin	5.674	6.641	35625077	261.3E6	17.209	18.885m
14)	MA Endrin	5.930	6.862	32801768	217.6E6	17.846	19.502
15)	B Endosulfa...	6.203	7.067	33393322	232.9E6	19.530	21.445
16)	A 4,4'-DDD	6.058	6.976	27557727	215.9E6	17.121	19.485
17)	MA 4,4'-DDT	6.297	7.278	27524122	201.6E6	16.976	19.425
18)	B Endrin al...	6.372	7.191	30734774	208.4E6	20.335	22.040
19)	B Endosulfa...	6.584	7.416	35370369	233.7E6	19.786	21.795
20)	A Methoxychlor	6.846	7.732	84123348	473.2E6	94.339	101.305
21)	B Endrin ke...	7.075	7.889	40883849	241.7E6	20.381	22.021

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062322\
Data File : PD070463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 18:44
Operator : AR\AJ
Sample : RESC028
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 12:12:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062322CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 23 12:10:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

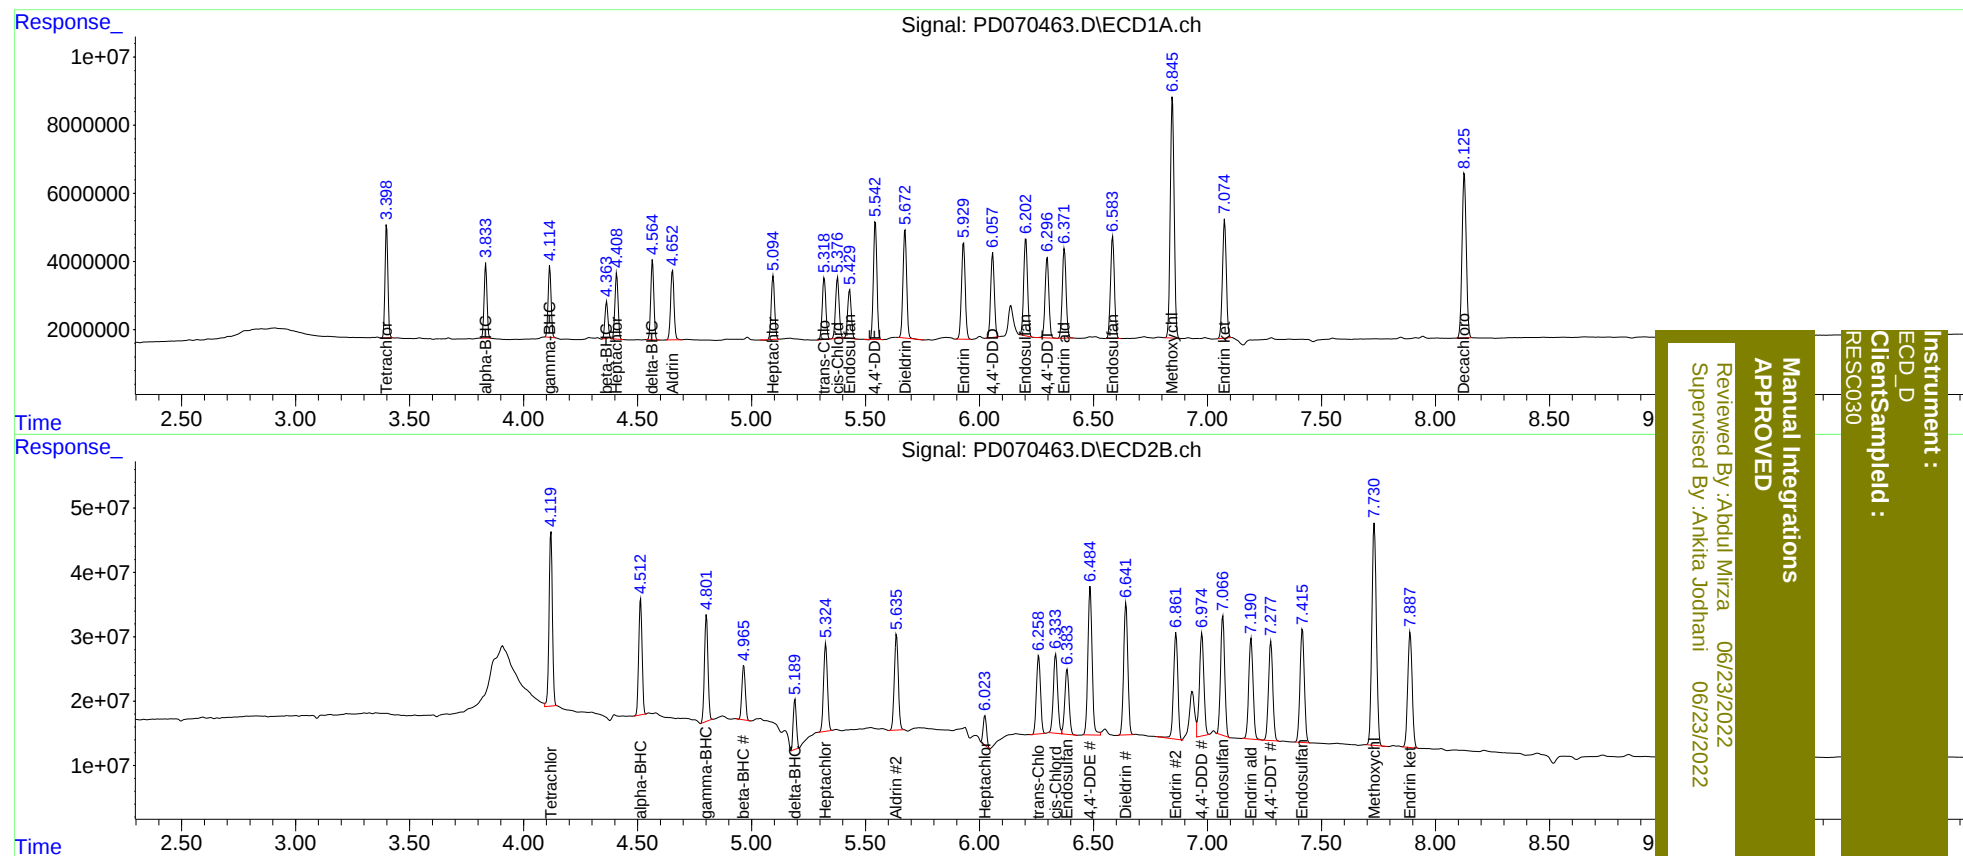

Reviewed By: Abdul Mirza 06/23/2022
Supervised By: Ankita Jodhani 06/23/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
RESC030