

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062323\
 Data File : PD076026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 08:43
 Operator : AR\AJ
 Sample : 03101-07
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEM0

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/22/2023
 Supervised By : Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 15:19:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.767	25677845	11694784	12.249	10.929
27)	SA Decachlor...	9.084	7.910	51391856	23074088	21.380	22.023
Target Compounds							
10)	B trans-Chl...	5.952	4.971	6995041	2848044	2.395m	2.157m
11)	B cis-Chlor...	6.036	5.034	10205414	2601648	3.367	1.895m#
12)	B 4,4'-DDE	6.203	5.224	4764984	3706128	1.711	3.216 #
16)	A 4,4'-DDD	6.723	5.779	29623178	13004972	13.731	14.204

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062323\
Data File : PD076026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 08:43
Operator : AR\AJ
Sample : 03101-07
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 15:19:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

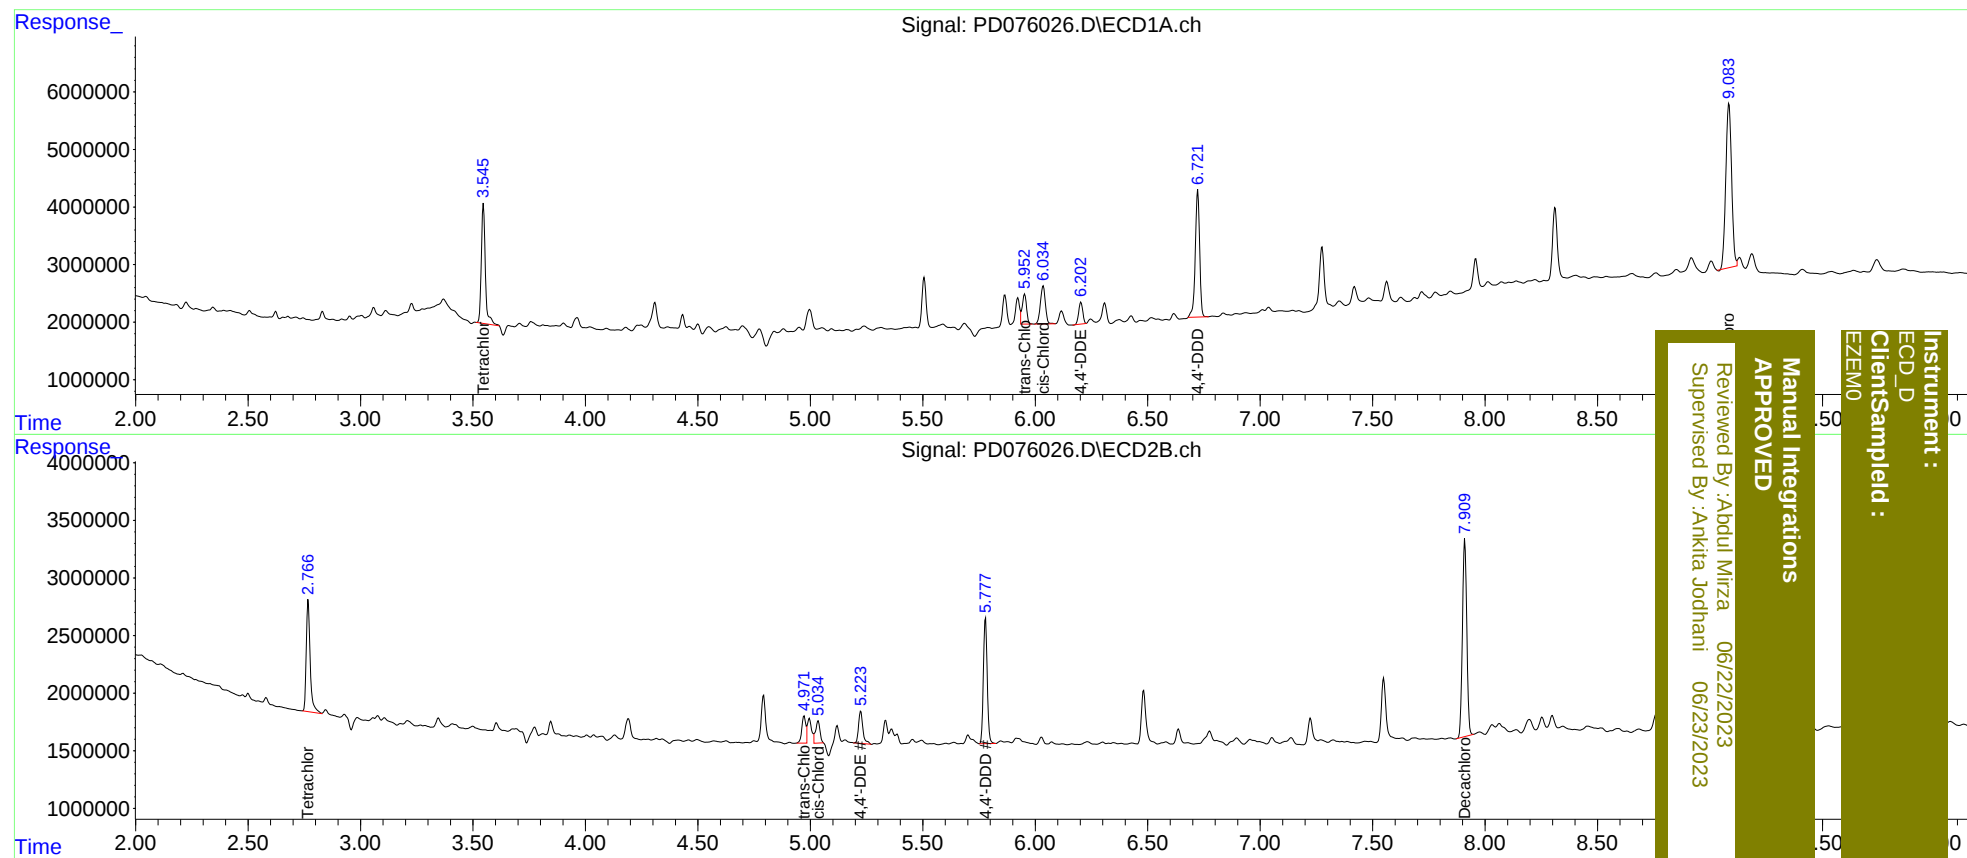

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/22/2023
Supervised By: Ankita Jodhani 06/23/2023

Instrument :
ECD_D
Client Sampled :
EZEMO