

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
 Data File : PD063976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2021 08:56
 Operator : AR\AJ
 Sample : PIBLK32
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 06:18:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.969	30493626	301.9E6	19.616	19.059
27)	SA Decachlor...	8.189	9.019	64562818	555.1E6	37.299	40.026
Target Compounds							
3)	MA gamma-BHC...	4.165	0.000	1504586	0	0.661	N.D. #
6)	B beta-BHC	4.368f	0.000	1300287	0	1.339	N.D. #
7)	B delta-BHC	0.000	5.004f	0	28687765	N.D.	1.224
8)	B Heptachlo...	0.000	5.848	0	4116473	N.D.	0.200
16)	A 4,4'-DDD	0.000	6.754f	0	3990934	N.D.	0.237


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
Data File : PD063976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2021 08:56
Operator : AR\AJ
Sample : PIBLK32
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 06:18:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

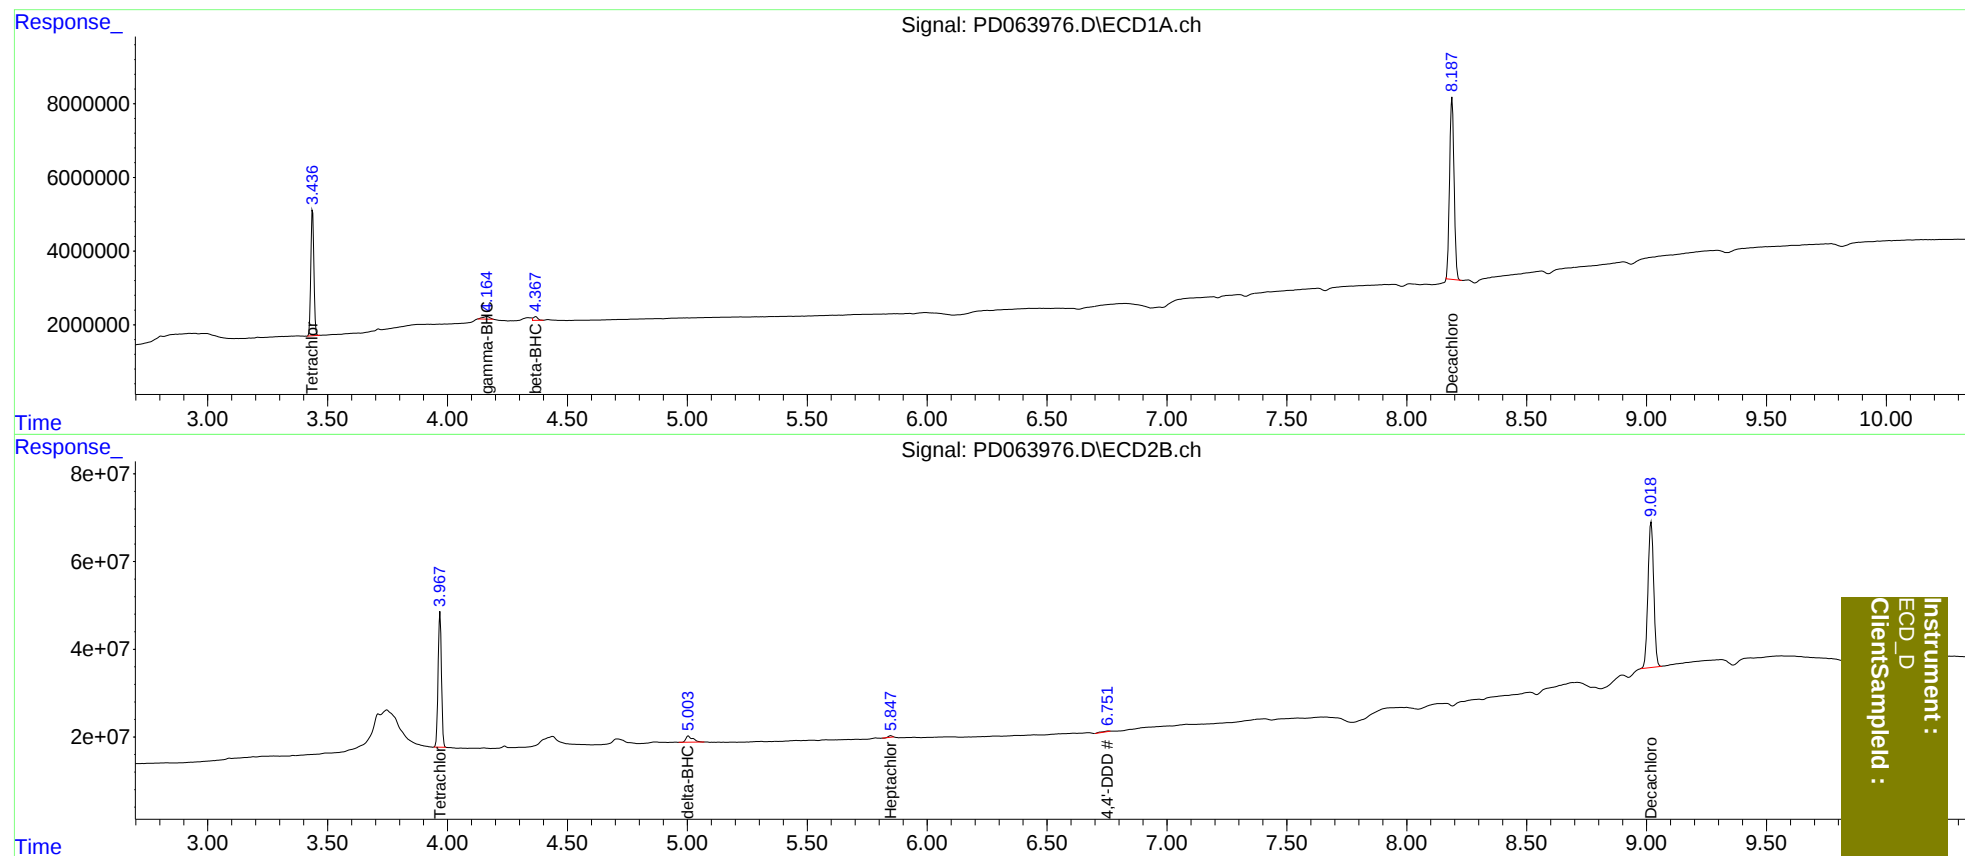


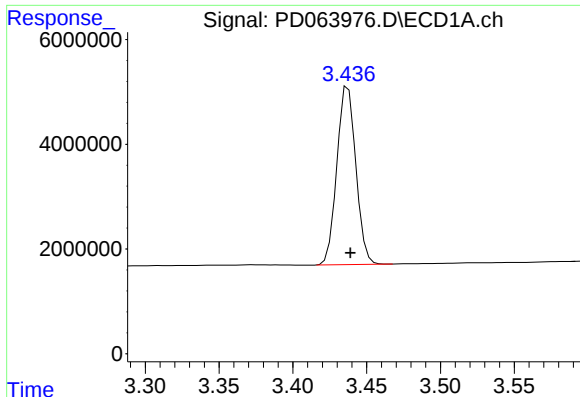

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: -0.002 min
Response: 30493626
Conc: 19.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

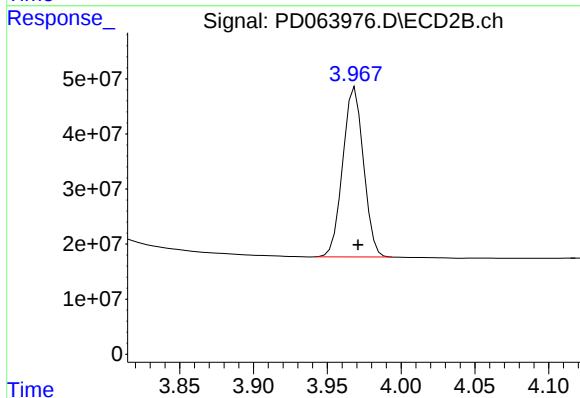


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.002 min
Response: 301860186
Conc: 19.06 ng/ml

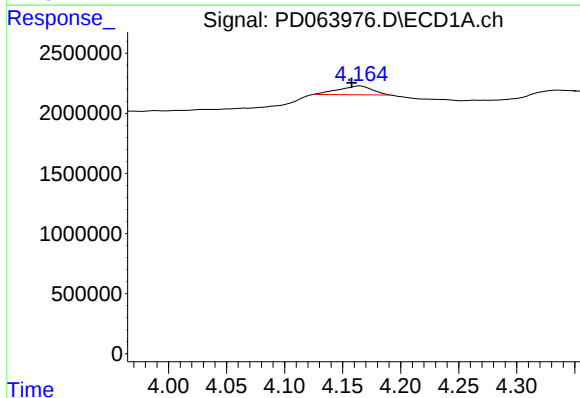


#3 gamma-BHC (Lindane)

R.T.: 4.165 min
Delta R.T.: 0.007 min
Response: 1504586
Conc: 0.66 ng/ml

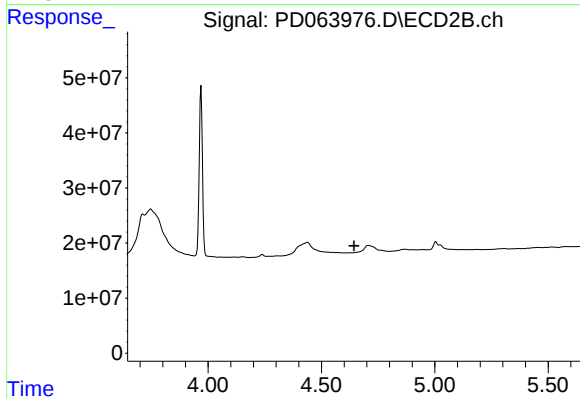

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.644 min
Response: 0
Conc: N.D.

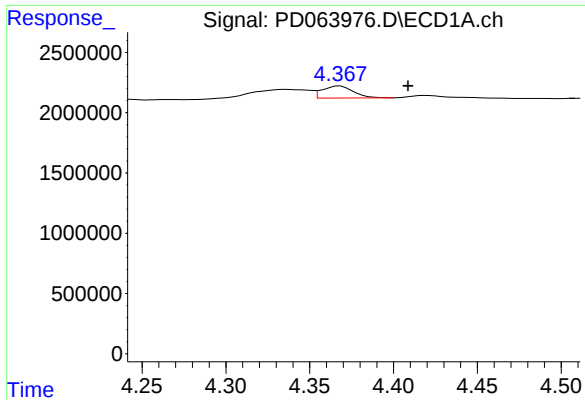

#6 beta-BHC


R.T.: 4.368 min
Delta R.T.: -0.041 min
Response: 1300287
Conc: 1.34 ng/ml

Instrument :
ECD_D
ClientSampleId :

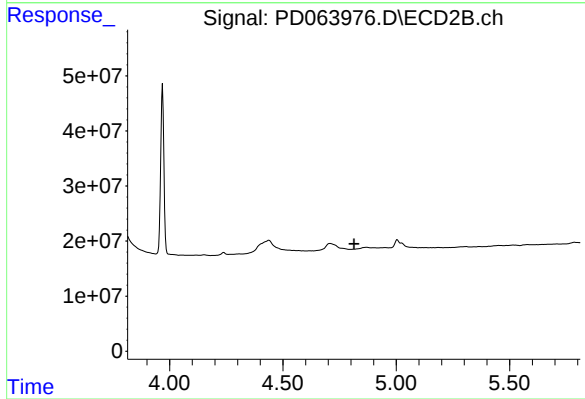


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.814 min
Response: 0
Conc: N.D.

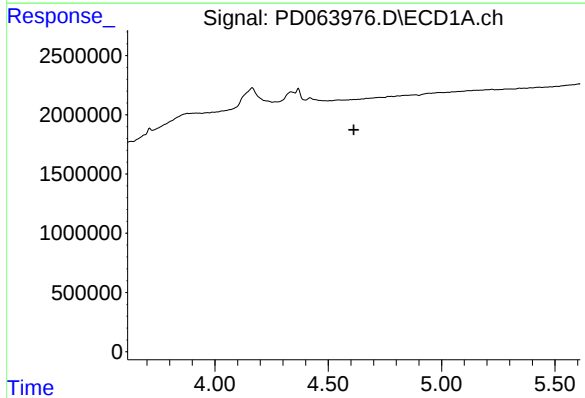


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

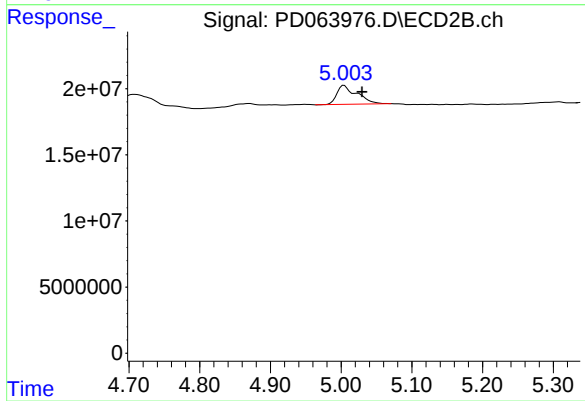

#7 delta-BHC


R.T.: 5.004 min
Delta R.T.: -0.026 min
Response: 28687765
Conc: 1.22 ng/ml

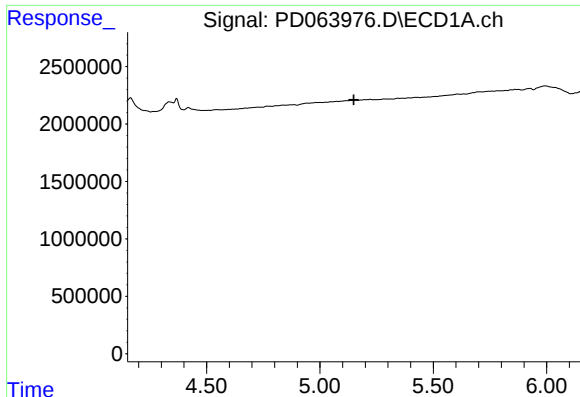

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

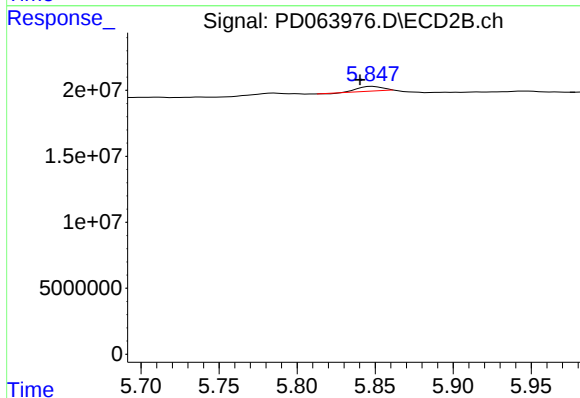


#8 Heptachlor epoxide

R.T.: 5.848 min
Delta R.T.: 0.008 min
Response: 4116473
Conc: 0.20 ng/ml

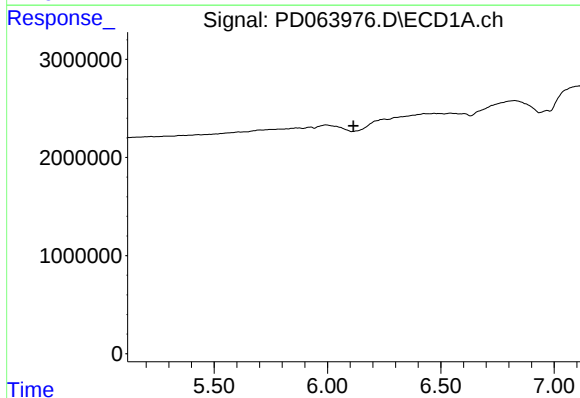


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.115 min
Response: 0
Conc: N.D.

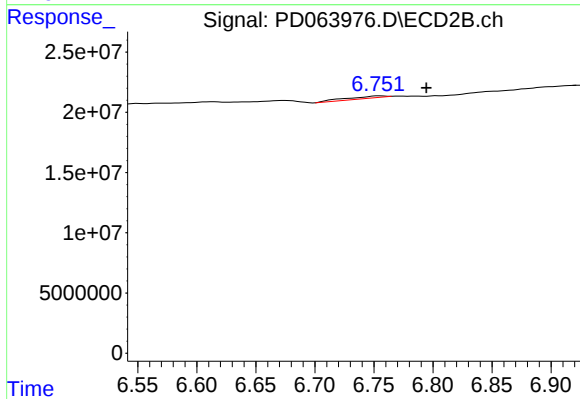

#16 4,4'-DDD


R.T.: 6.754 min
Delta R.T.: -0.040 min
Response: 3990934
Conc: 0.24 ng/ml

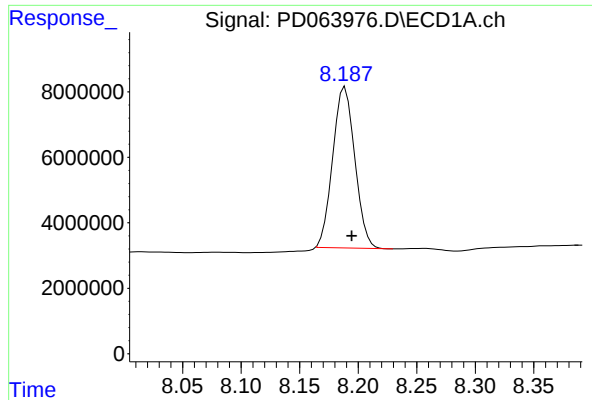

#27 Decachlorobiphenyl

R.T.: 8.189 min
Delta R.T.: -0.006 min
Response: 64562818
Conc: 37.30 ng/ml

Instrument :
ECD_D
ClientSampleId :

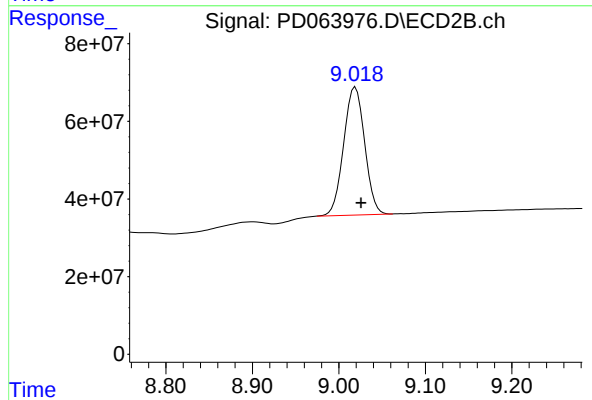

#27 Decachlorobiphenyl

R.T.: 9.019 min
Delta R.T.: -0.007 min
Response: 555095861
Conc: 40.03 ng/ml