

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
 Data File : PD063979.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2021 10:43
 Operator : AR\AJ
 Sample : PB137299BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS299

Manual Integrations
 APPROVED

Ankita
 6/25/2021 11:06:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 08:42:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.968	34364670	334.2E6	22.106	21.104
27)	SA Decachlor...	8.190	9.019	78009334	632.0E6	45.067	45.571
Target Compounds							
2)	A alpha-BHC	3.873	4.356	12160342	132.3E6	5.199	5.325
3)	MA gamma-BHC...	4.157	4.640	11869186	122.2E6	5.215	5.355
4)	MA Heptachlor	4.456	5.145	11123953	125.3E6	5.095	5.379m
5)	MB Aldrin	4.704	5.451	10833156	122.2E6	5.345	5.545
6)	B beta-BHC	4.408	4.811	6193418	53065209	6.378	5.441
7)	B delta-BHC	4.611	5.027	11030240	145.3E6	5.110	6.200
8)	B Heptachlo...	5.147	5.836	10322604	130.7E6	5.444	6.354m
9)	A Endosulfan I	5.485	6.193	9430066	104.5E6	5.153	5.273
10)	B trans-Chl...	5.374	6.071	10201714	111.1E6	5.246	5.281
11)	B cis-Chlor...	5.432	6.143	10200625	108.6E6	5.369	5.393
12)	B 4,4'-DDE	5.595	6.300	21181088	219.0E6	10.728	10.837
13)	MA Dieldrin	5.729	6.449	21074648	221.1E6	10.070	10.571
14)	MA Endrin	5.986	6.666	17691483	171.2E6	9.782	9.783
15)	B Endosulfa...	6.259	6.876	18216799	193.9E6	11.148	11.985
16)	A 4,4'-DDD	6.112	6.789	17363101	198.3E6	10.516	11.778
17)	MA 4,4'-DDT	6.353	7.088	14480152	149.2E6	8.604	9.064
18)	B Endrin al...	6.428	7.000	16079588	157.5E6	11.263	11.192
19)	B Endosulfa...	6.642	7.223	16658975	178.3E6	10.731	10.836
20)	A Methoxychlor	6.900	7.547	47376322	400.8E6	51.388	51.806
21)	B Endrin ke...	7.132	7.691	22615959	183.2E6	11.921m	11.541m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
Data File : PD063979.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2021 10:43
Operator : AR\AJ
Sample : PB137299BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 08:42:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

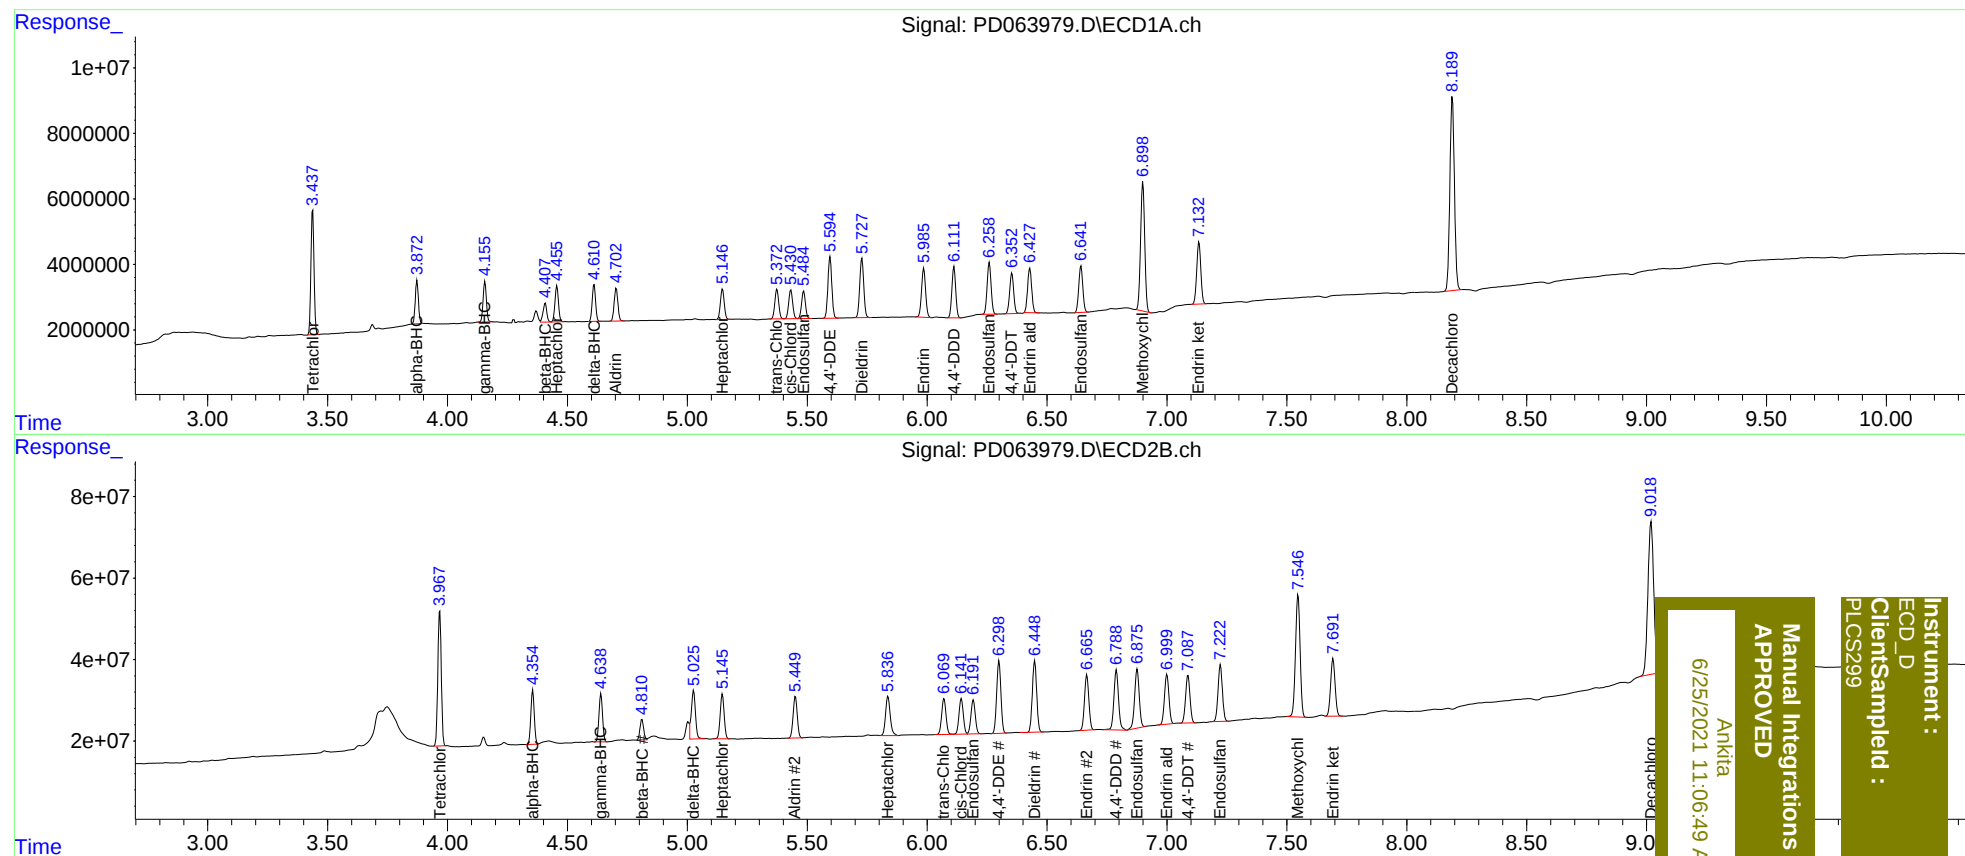

6/25/2021 11:06:49 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sample :
PLCS299