

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
 Data File : PD063982.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2021 11:24
 Operator : AR\AJ
 Sample : M2761-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLX83MSD

Manual Integrations
 APPROVED

Ankita
 6/25/2021 11:06:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 09:02:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.968	15411149	169.4E6	9.914	10.693
2)	SA Decachlor...	8.189	9.019	26550681	209.3E6	15.339	15.093m
Target Compounds							
2)	A alpha-BHC	3.873	4.355	127.5E6	1203.5E6	54.530	48.439m
3)	MA gamma-BHC...	4.155	4.641	115.1E6	1103.8E6	50.562	48.377
4)	MA Heptachlor	4.456	5.147	122.1E6	1157.9E6	55.914	49.702
5)	MB Aldrin	4.703	5.451	112.8E6	1054.3E6	55.662	47.857
6)	B beta-BHC	4.407	4.812	53450321	427.1E6	55.047	43.790
7)	B delta-BHC	4.610	5.028	83168327	788.8E6	38.530	33.666
8)	B Heptachlo...	5.146	5.836	110.0E6	962.9E6	58.021	46.802m
9)	A Endosulfan I	5.485	6.193	95553666	921.0E6	52.219	46.492
10)	B trans-Chl...	5.373	6.072	110.2E6	1008.2E6	56.680	47.929
11)	B cis-Chlor...	5.431	6.144	104.9E6	953.4E6	55.220	47.337
12)	B 4,4'-DDE	5.594	6.300	229.9E6	1874.2E6	116.449	92.762
13)	MA Dieldrin	5.728	6.450	230.9E6	1983.2E6	110.322	94.800
14)	MA Endrin	5.985	6.666	197.9E6	1625.6E6	109.444	92.910m
15)	B Endosulfa...	6.259	6.877	189.0E6	1632.7E6	115.630	100.902
16)	A 4,4'-DDD	6.111	6.790	186.3E6	1648.4E6	112.855	97.924
17)	MA 4,4'-DDT	6.352	7.089	190.5E6	1598.2E6	113.197	97.081
18)	B Endrin al...	6.426	7.001	163.8E6	1381.6E6	114.730m	98.211
19)	B Endosulfa...	6.642	7.224	245.3E6	1521.0E6	158.010	92.415 #
20)	A Methoxychlor	6.898	7.547	475.3E6	3571.2E6	515.530	461.593
21)	B Endrin ke...	7.131	7.693	221.9E6	1638.8E6	116.950m	103.263m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
Data File : PD063982.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2021 11:24
Operator : AR\AJ
Sample : M2761-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 09:02:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

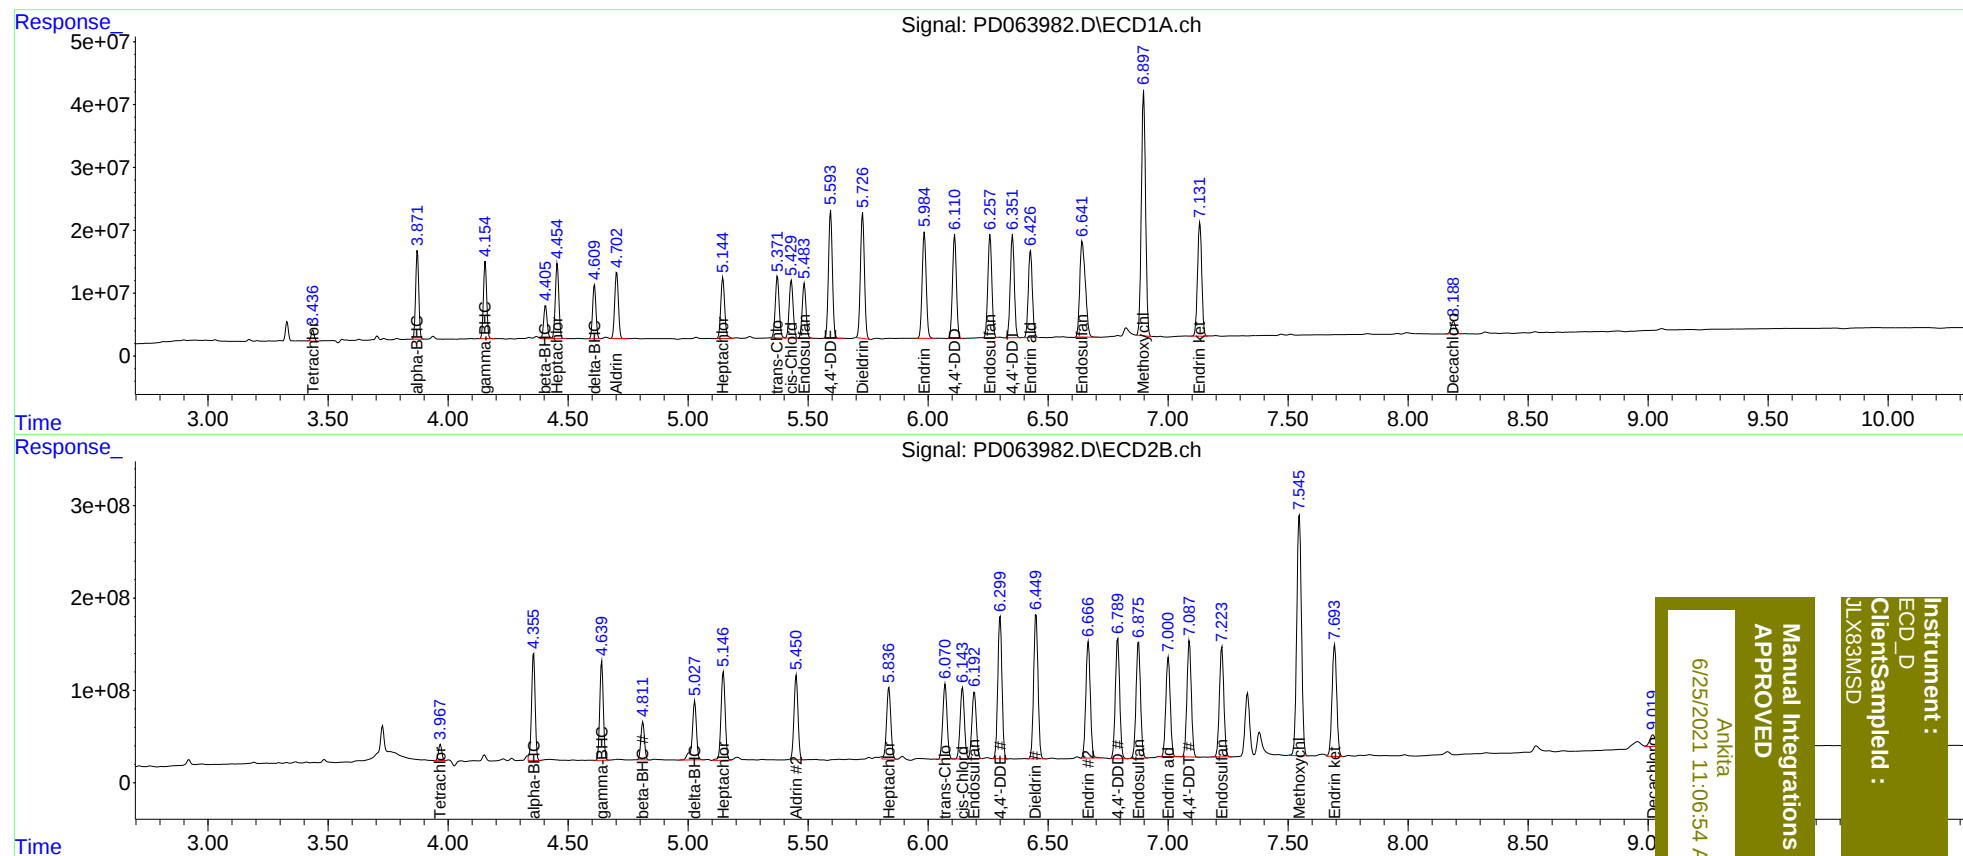

Manual Integrations
APPROVED

Ankita
6/25/2021 11:06:54 AM

Instrument :
ECD_D
Client Sample :
JLX83MSD