

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
 Data File : PD063986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2021 12:29
 Operator : AR\AJ
 Sample : M2682-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BGD71

Manual Integrations
 APPROVED

Ankita
 6/25/2021 11:07:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 09:07:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.969	15122870	144.3E6	9.728	9.110
27)	SA Decachlor...	8.187	9.018	41048051	307.8E6	23.714	22.196m
Target Compounds							
3)	MA gamma-BHC...	4.160	4.620	9235634	37122847	4.058	1.627m#
12)	B 4,4'-DDE	5.615	6.290	6266034	30733644	3.174	1.521m#
16)	A 4,4'-DDD	6.111	6.785	1454459	67870140	0.881m	4.032 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062421\
Data File : PD063986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2021 12:29
Operator : AR\AJ
Sample : M2682-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 09:07:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

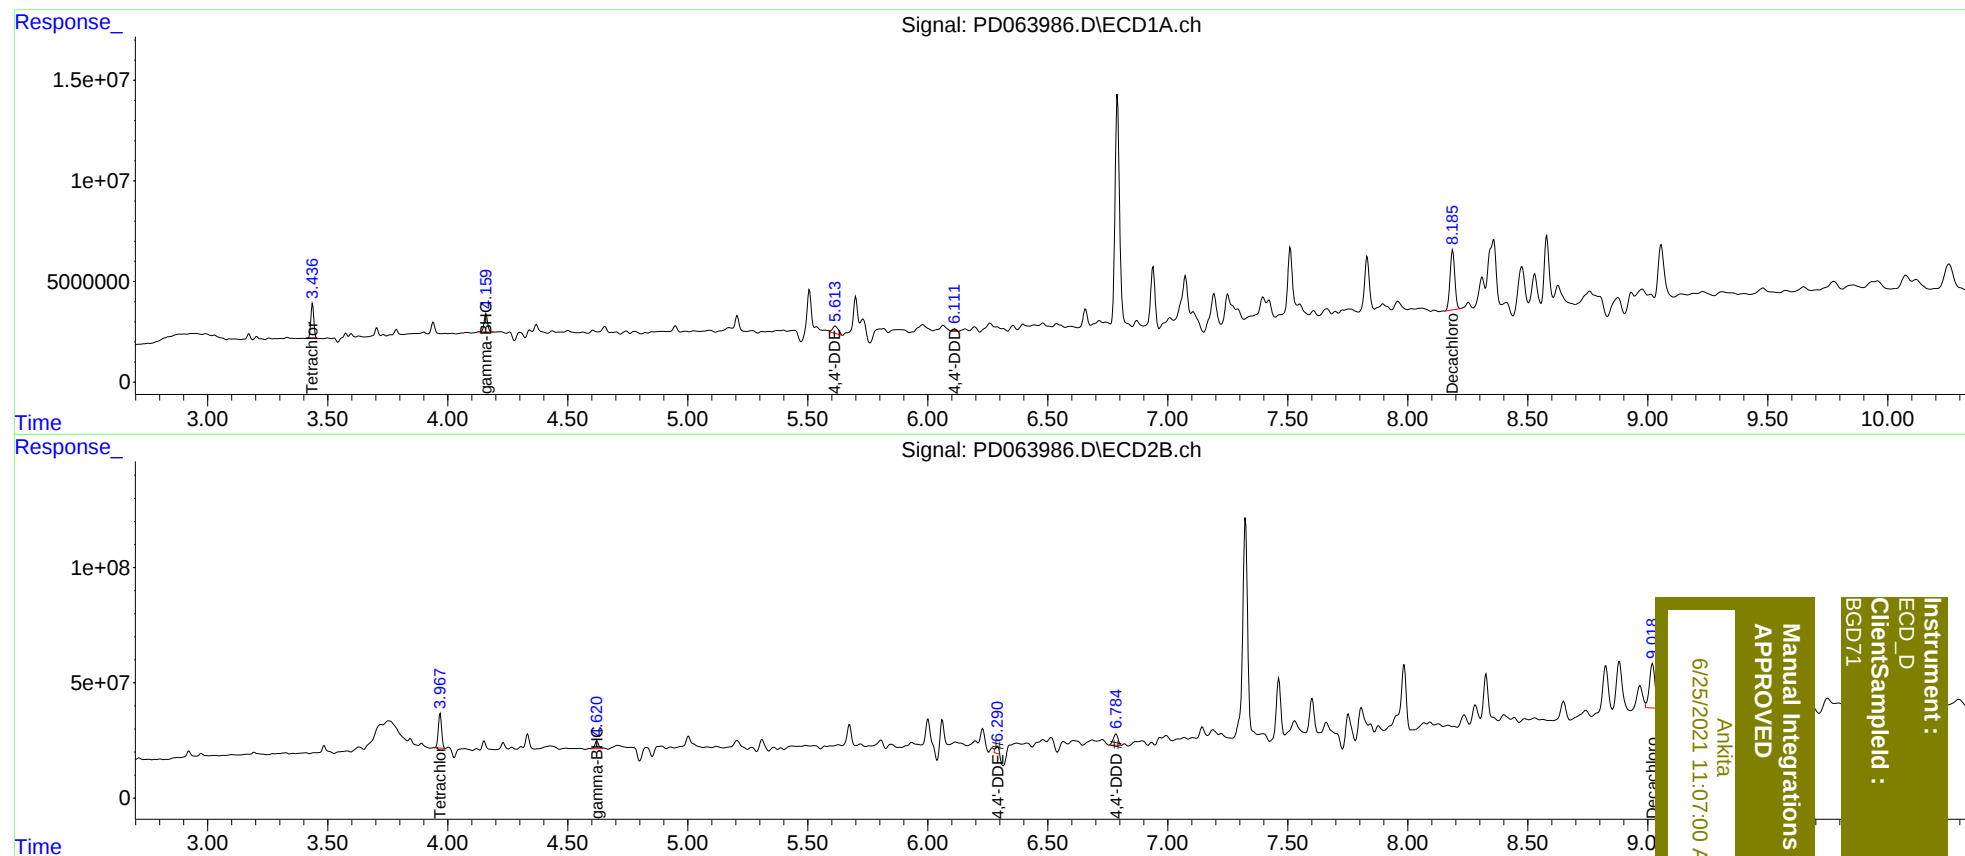

Manual Integrations
APPROVED

Ankita
6/25/2021 11:07:00 AM

Instrument :
ECD_D
Client Sampled :
BGD71