

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 18:14
 Operator : AR\AJ
 Sample : PB153684BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB153683BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:24:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	40309242	20429105	18.923	18.830
28)	SA Decachlor...	9.084	7.910	47716986	20208017	18.835	20.667
Target Compounds							
7)	B delta-BHC	4.773	0.000	2833415	0	0.852	N.D. #
8)	B Heptachlo...	5.690	0.000	1072763	0	0.333	N.D. #
9)	A Endosulfan I	6.068f	0.000	112808	0	0.038	N.D. #
10)	B gamma-Chl...	5.976f	0.000	257184	0	0.080	N.D. #
11)	B alpha-Chl...	6.037	0.000	79951	0	0.025	N.D. #
13)	MA Dieldrin	6.368	0.000	93639	0	0.030	N.D. #
15)	B Endosulfa...	6.833f	0.000	193901	0	0.075	N.D. #
21)	B Endrin ke...	7.690f	0.000	823723	0	0.296	N.D. #
25)	Chlordane-3	5.976f	0.000	257184	0	0.495	N.D. #
26)	Chlordane-4	6.037	0.000	79951	0	0.127	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 18:14
Operator : AR\AJ
Sample : PB153684BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB153683BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:24:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

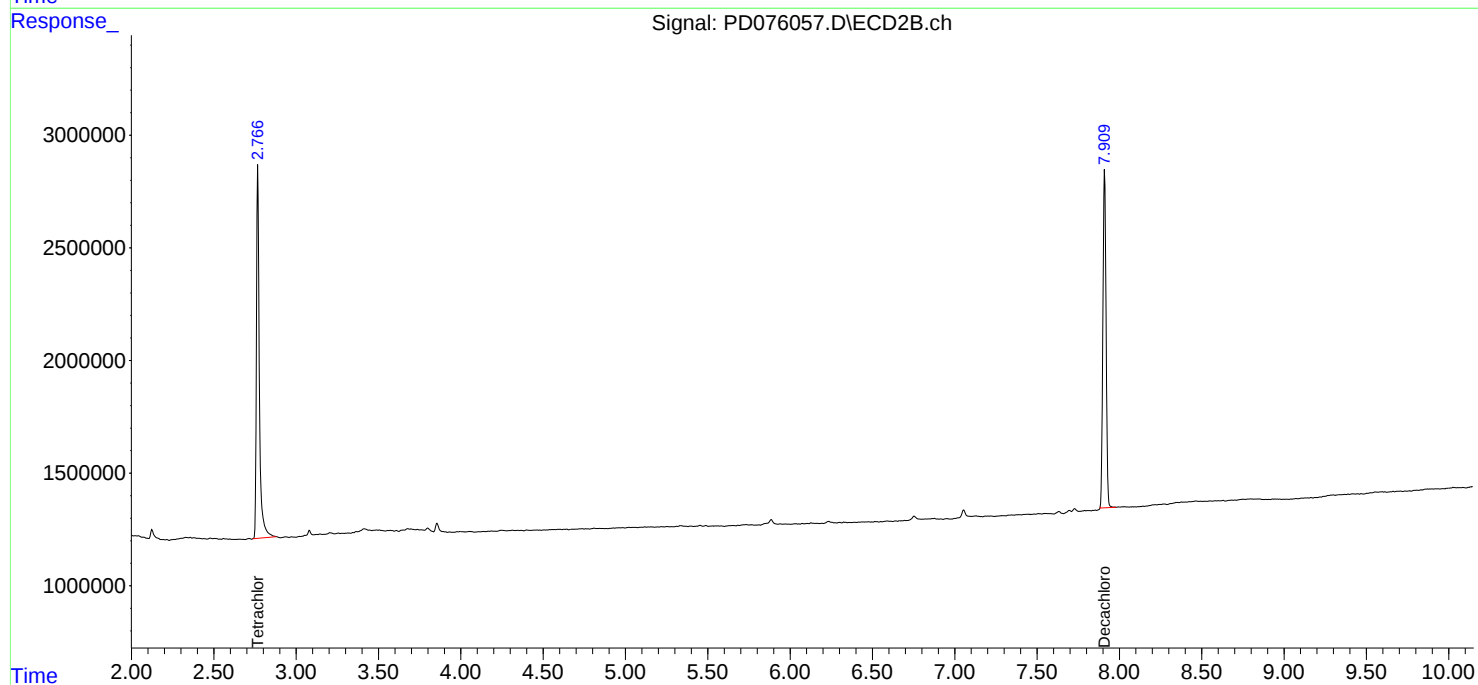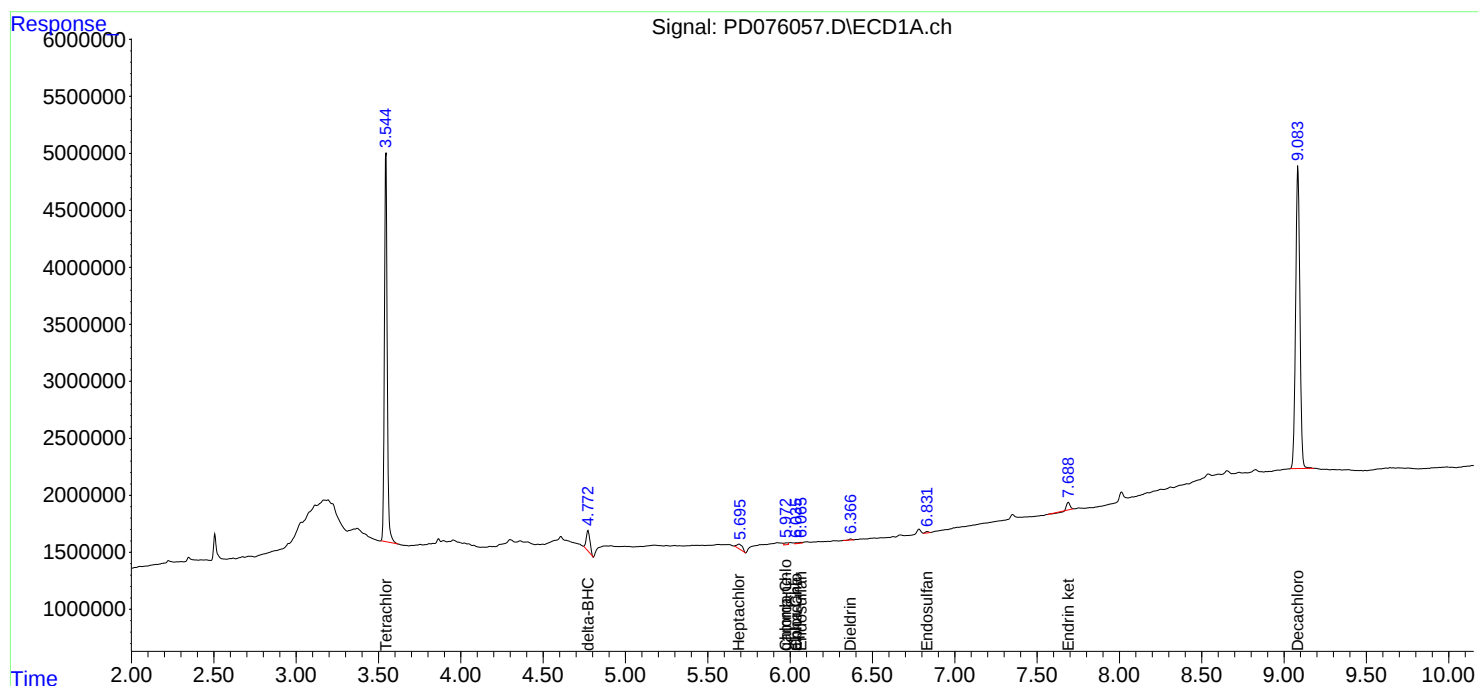


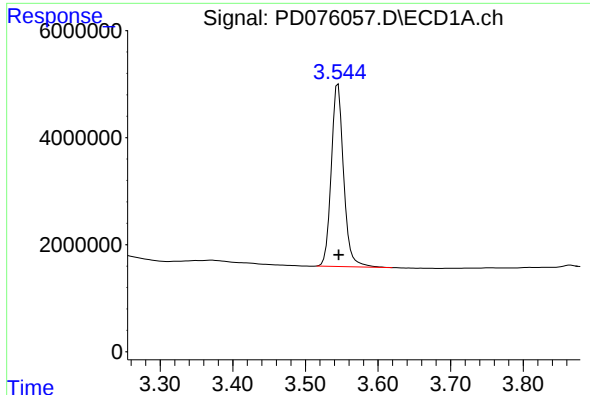

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 40309242
Conc: 18.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153683BL

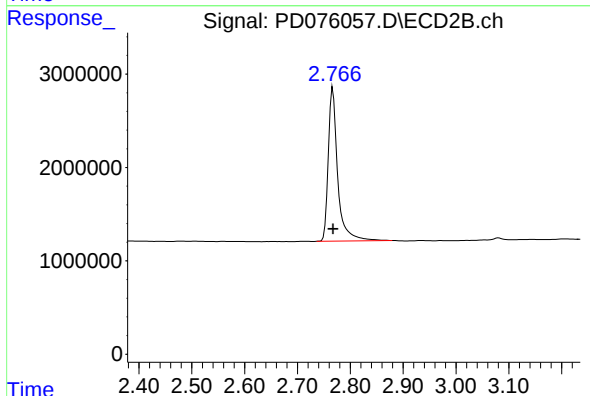


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 20429105
Conc: 18.83 ng/ml

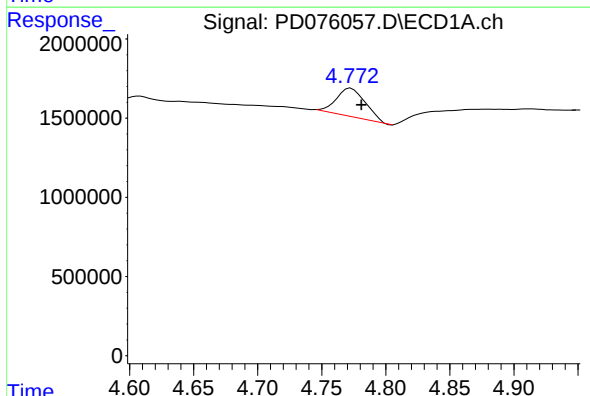


#7 delta-BHC

R.T.: 4.773 min
Delta R.T.: -0.008 min
Response: 2833415
Conc: 0.85 ng/ml

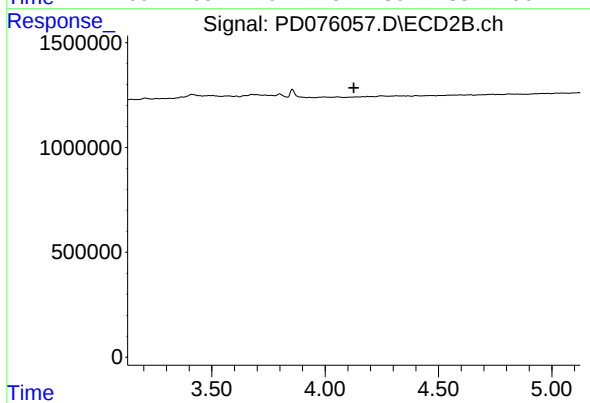

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

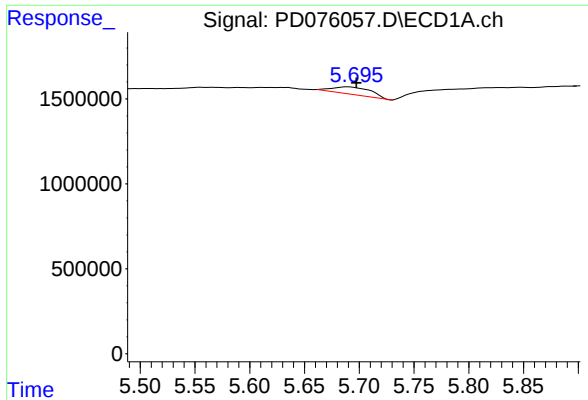

#8 Heptachlor epoxide


R.T.: 5.690 min
Delta R.T.: -0.007 min
Response: 1072763
Conc: 0.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153683BL

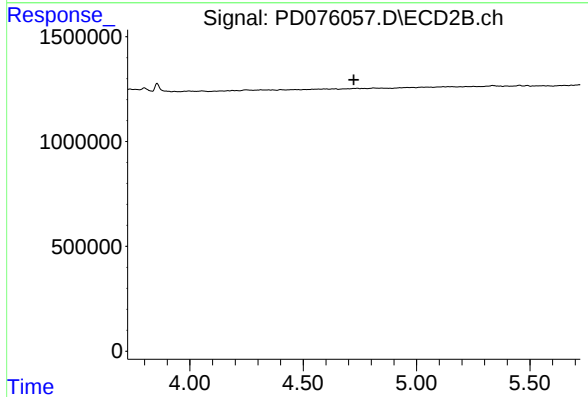


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

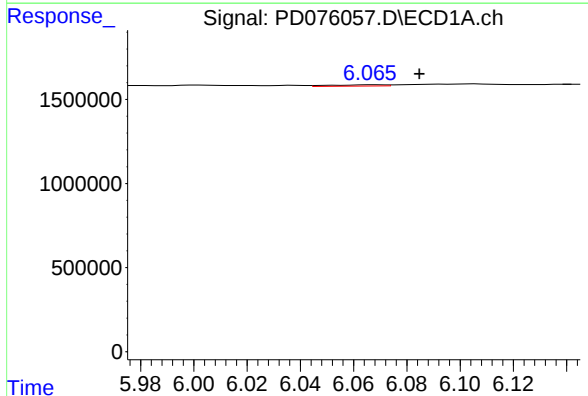


#9 Endosulfan I

R.T.: 6.068 min
Delta R.T.: -0.016 min
Response: 112808
Conc: 0.04 ng/ml

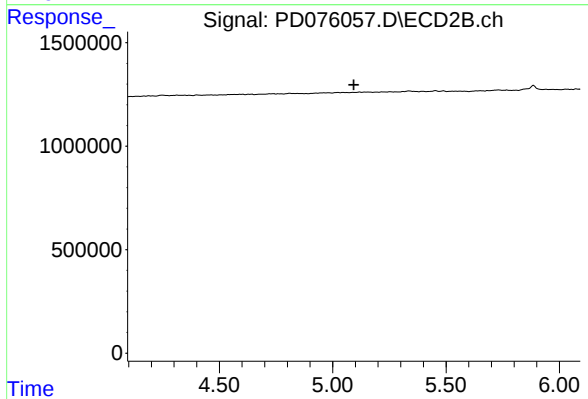

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

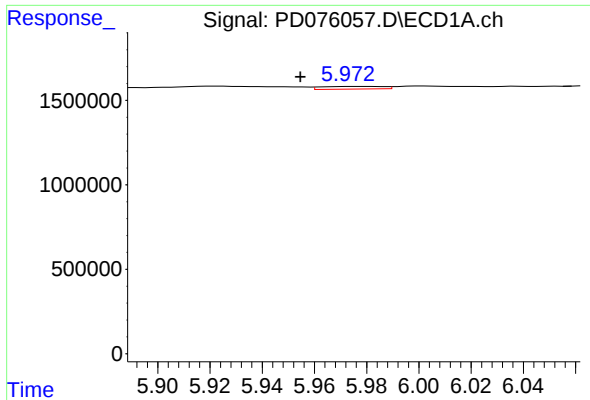

#10 gamma-Chlordane


R.T.: 5.976 min
Delta R.T.: 0.021 min
Response: 257184
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153683BL

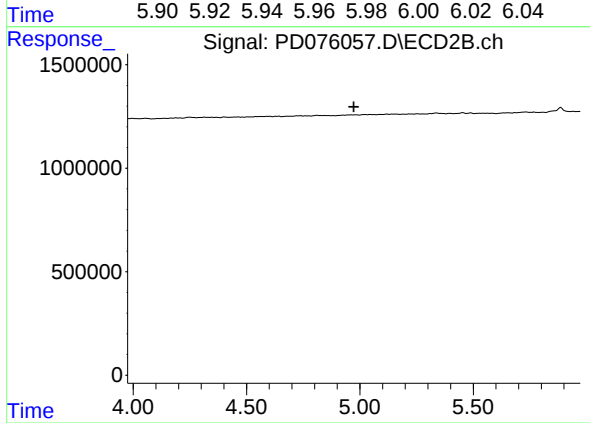


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

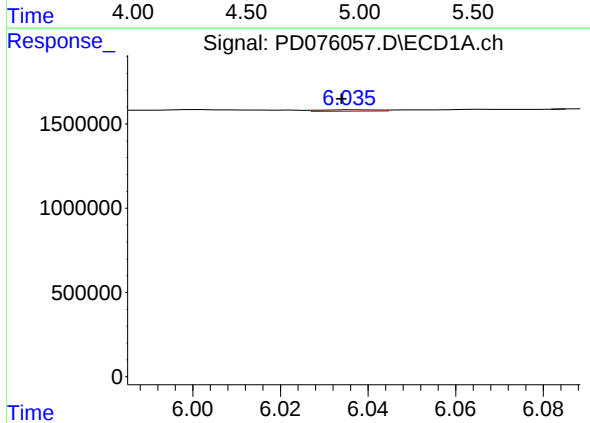


#11 alpha-Chlordane

R.T.: 6.037 min
Delta R.T.: 0.003 min
Response: 79951
Conc: 0.02 ng/ml

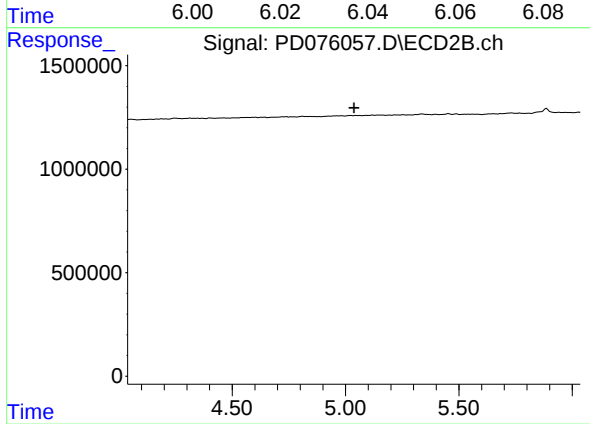

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

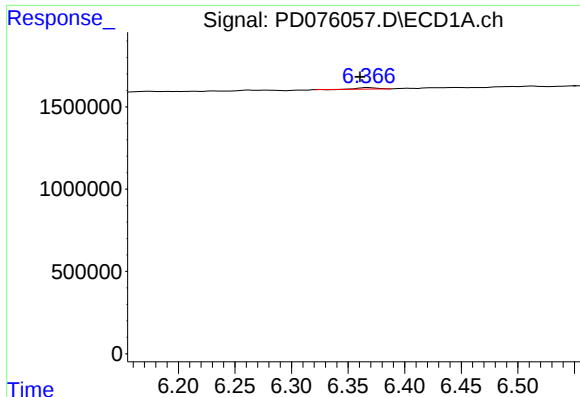

#13 Dieldrin


R.T.: 6.368 min
Delta R.T.: 0.007 min
Response: 93639
Conc: 0.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153683BL

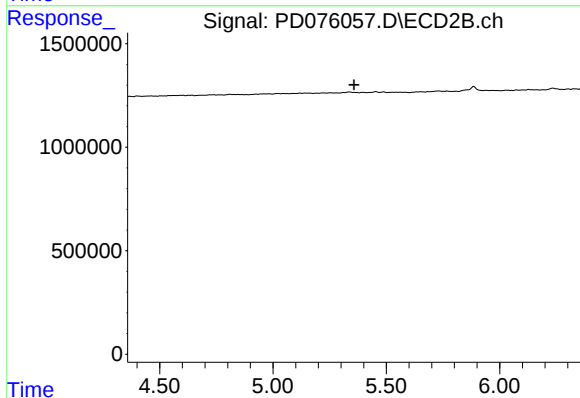


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

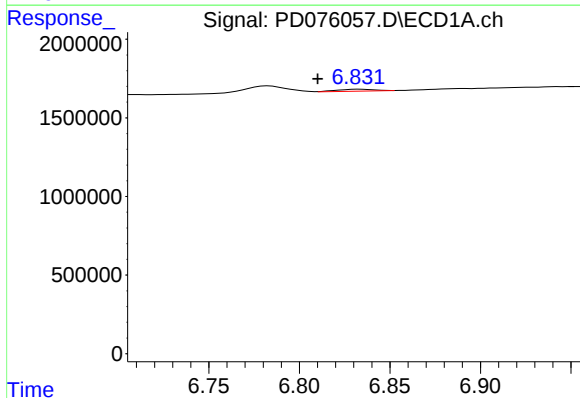


#15 Endosulfan II

R.T.: 6.833 min
Delta R.T.: 0.022 min
Response: 193901
Conc: 0.08 ng/ml

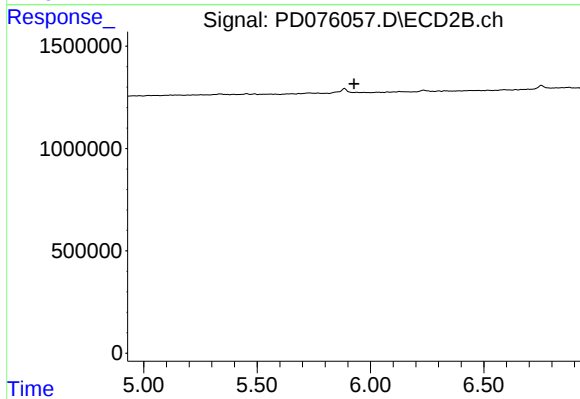

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

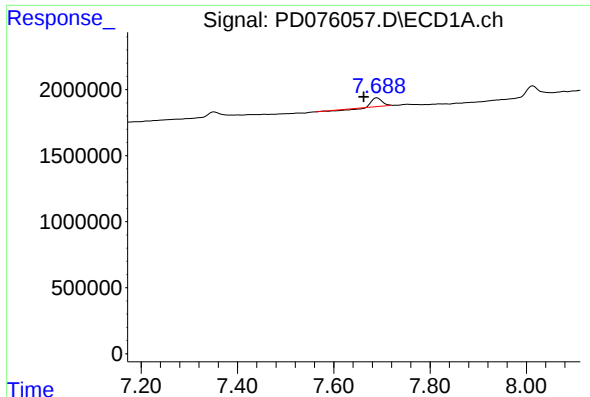

#21 Endrin ketone


R.T.: 7.690 min
Delta R.T.: 0.027 min
Response: 823723
Conc: 0.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153683BL

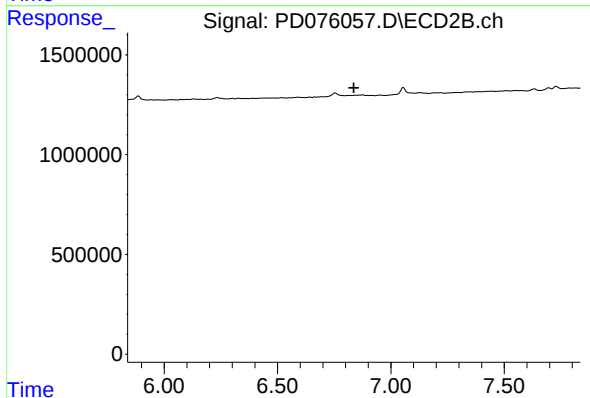


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

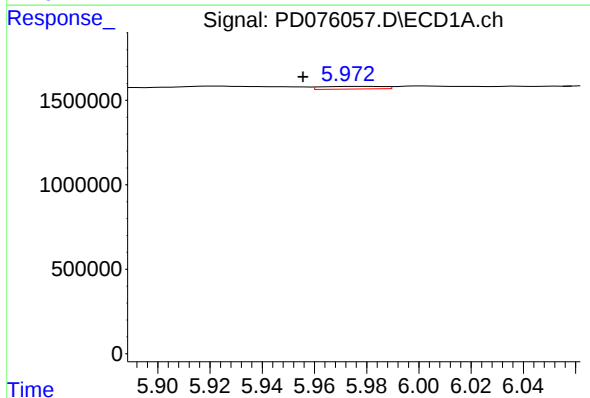


#25 Chlordane-3

R.T.: 5.976 min
Delta R.T.: 0.020 min
Response: 257184
Conc: 0.50 ng/ml

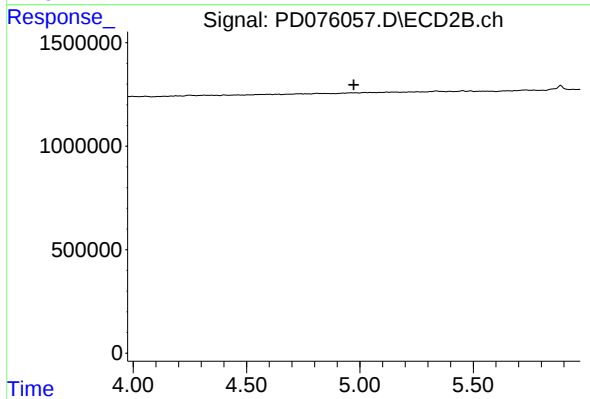

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

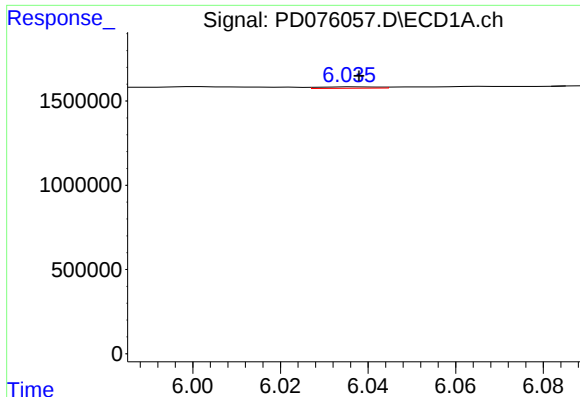

#26 Chlordane-4


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 79951
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153683BL

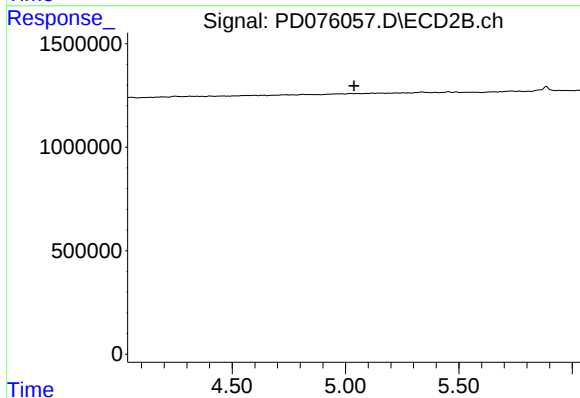


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

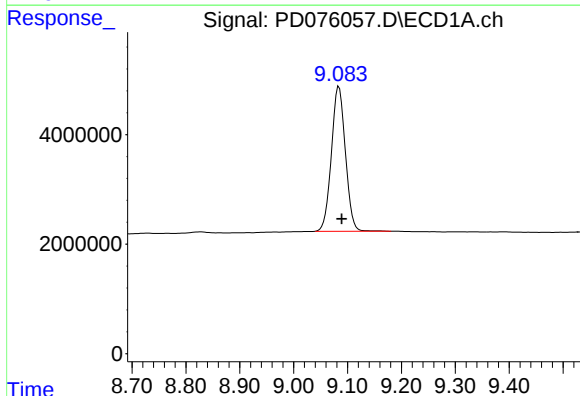

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.005 min
Response: 47716986
Conc: 18.84 ng/ml

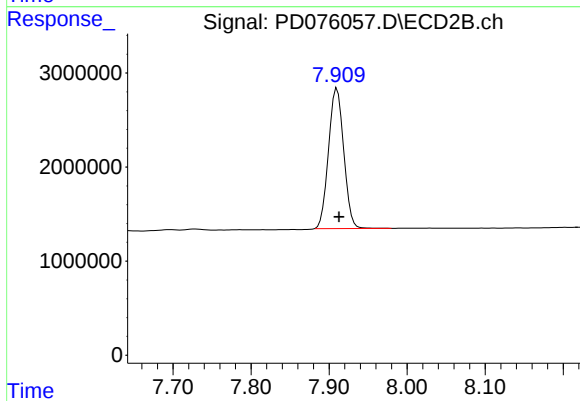

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.002 min
Response: 20208017
Conc: 20.67 ng/ml