

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076060.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 18:55
 Operator : AR\AJ
 Sample : 03337-04
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-17

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:25:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	24426999	12801204	11.467	11.799
28)	SA Decachlor...	9.085	7.910	29974877	13351931	11.832	13.655
Target Compounds							
2)	A alpha-BHC	4.023f	0.000	802379	0	0.217	N.D. #
7)	B delta-BHC	4.770	0.000	1332313	0	0.401	N.D. #
8)	B Heptachlo...	5.691	0.000	937094	0	0.291	N.D. #
9)	A Endosulfan I	6.081	0.000	40178	0	0.013	N.D. #
10)	B gamma-Chl...	5.946	0.000	168196	0	0.052	N.D. #
11)	B alpha-Chl...	6.039	0.000	158063	0	0.049	N.D. #
15)	B Endosulfa...	6.783f	0.000	759749	0	0.294	N.D. #
21)	B Endrin ke...	7.689f	0.000	1315851	0	0.472	N.D. #
25)	Chlordane-3	5.946	0.000	168196	0	0.324	N.D. #
26)	Chlordane-4	6.039	0.000	158063	0	0.251	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076060.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 18:55
Operator : AR\AJ
Sample : 03337-04
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
WC-17

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:25:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

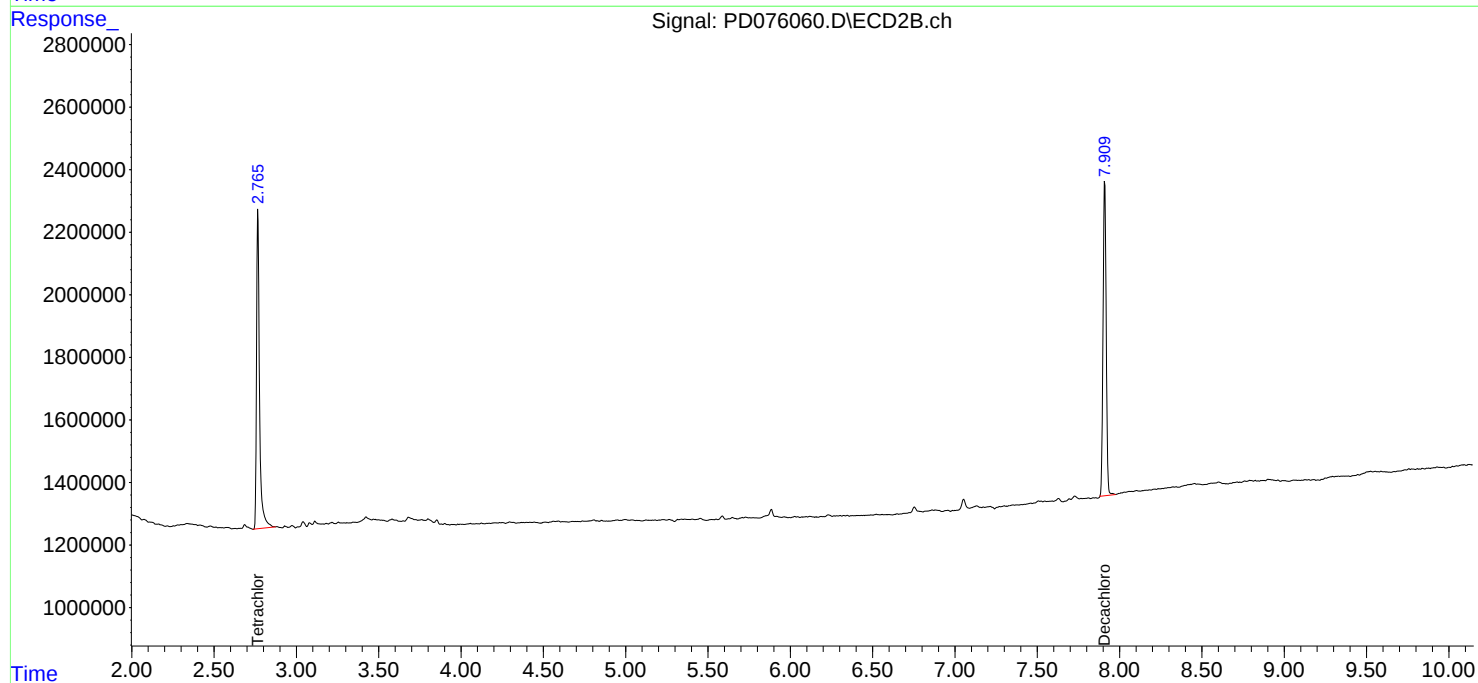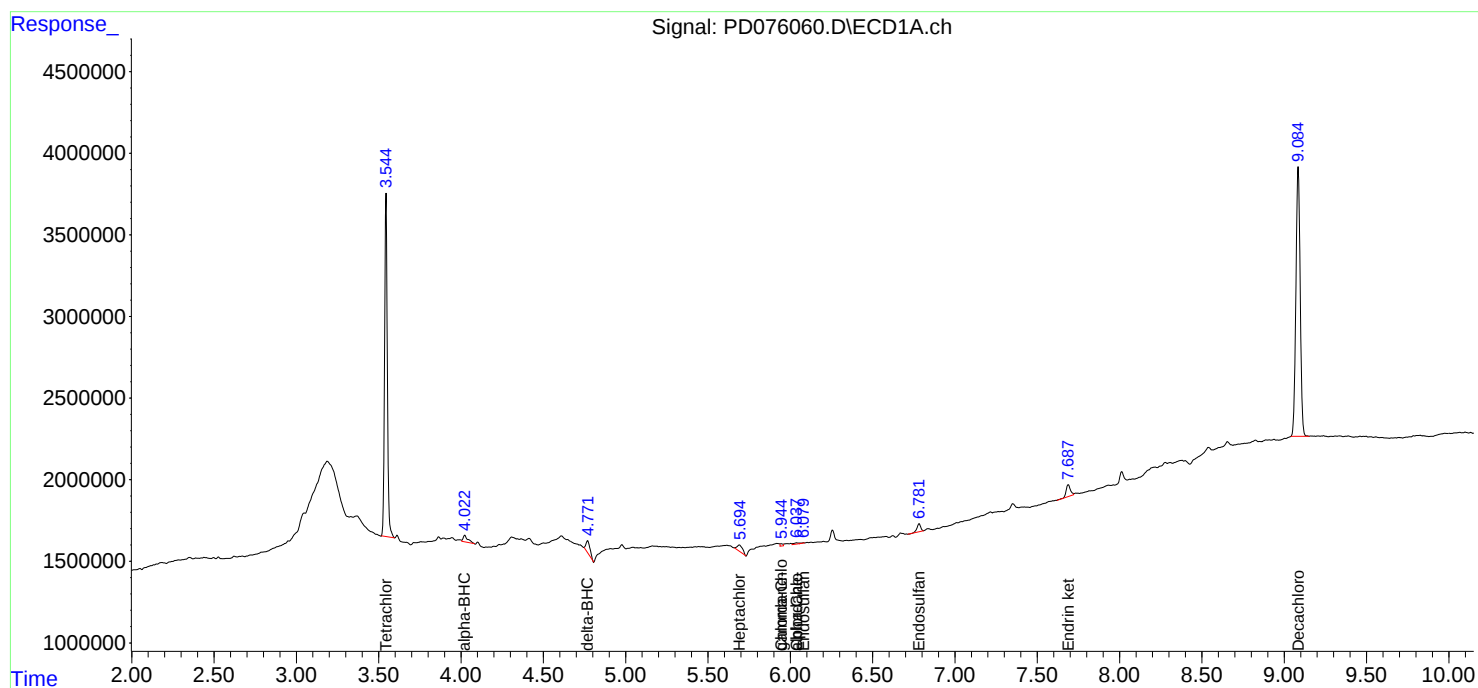


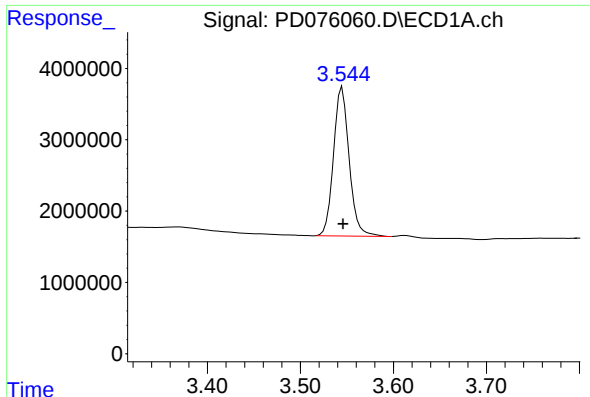

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: -0.001 min
Response: 24426999
Conc: 11.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-17

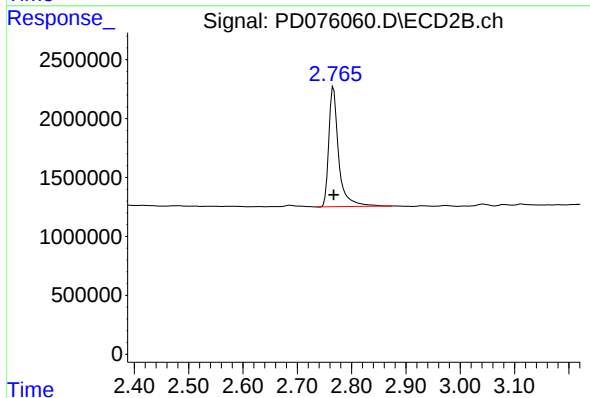


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 12801204
Conc: 11.80 ng/ml

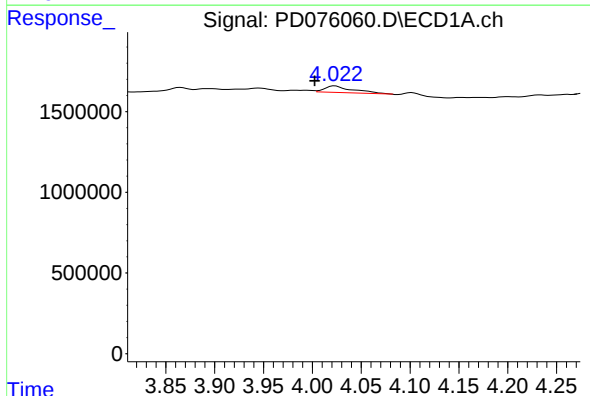


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.021 min
Response: 802379
Conc: 0.22 ng/ml

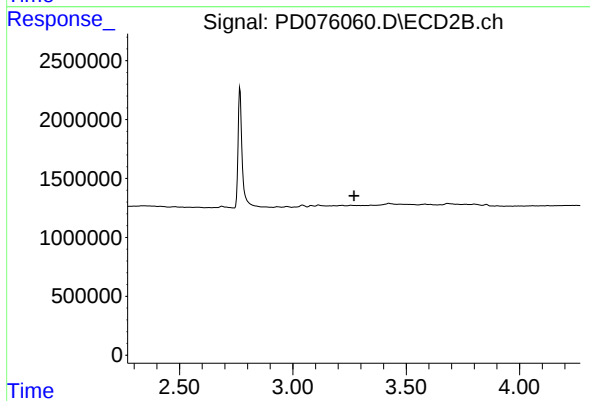

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.270 min
Response: 0
Conc: N.D.

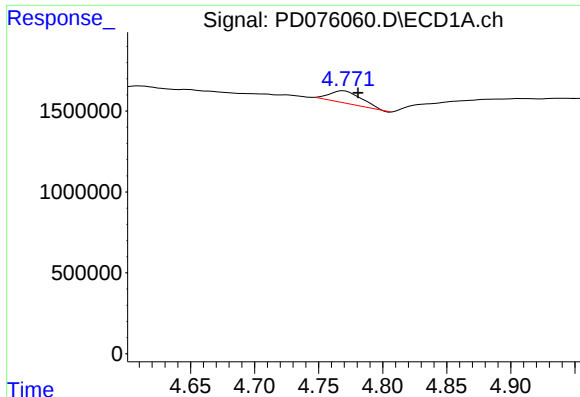

#7 delta-BHC


R.T.: 4.770 min
Delta R.T.: -0.011 min
Response: 1332313
Conc: 0.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-17

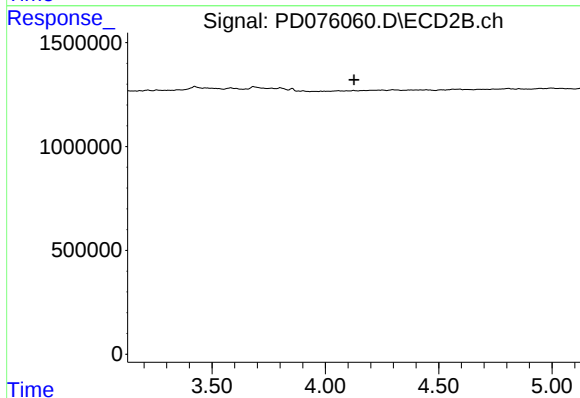


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

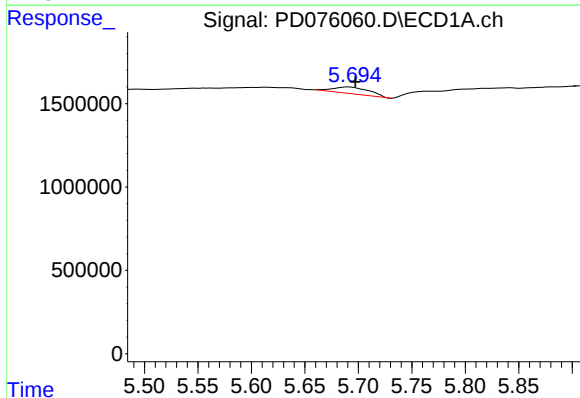


#8 Heptachlor epoxide

R.T.: 5.691 min
Delta R.T.: -0.006 min
Response: 937094
Conc: 0.29 ng/ml

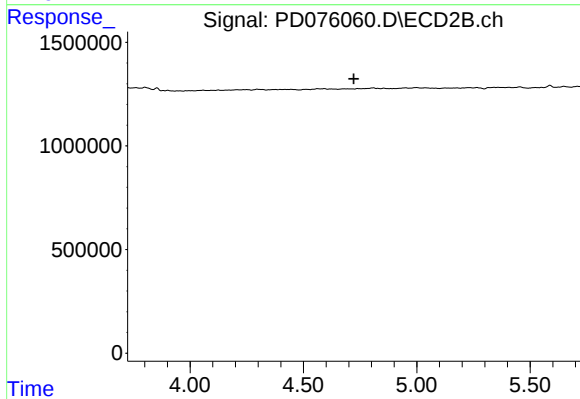

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

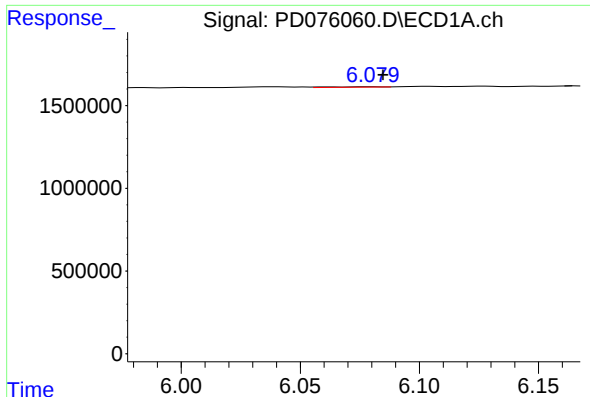

#9 Endosulfan I


R.T.: 6.081 min
Delta R.T.: -0.004 min
Response: 40178
Conc: 0.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-17

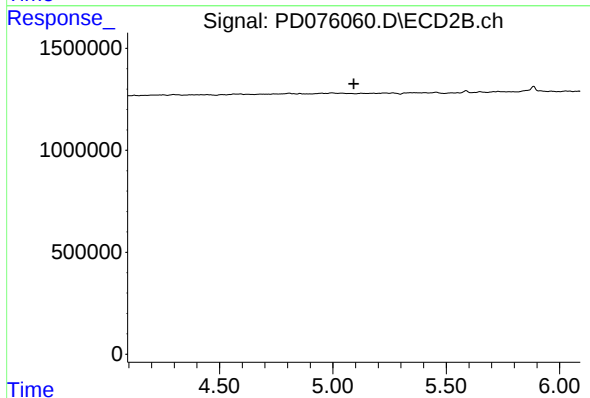


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

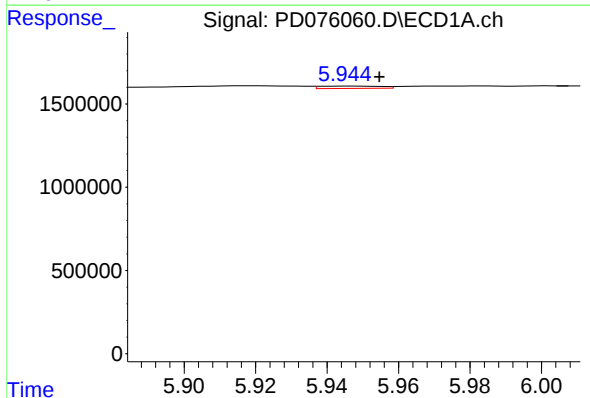


#10 gamma-Chlordane

R.T.: 5.946 min
Delta R.T.: -0.009 min
Response: 168196
Conc: 0.05 ng/ml

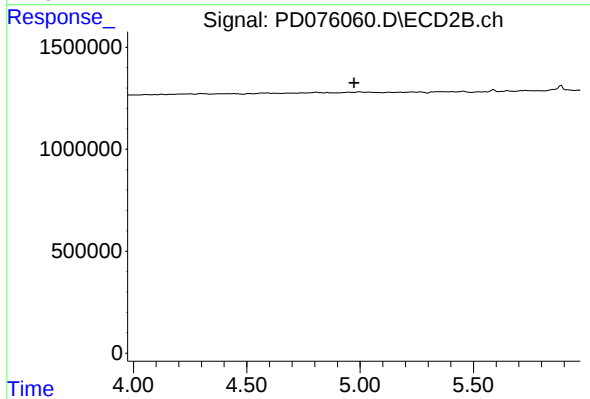

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

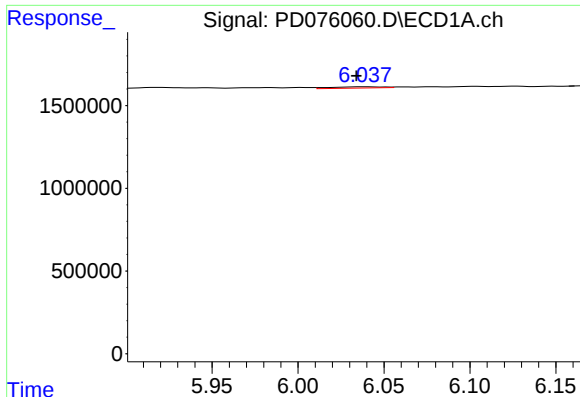

#11 alpha-Chlordane


R.T.: 6.039 min
Delta R.T.: 0.005 min
Response: 158063
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-17

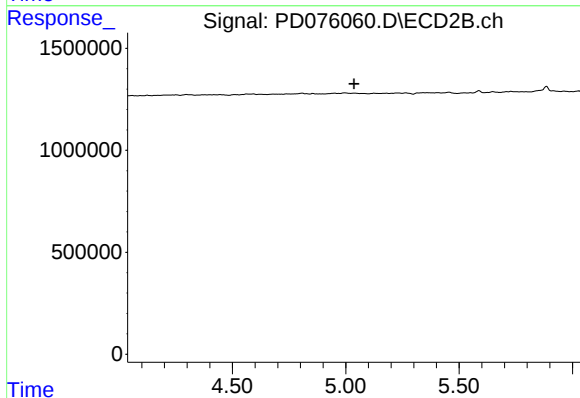


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

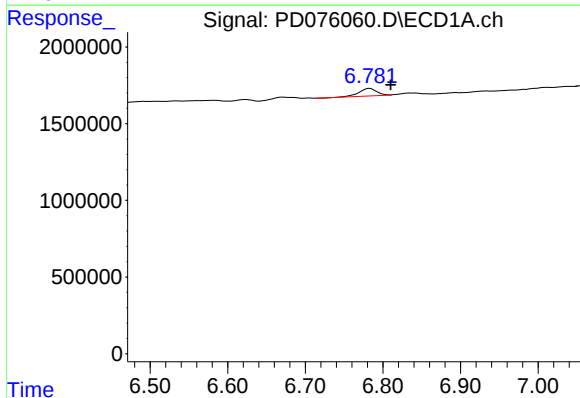


#15 Endosulfan II

R.T.: 6.783 min
Delta R.T.: -0.027 min
Response: 759749
Conc: 0.29 ng/ml

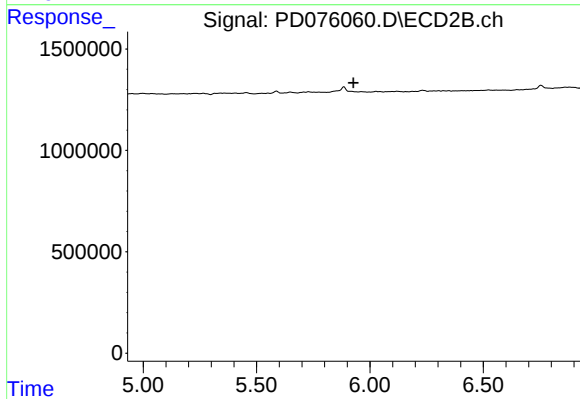

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

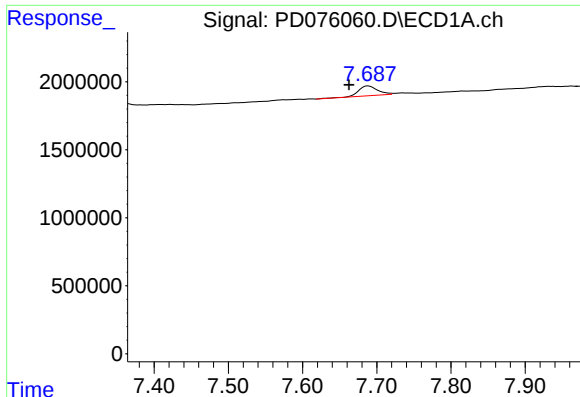

#21 Endrin ketone


R.T.: 7.689 min
Delta R.T.: 0.026 min
Response: 1315851
Conc: 0.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-17

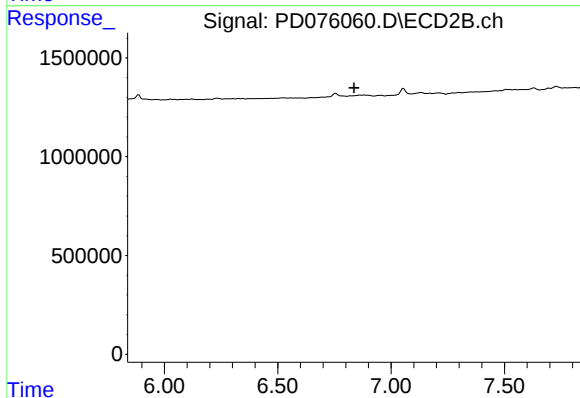


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

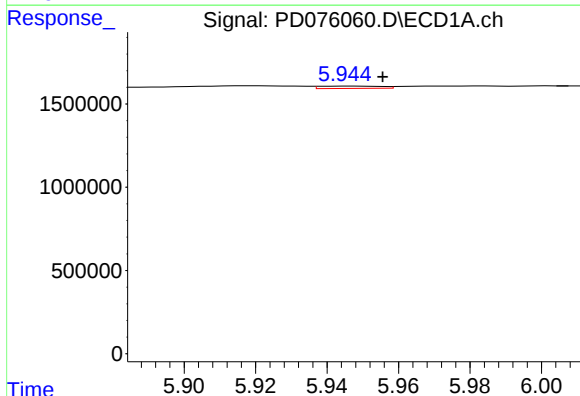


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: -0.010 min
Response: 168196
Conc: 0.32 ng/ml

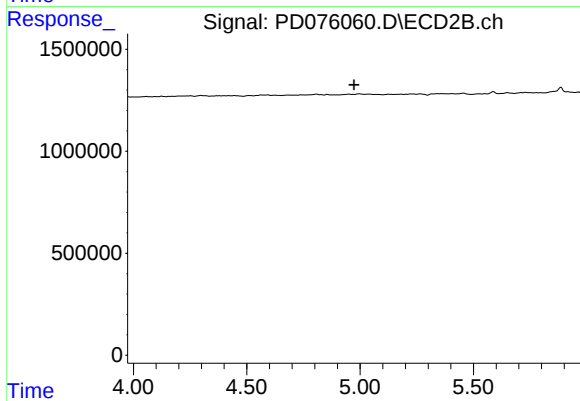

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

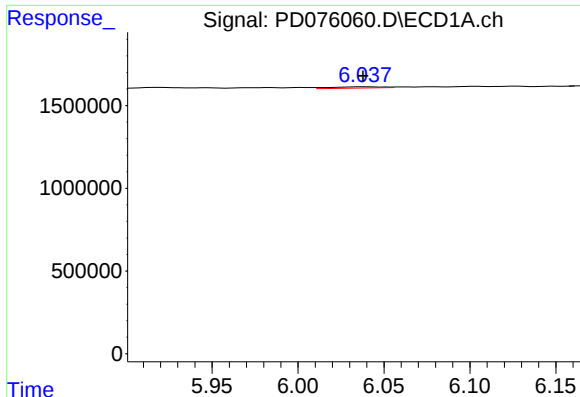

#26 Chlordane-4


R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 158063
Conc: 0.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-17

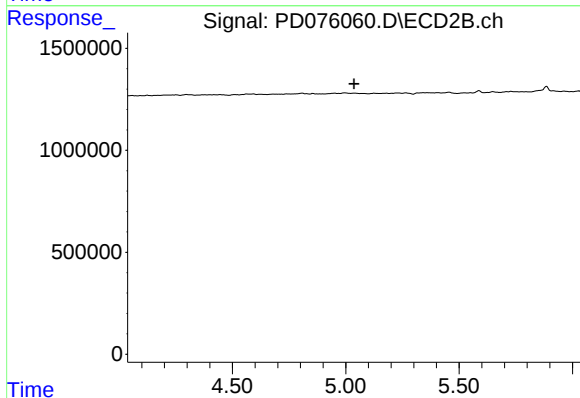


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

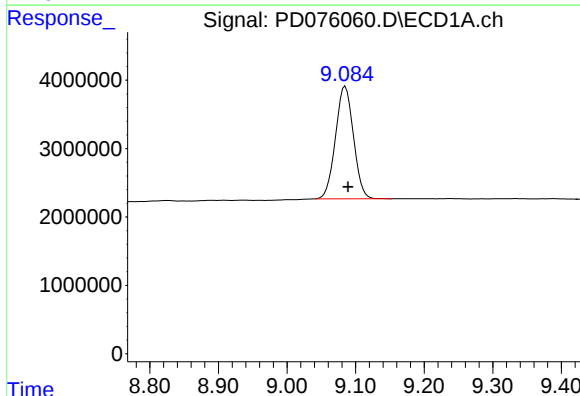

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.004 min
Response: 29974877
Conc: 11.83 ng/ml

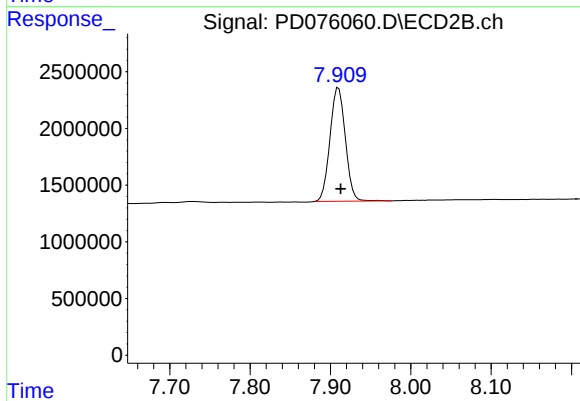

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.002 min
Response: 13351931
Conc: 13.66 ng/ml