

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 19:22
 Operator : AR\AJ
 Sample : 03337-10
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:26:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	24169337	12400394	11.346	11.430
28)	SA Decachlor...	9.084	7.910	30205545	12977502	11.923	13.272
Target Compounds							
7)	B delta-BHC	4.770	0.000	1360283	0	0.409	N.D. #
8)	B Heptachlo...	5.690	0.000	961939	0	0.299	N.D. #
9)	A Endosulfan I	6.095	0.000	94437	0	0.031	N.D. #
10)	B gamma-Chl...	5.962	0.000	393013	0	0.122	N.D. #
11)	B alpha-Chl...	6.040	0.000	339932	0	0.105	N.D. #
15)	B Endosulfa...	6.830f	0.000	145535	0	0.056	N.D. #
17)	MA 4,4'-DDT	7.053	0.000	118617	0	0.052	N.D. #
21)	B Endrin ke...	7.689f	0.000	711722	0	0.255	N.D. #
25)	Chlordane-3	5.962	0.000	393013	0	0.757	N.D. #
26)	Chlordane-4	6.040	0.000	339932	0	0.539	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 19:22
Operator : AR\AJ
Sample : 03337-10
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
WC-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:26:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

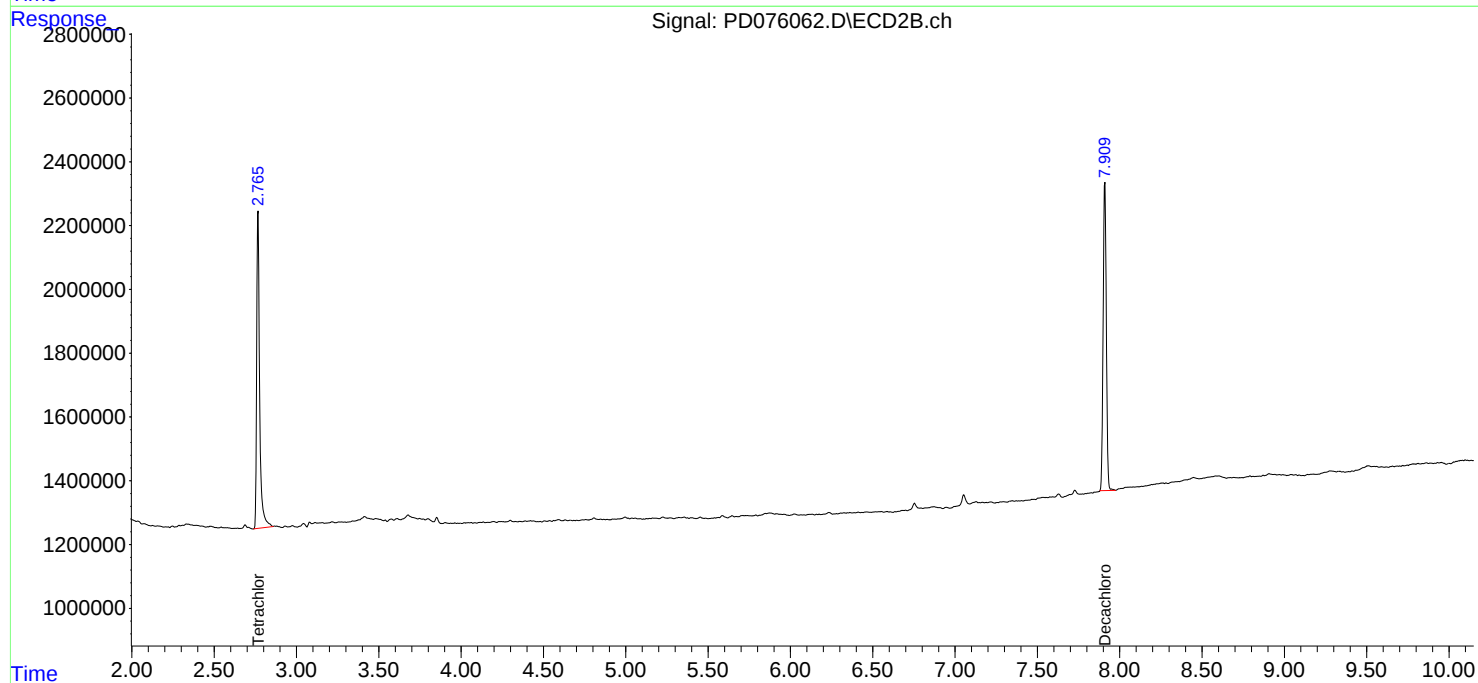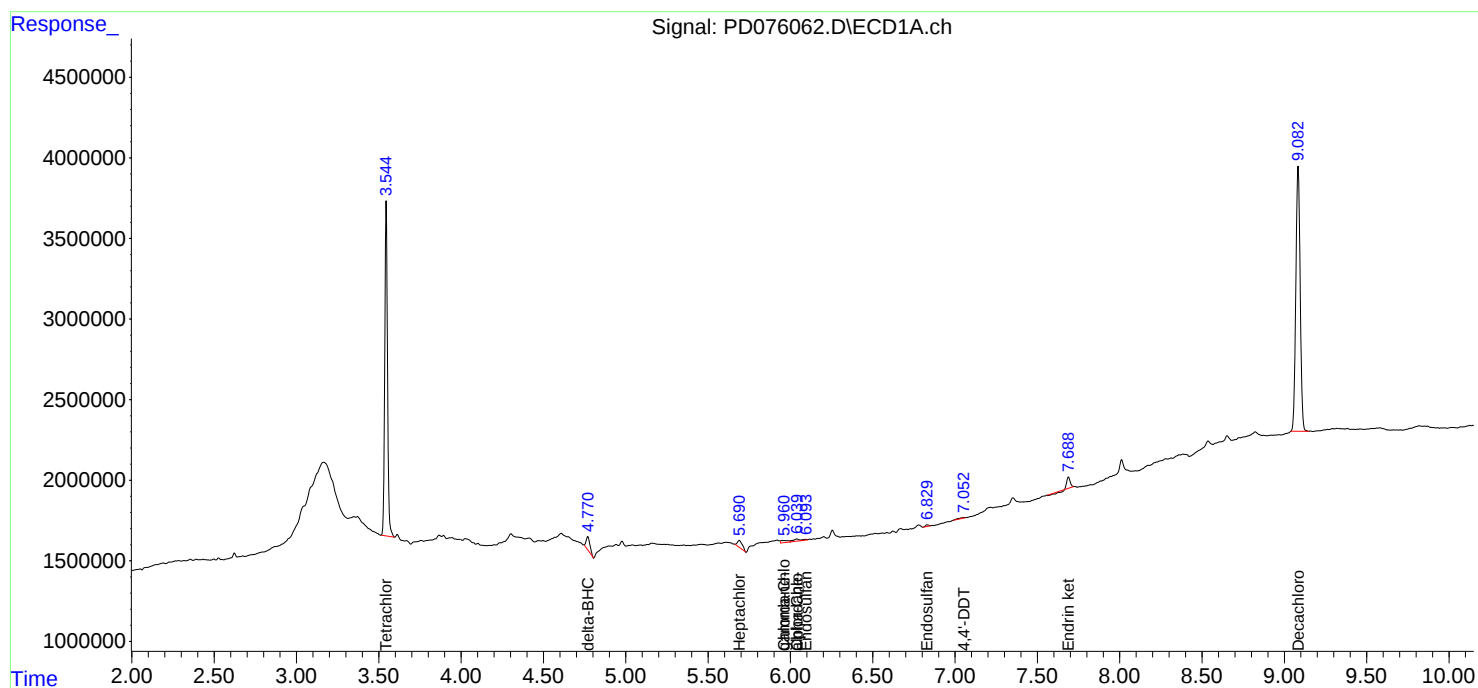


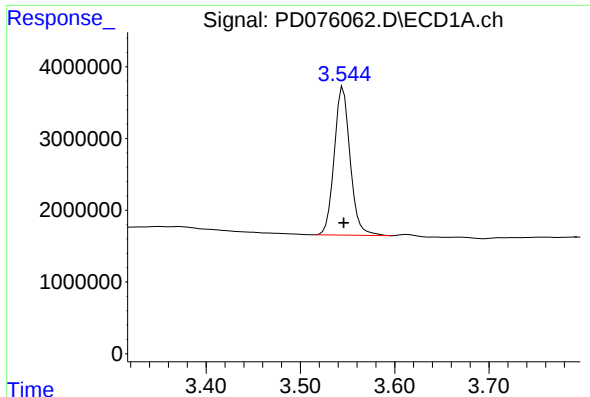

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 24169337
Conc: 11.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-8

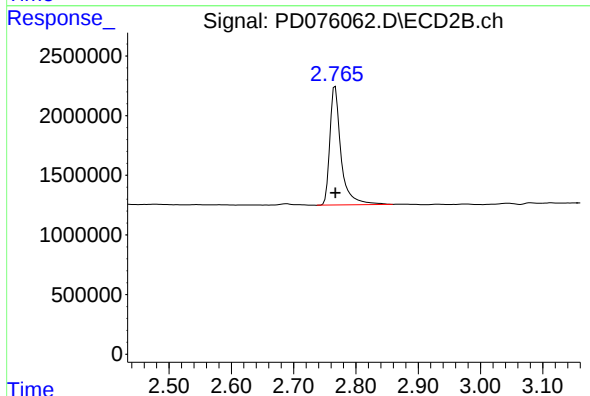


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 12400394
Conc: 11.43 ng/ml

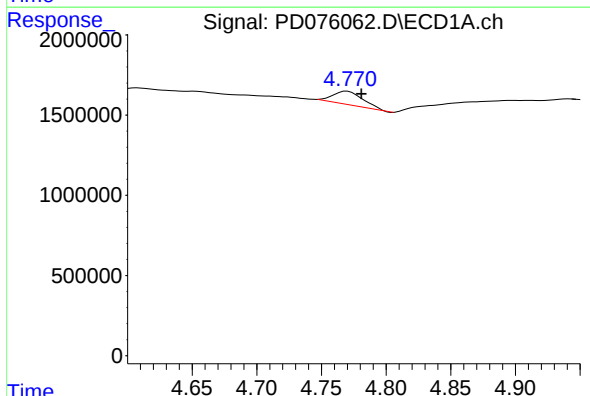


#7 delta-BHC

R.T.: 4.770 min
Delta R.T.: -0.011 min
Response: 1360283
Conc: 0.41 ng/ml

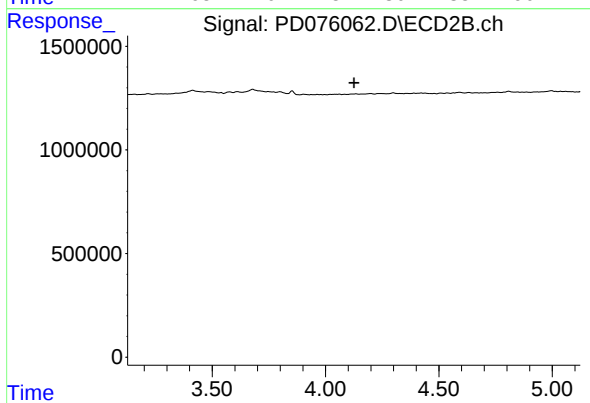

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

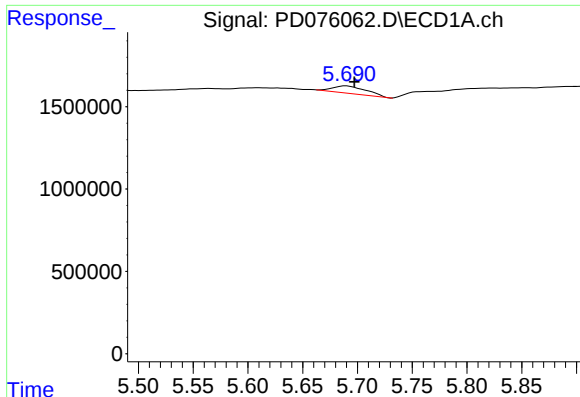

#8 Heptachlor epoxide


R.T.: 5.690 min
Delta R.T.: -0.007 min
Response: 961939
Conc: 0.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-8

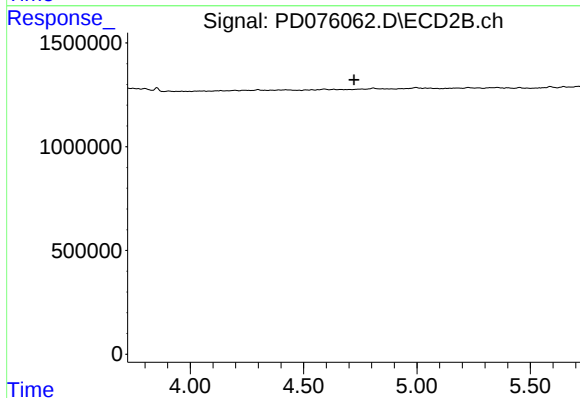


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

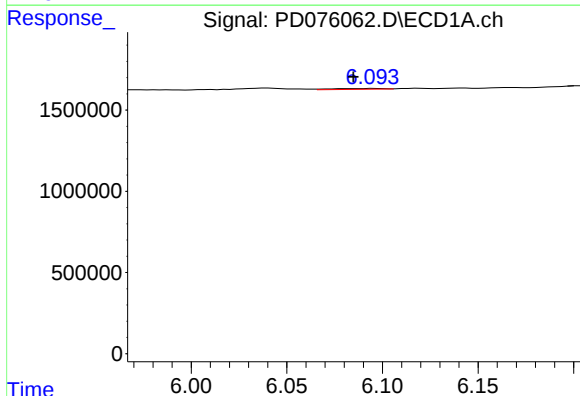


#9 Endosulfan I

R.T.: 6.095 min
Delta R.T.: 0.011 min
Response: 94437
Conc: 0.03 ng/ml

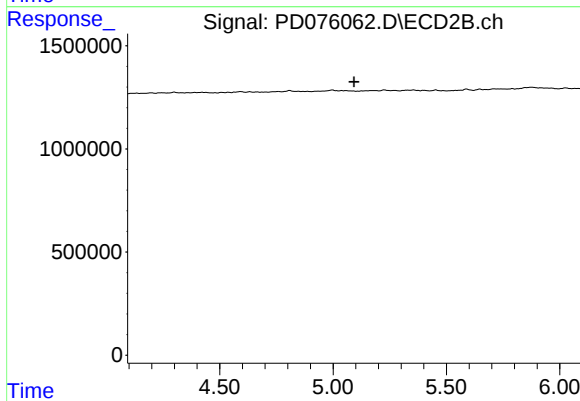

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

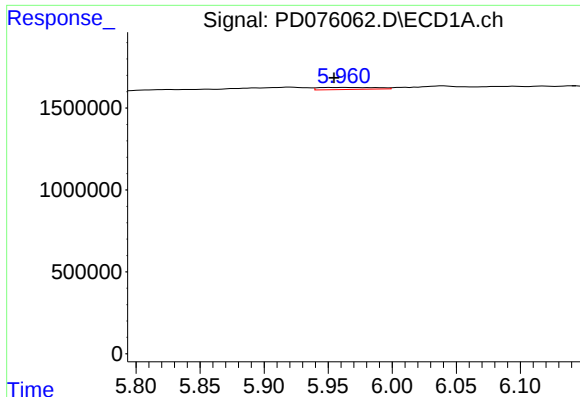

#10 gamma-Chlordane


R.T.: 5.962 min
Delta R.T.: 0.007 min
Response: 393013
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-8

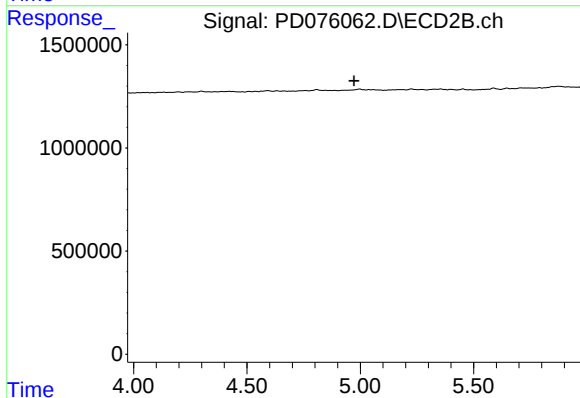


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

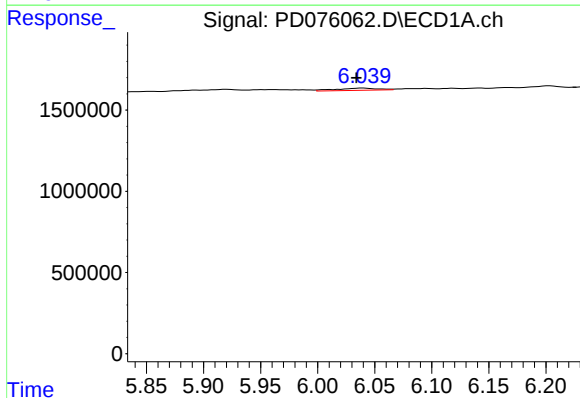


#11 alpha-Chlordane

R.T.: 6.040 min
Delta R.T.: 0.006 min
Response: 339932
Conc: 0.11 ng/ml

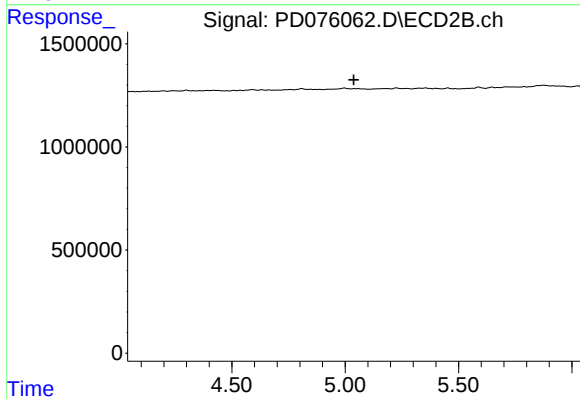

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

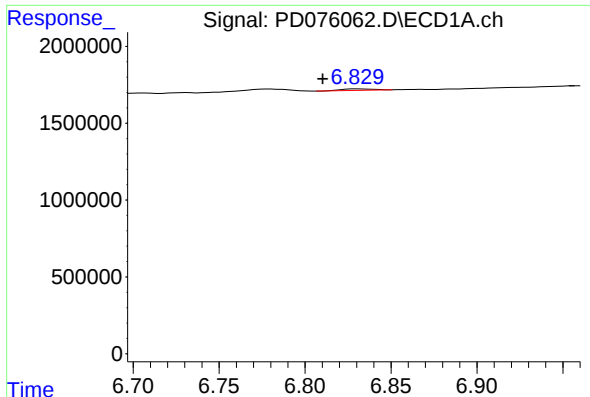

#15 Endosulfan II


R.T.: 6.830 min
Delta R.T.: 0.020 min
Response: 145535
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-8

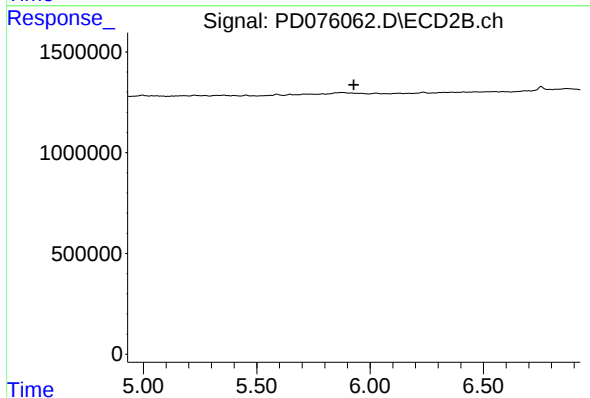


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

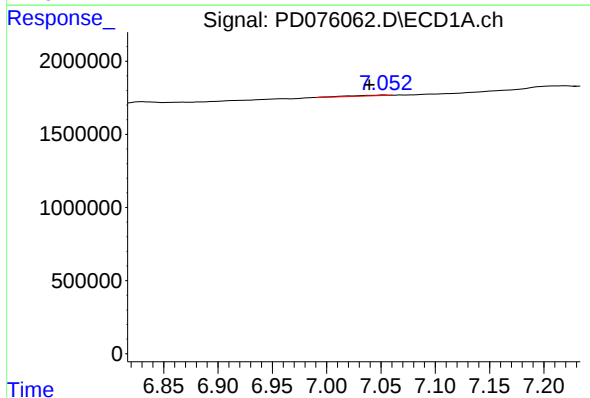


#17 4,4'-DDT

R.T.: 7.053 min
Delta R.T.: 0.014 min
Response: 118617
Conc: 0.05 ng/ml

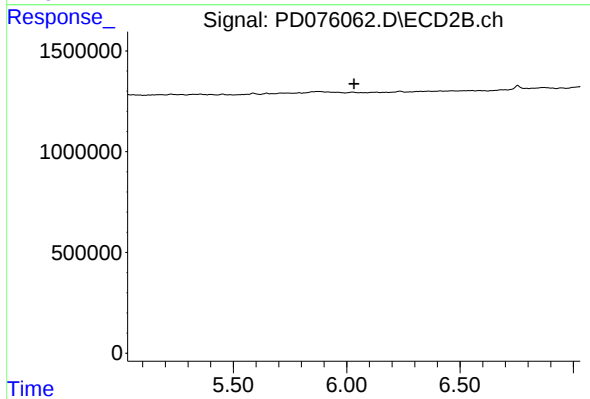

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

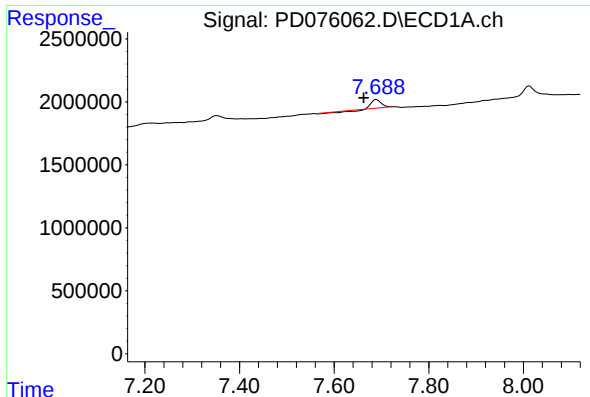

#21 Endrin ketone


R.T.: 7.689 min
Delta R.T.: 0.027 min
Response: 711722
Conc: 0.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-8

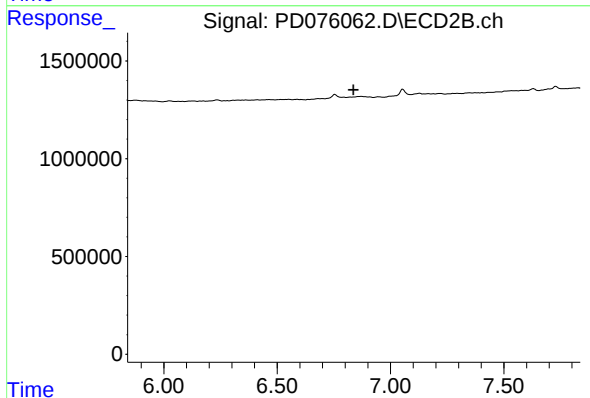


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

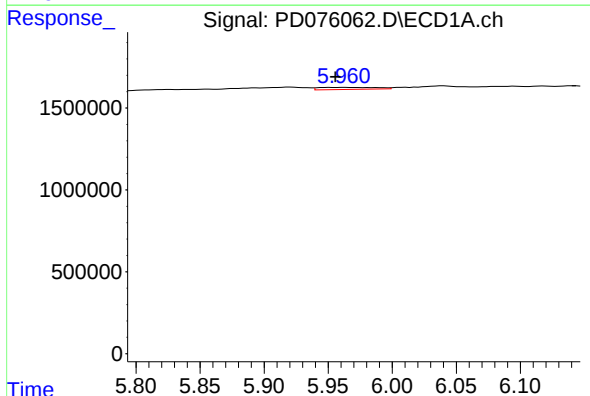


#25 Chlordane-3

R.T.: 5.962 min
Delta R.T.: 0.006 min
Response: 393013
Conc: 0.76 ng/ml

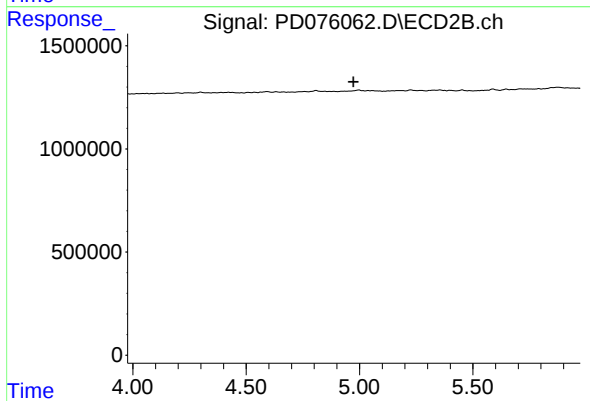

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

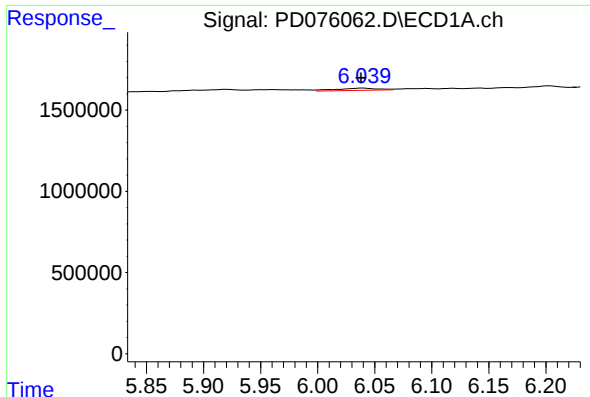

#26 Chlordane-4


R.T.: 6.040 min
Delta R.T.: 0.002 min
Response: 339932
Conc: 0.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-8

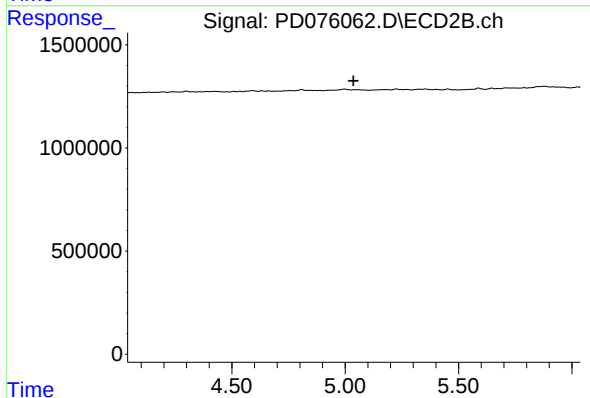


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.037 min
Response: 0
Conc: N.D.

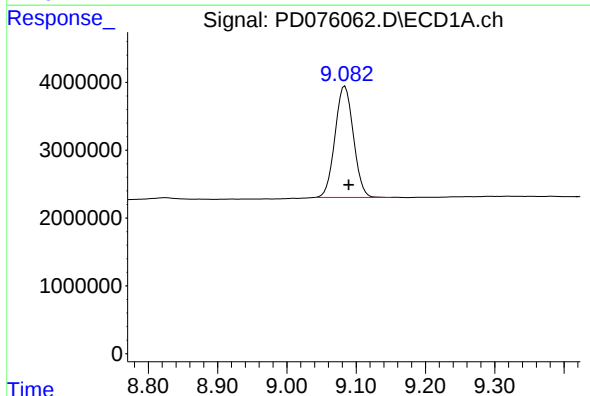

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.005 min
Response: 30205545
Conc: 11.92 ng/ml

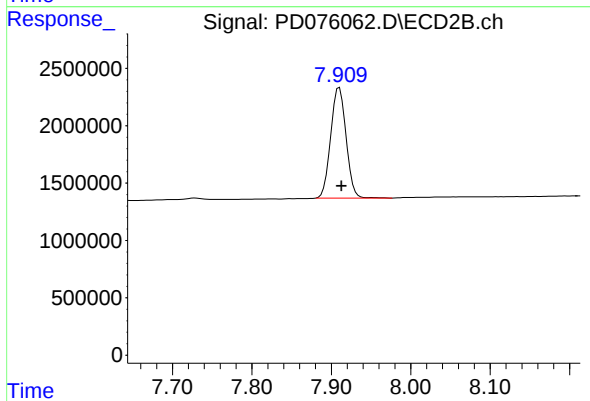

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.003 min
Response: 12977502
Conc: 13.27 ng/ml