

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 19:36
 Operator : AR\AJ
 Sample : 03337-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:27:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.766	23678958	12488014	11.116	11.510
28)	SA Decachlor...	9.085	7.911	30548657	13738221	12.059	14.050
Target Compounds							
2)	A alpha-BHC	4.023f	0.000	248161	0	0.067	N.D. #
7)	B delta-BHC	4.769	0.000	1304836	0	0.393	N.D. #
9)	A Endosulfan I	6.093	0.000	124641	0	0.042	N.D. #
10)	B gamma-Chl...	5.977f	0.000	432741	0	0.134	N.D. #
11)	B alpha-Chl...	6.005f	0.000	63896	0	0.020	N.D. #
15)	B Endosulfa...	6.783f	0.000	185440	0	0.072	N.D. #
17)	MA 4,4'-DDT	7.035	0.000	85307	0	0.038	N.D. #
21)	B Endrin ke...	7.689f	0.000	519100	0	0.186	N.D. #
25)	Chlordane-3	5.977f	0.000	432741	0	0.833	N.D. #
26)	Chlordane-4	6.066f	0.000	272335	0	0.432	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 19:36
Operator : AR\AJ
Sample : 03337-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
WC-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:27:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

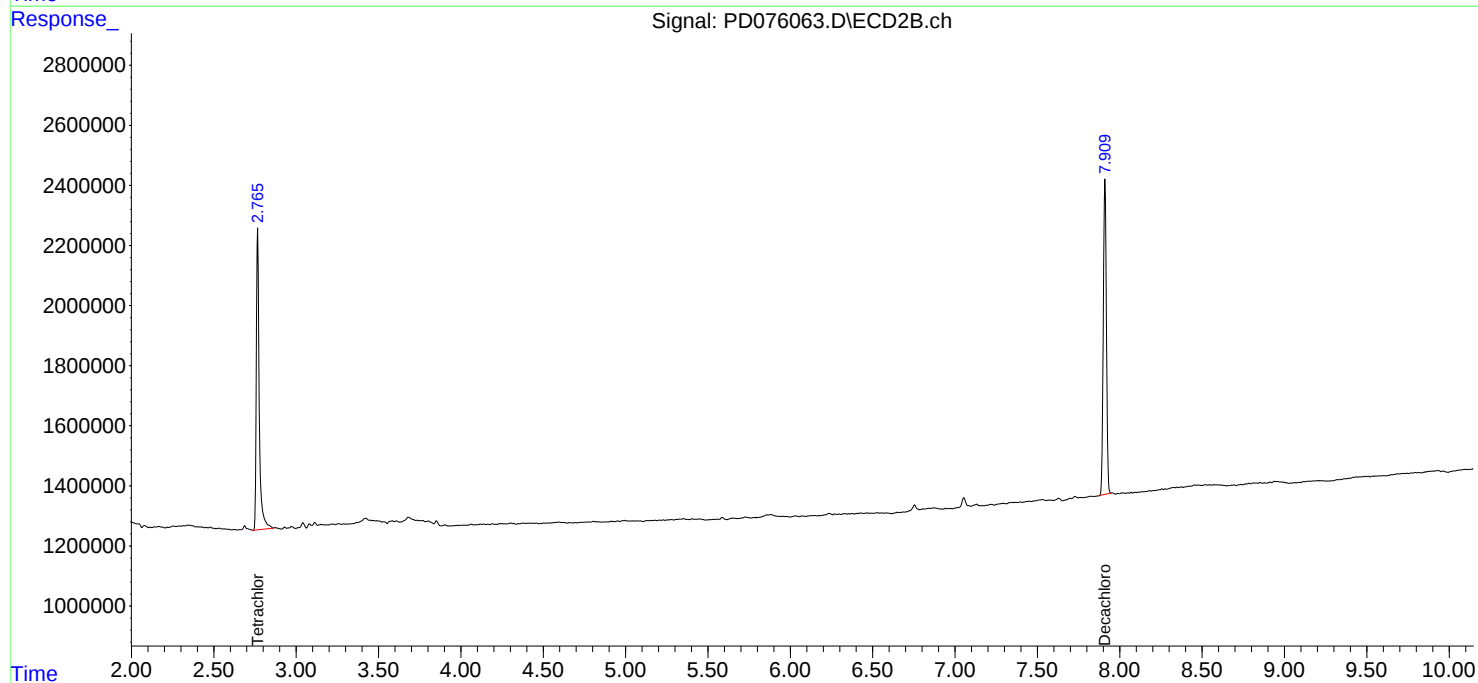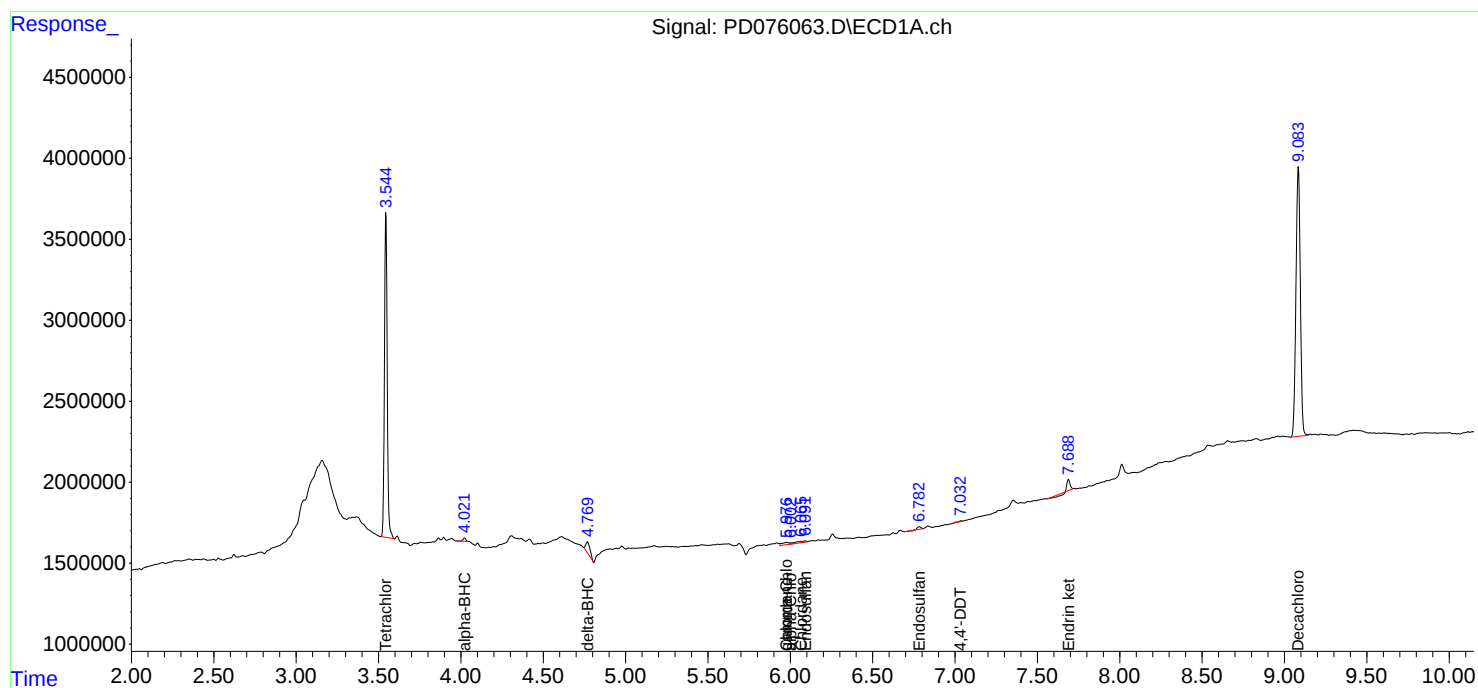


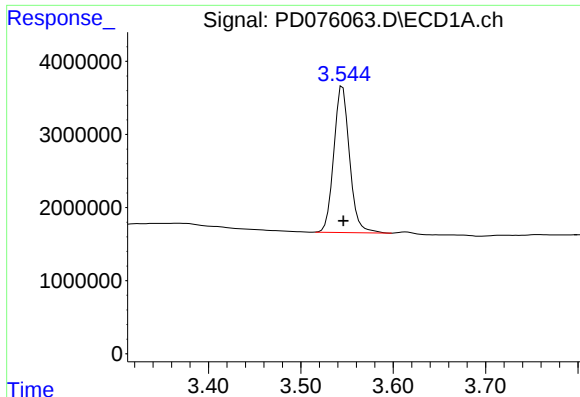

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 23678958
Conc: 11.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-7

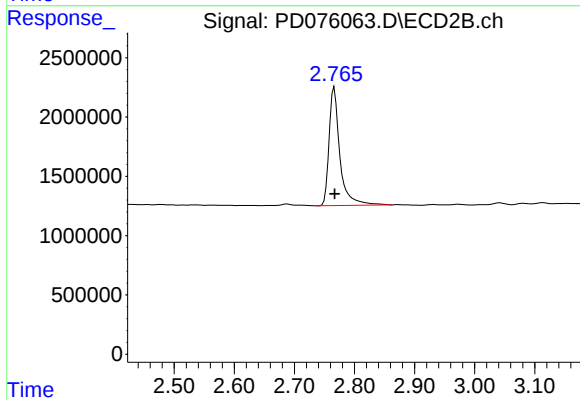


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 12488014
Conc: 11.51 ng/ml

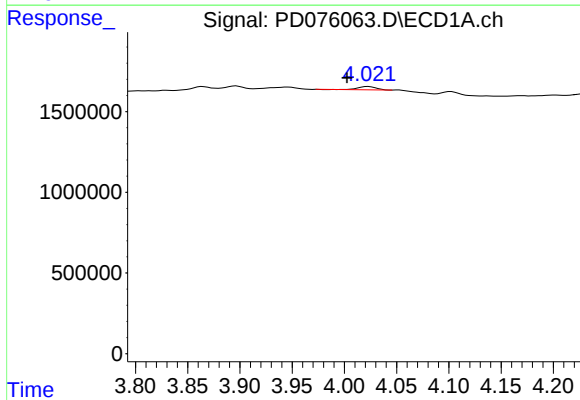


#2 alpha-BHC

R.T.: 4.023 min
Delta R.T.: 0.020 min
Response: 248161
Conc: 0.07 ng/ml

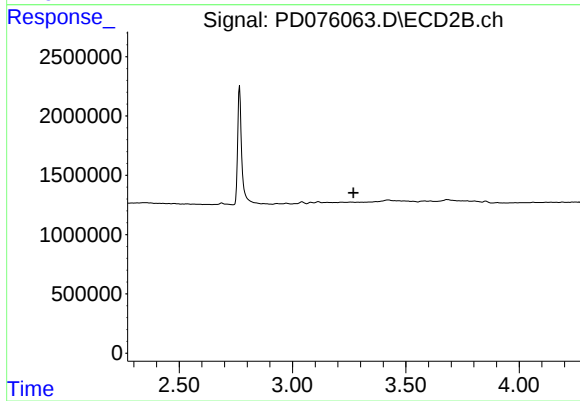

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.270 min
Response: 0
Conc: N.D.

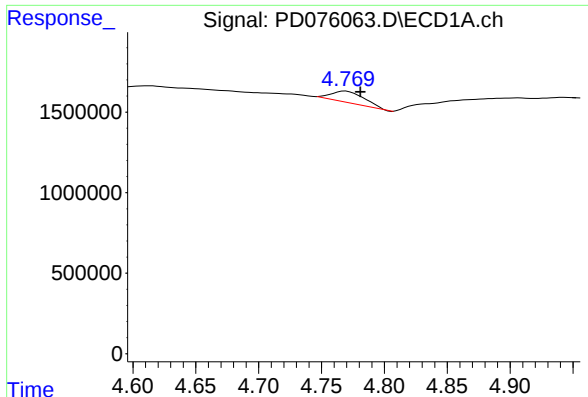

#7 delta-BHC


R.T.: 4.769 min
Delta R.T.: -0.011 min
Response: 1304836
Conc: 0.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-7

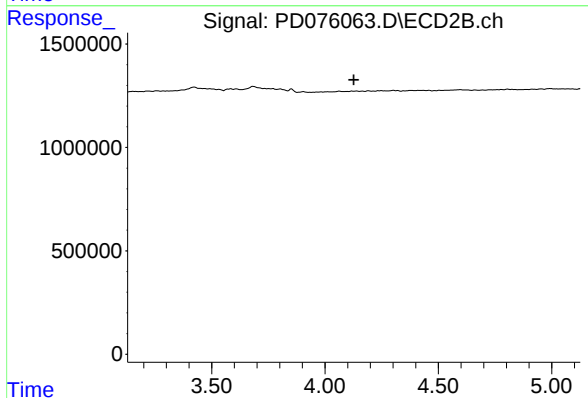


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

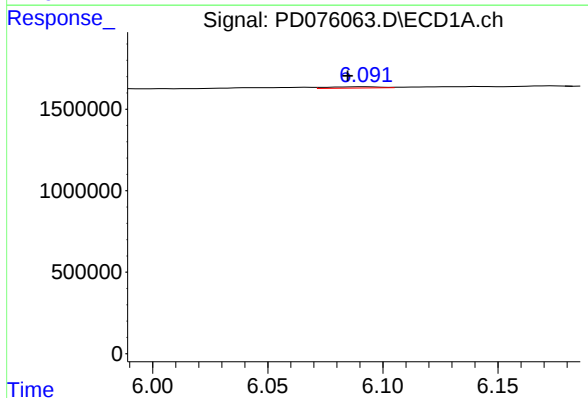


#9 Endosulfan I

R.T.: 6.093 min
Delta R.T.: 0.008 min
Response: 124641
Conc: 0.04 ng/ml

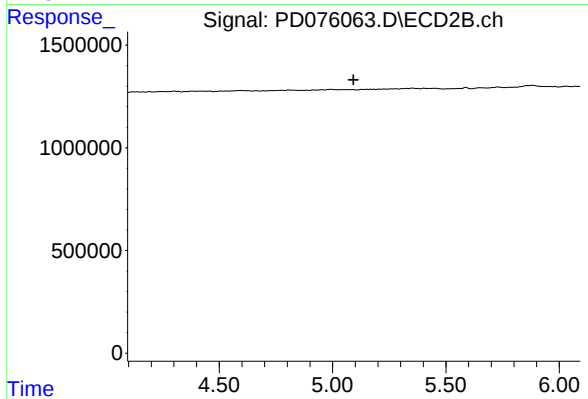

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

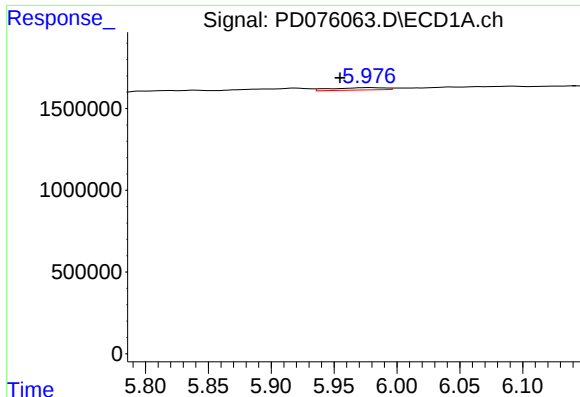

#10 gamma-Chlordane


R.T.: 5.977 min
Delta R.T.: 0.023 min
Response: 432741
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-7

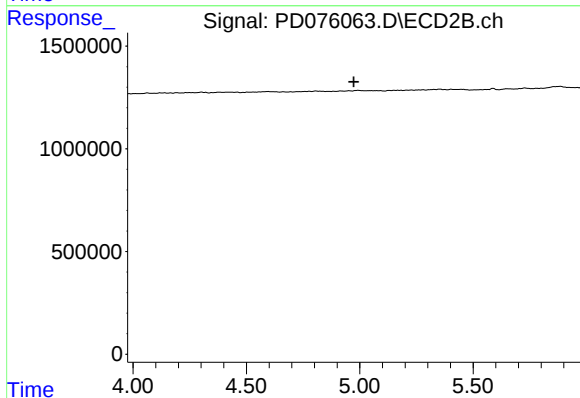


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

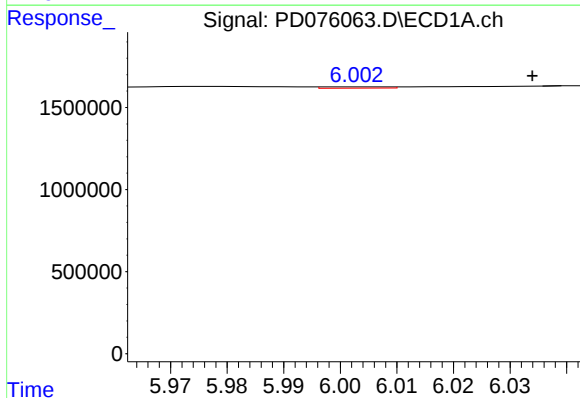


#11 alpha-Chlordane

R.T.: 6.005 min
Delta R.T.: -0.029 min
Response: 63896
Conc: 0.02 ng/ml

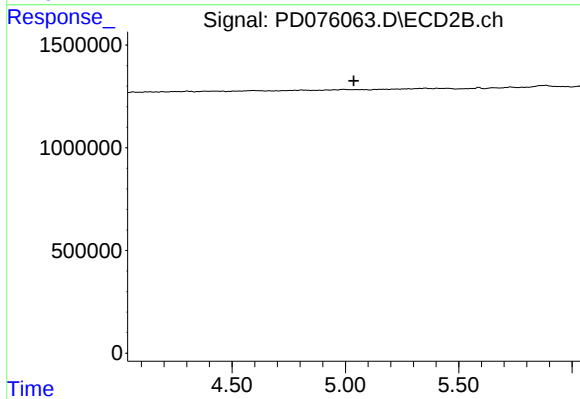

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

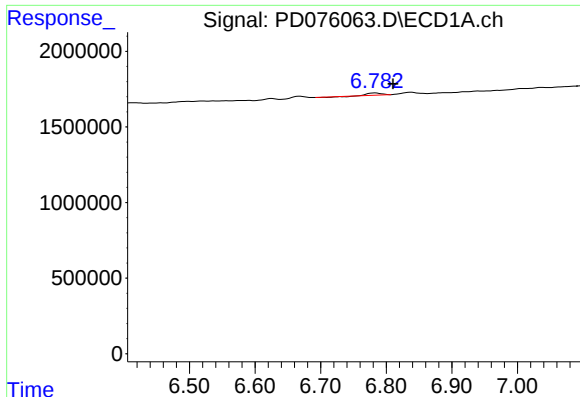

#15 Endosulfan II


R.T.: 6.783 min
Delta R.T.: -0.027 min
Response: 185440
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-7

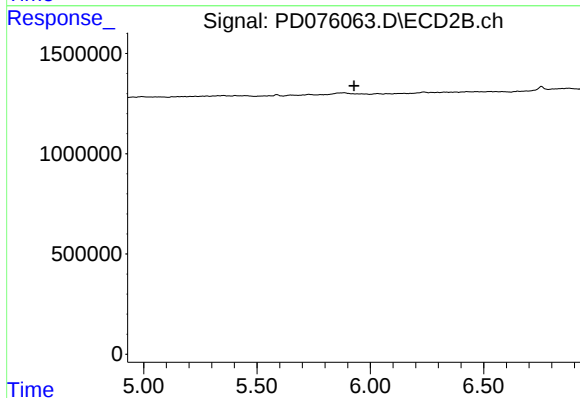


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

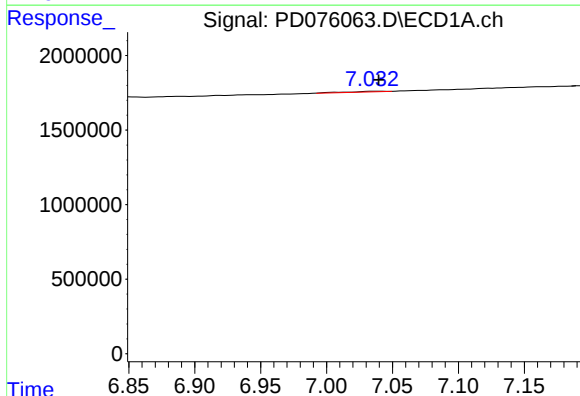


#17 4,4'-DDT

R.T.: 7.035 min
Delta R.T.: -0.004 min
Response: 85307
Conc: 0.04 ng/ml

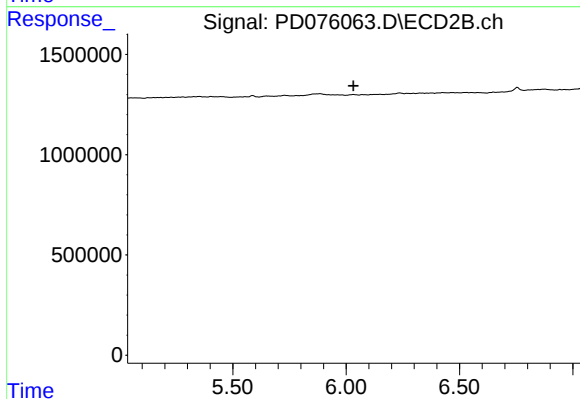

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

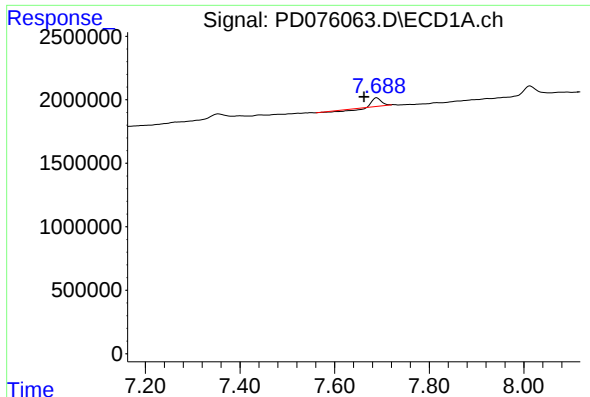

#21 Endrin ketone


R.T.: 7.689 min
Delta R.T.: 0.027 min
Response: 519100
Conc: 0.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-7

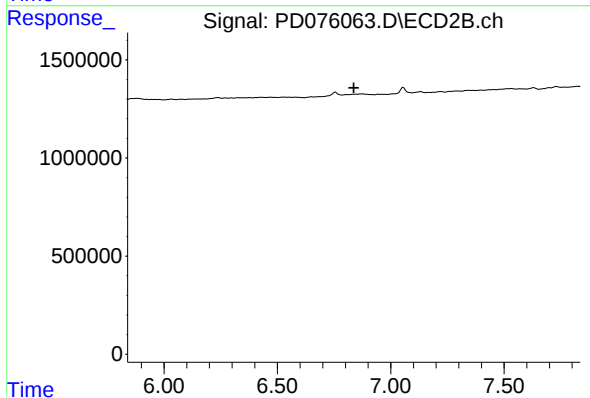


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

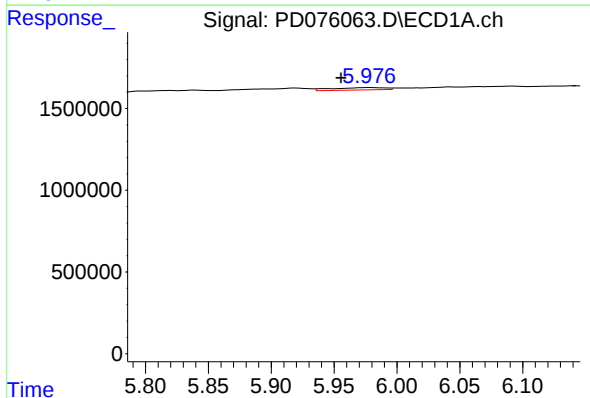


#25 Chlordane-3

R.T.: 5.977 min
Delta R.T.: 0.022 min
Response: 432741
Conc: 0.83 ng/ml

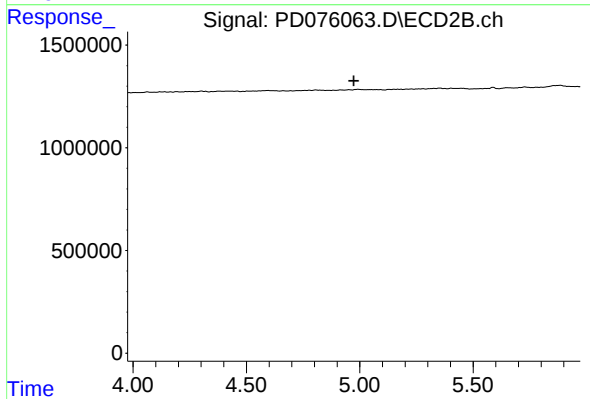

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

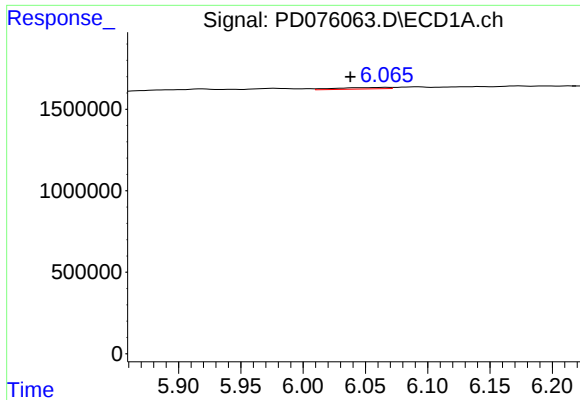

#26 Chlordane-4


R.T.: 6.066 min
Delta R.T.: 0.028 min
Response: 272335
Conc: 0.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-7

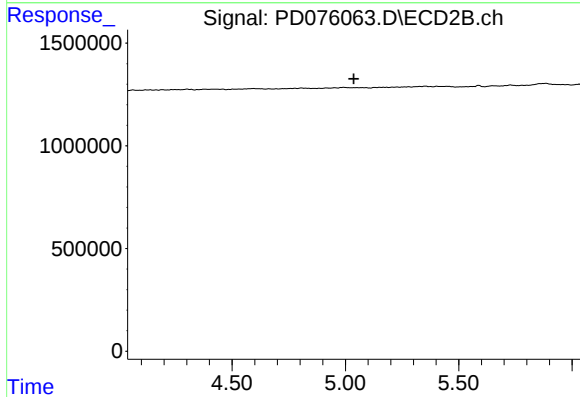


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

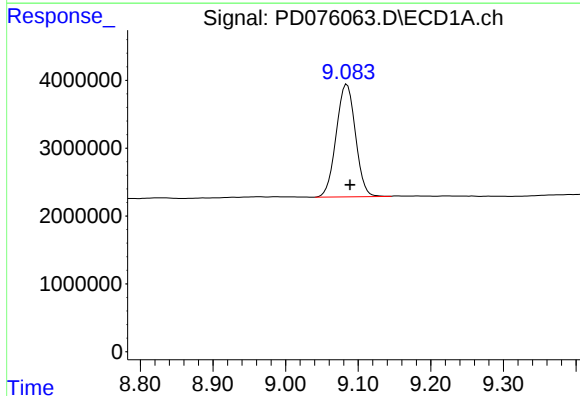

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.005 min
Response: 30548657
Conc: 12.06 ng/ml

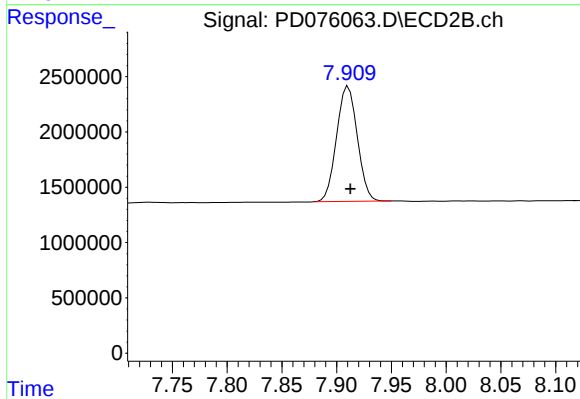

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.002 min
Response: 13738221
Conc: 14.05 ng/ml