

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 19:49
 Operator : AR\AJ
 Sample : 03337-16
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:27:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	25126160	13007352	11.796	11.989
28)	SA Decachlor...	9.083	7.910	30315258	13317160	11.966	13.620
Target Compounds							
7)	B delta-BHC	4.770	0.000	1130306	0	0.340	N.D. #
10)	B gamma-Chl...	5.945	0.000	231469	0	0.072	N.D. #
11)	B alpha-Chl...	6.042	0.000	89364	0	0.028	N.D. #
12)	B 4,4'-DDE	6.204	5.225	393054	223306	0.138	0.200 #
15)	B Endosulfa...	6.834f	0.000	84769	0	0.033	N.D. #
17)	MA 4,4'-DDT	7.039	0.000	202873	0	0.089	N.D. #
21)	B Endrin ke...	7.689f	0.000	1147659	0	0.412	N.D. #
25)	Chlordane-3	5.945	0.000	231469	0	0.446	N.D. #
26)	Chlordane-4	6.042	0.000	89364	0	0.142	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 19:49
Operator : AR\AJ
Sample : 03337-16
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
WC-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:27:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

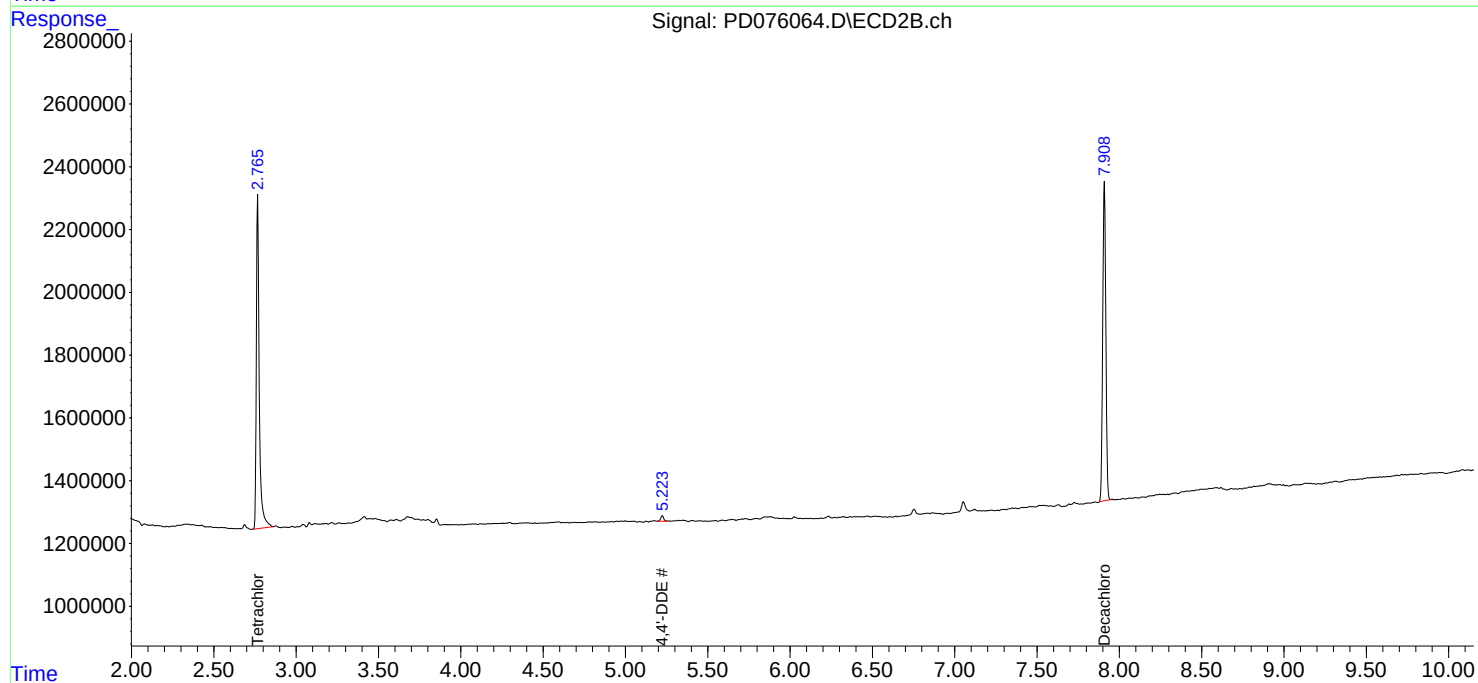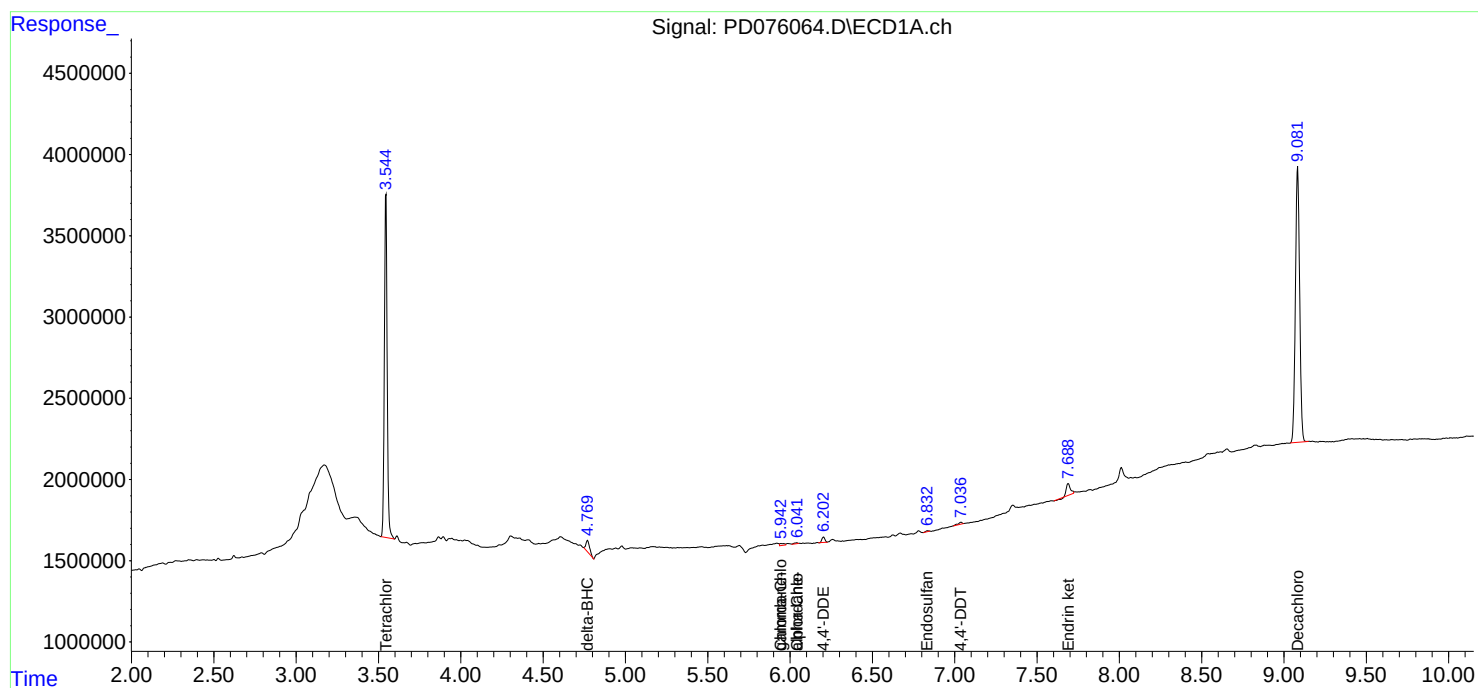


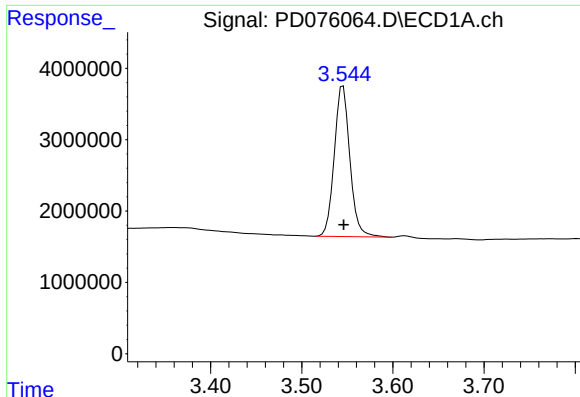

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 25126160
Conc: 11.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-15

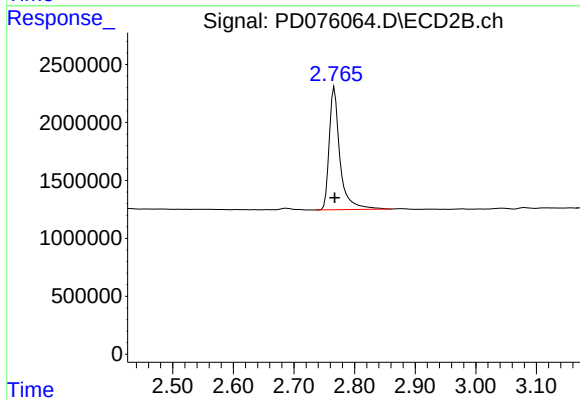


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 13007352
Conc: 11.99 ng/ml

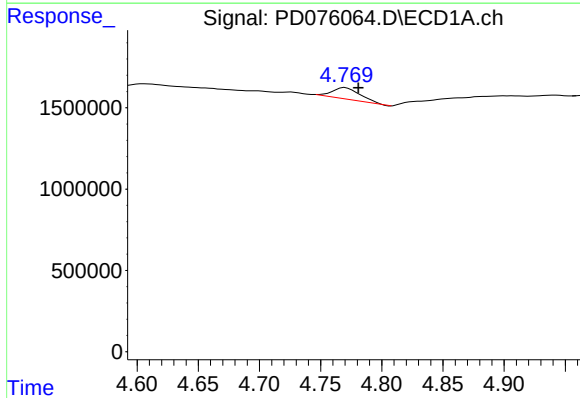


#7 delta-BHC

R.T.: 4.770 min
Delta R.T.: -0.011 min
Response: 1130306
Conc: 0.34 ng/ml

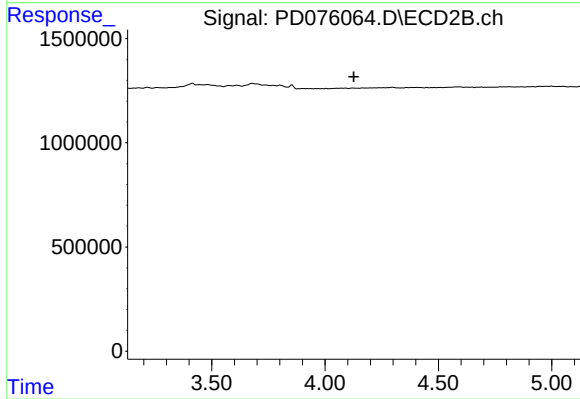

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

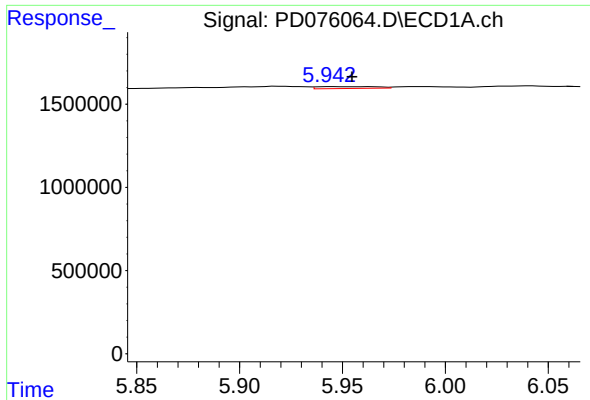

#10 gamma-Chlordane


R.T.: 5.945 min
Delta R.T.: -0.010 min
Response: 231469
Conc: 0.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-15

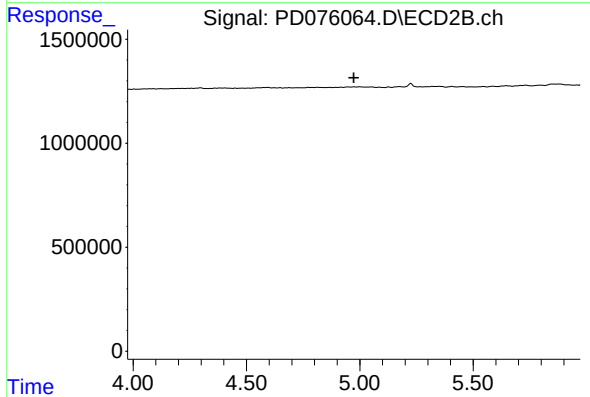


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

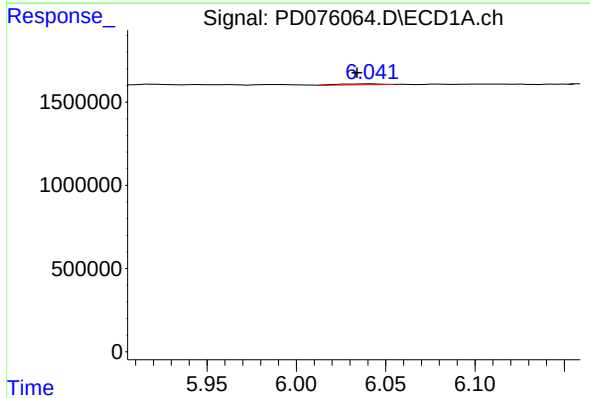


#11 alpha-Chlordane

R.T.: 6.042 min
Delta R.T.: 0.008 min
Response: 89364
Conc: 0.03 ng/ml

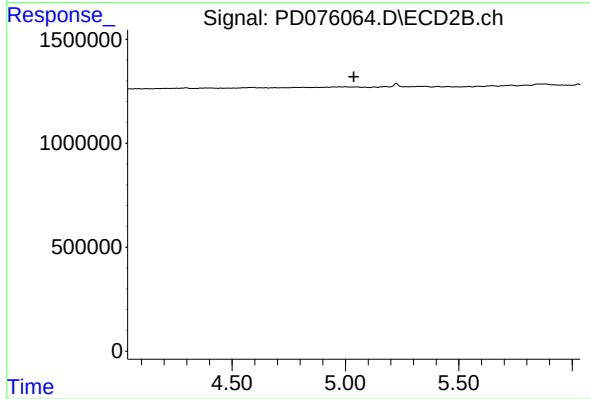

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

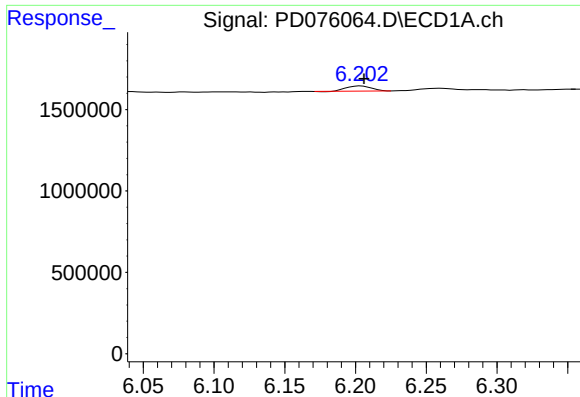

#12 4,4'-DDE


R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 393054
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-15

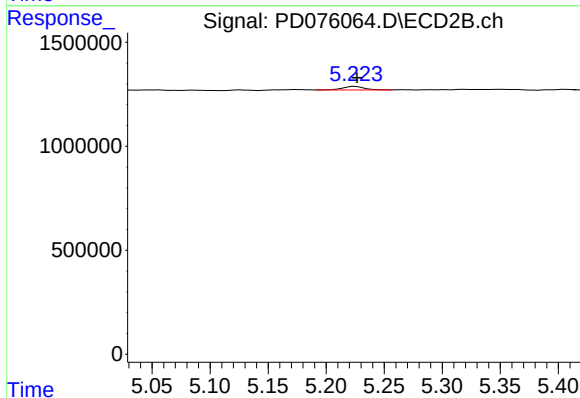


#12 4,4'-DDE

R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 223306
Conc: 0.20 ng/ml

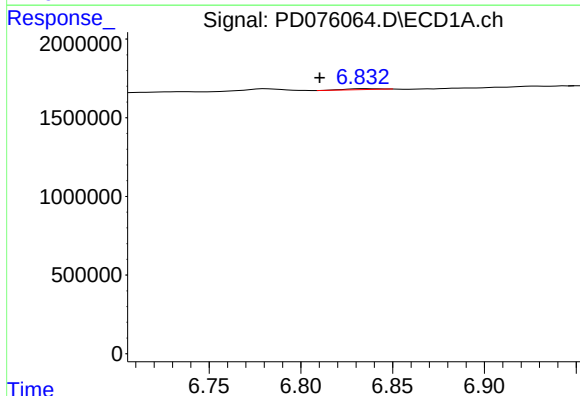


#15 Endosulfan II

R.T.: 6.834 min
Delta R.T.: 0.024 min
Response: 84769
Conc: 0.03 ng/ml

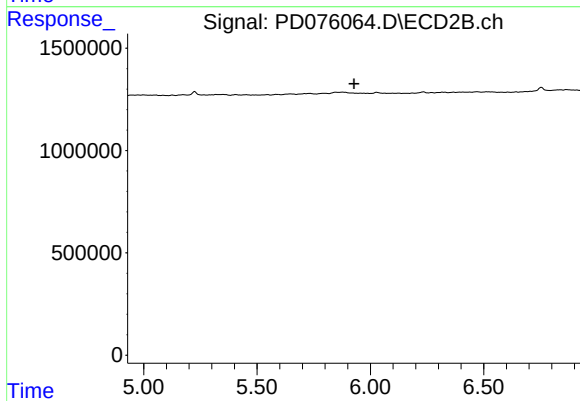

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

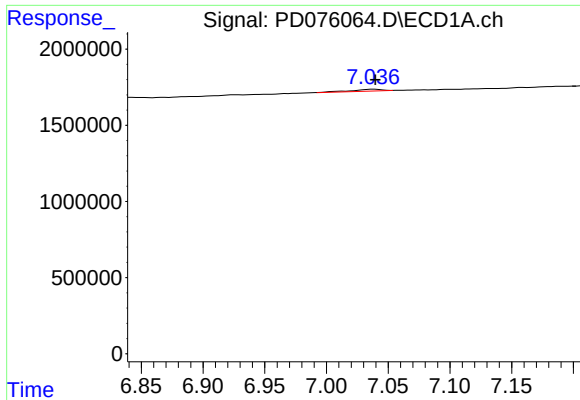

#17 4,4'-DDT


R.T.: 7.039 min
Delta R.T.: 0.000 min
Response: 202873
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-15

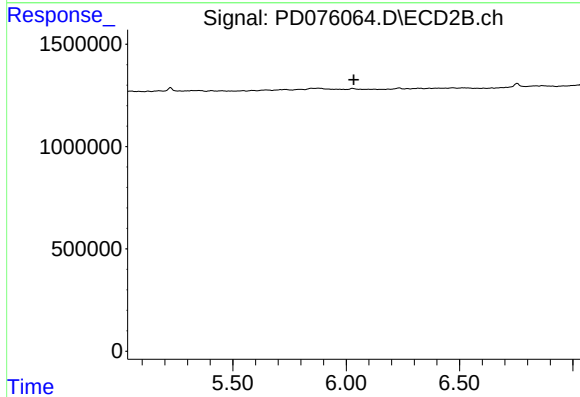


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.033 min
Response: 0
Conc: N.D.

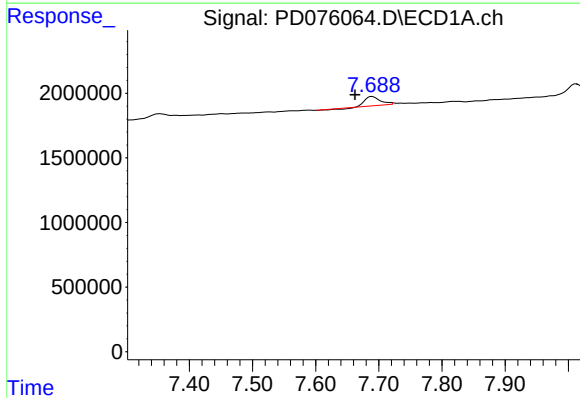


#21 Endrin ketone

R.T.: 7.689 min
Delta R.T.: 0.027 min
Response: 1147659
Conc: 0.41 ng/ml

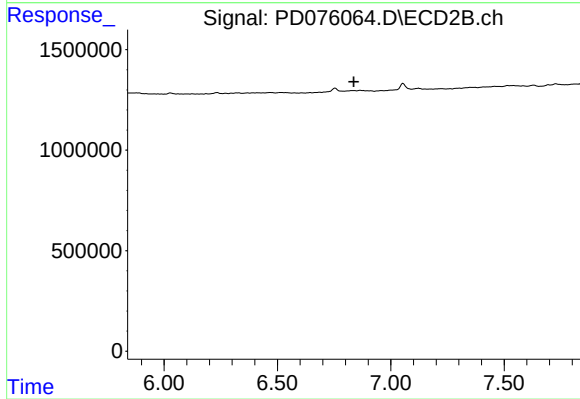

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

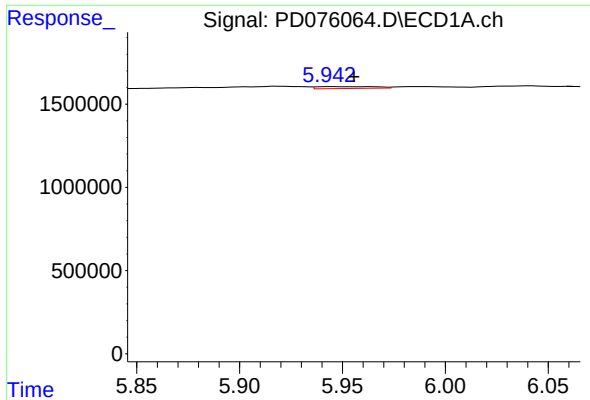

#25 Chlordane-3


R.T.: 5.945 min
Delta R.T.: -0.011 min
Response: 231469
Conc: 0.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-15

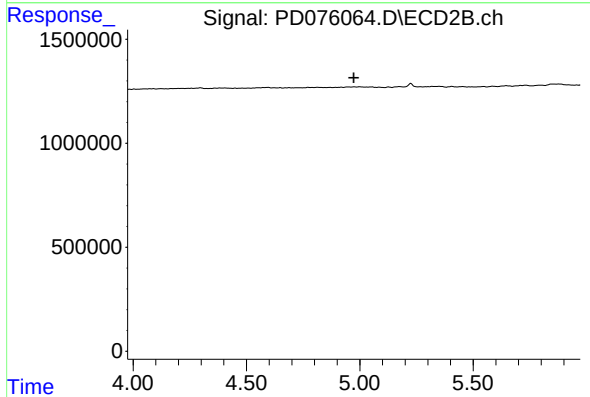


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

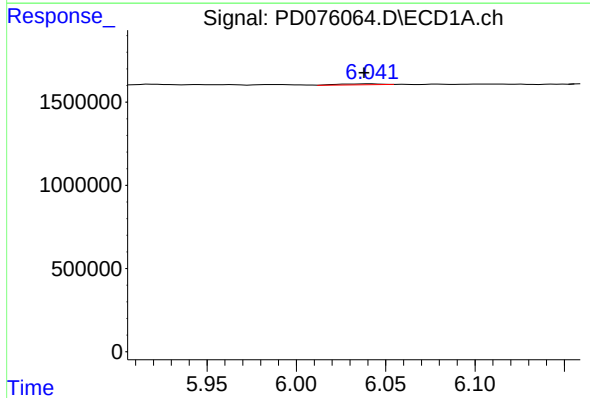


#26 Chlordane-4

R.T.: 6.042 min
Delta R.T.: 0.004 min
Response: 89364
Conc: 0.14 ng/ml

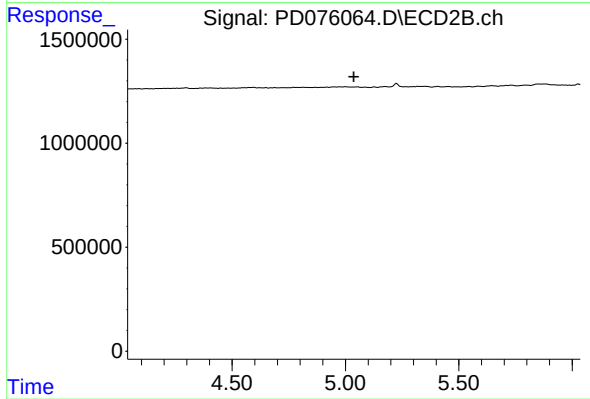

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

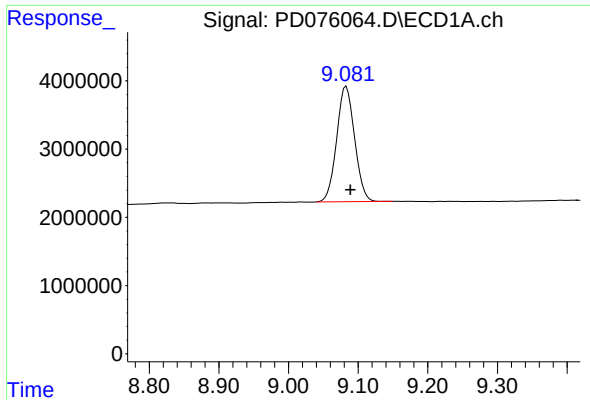

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.006 min
Response: 30315258
Conc: 11.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-15

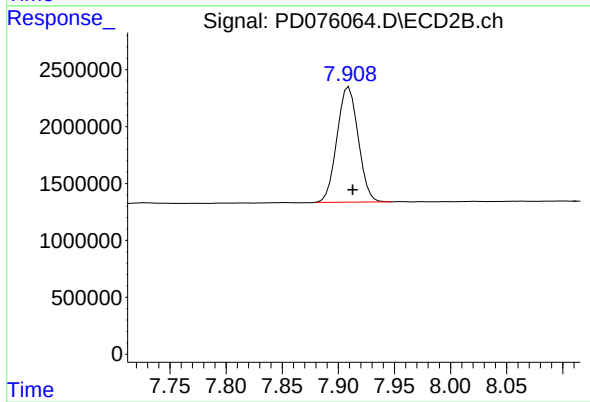

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.003 min
Response: 13317160
Conc: 13.62 ng/ml