

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076065.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 20:03
 Operator : AR\AJ
 Sample : 03337-19
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:28:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	26302715	13816767	12.348	12.735
28)	SA Decachlor...	9.085	7.909	32855336	14911689	12.969	15.250
Target Compounds							
7)	B delta-BHC	4.771	0.000	1768410	0	0.532	N.D. #
8)	B Heptachlo...	5.691	0.000	1214405	0	0.377	N.D. #
9)	A Endosulfan I	6.071	0.000	233950	0	0.078	N.D. #
10)	B gamma-Chl...	5.929f	0.000	1226724	0	0.381	N.D. #
11)	B alpha-Chl...	6.032	0.000	149815	0	0.046	N.D. #
15)	B Endosulfa...	6.835f	0.000	123306	0	0.048	N.D. #
21)	B Endrin ke...	7.637f	0.000	78434	0	0.028	N.D. #
25)	Chlordane-3	5.929f	0.000	1226724	0	2.362	N.D. #
26)	Chlordane-4	6.032	0.000	149815	0	0.238	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076065.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 20:03
Operator : AR\AJ
Sample : 03337-19
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
WC-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:28:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

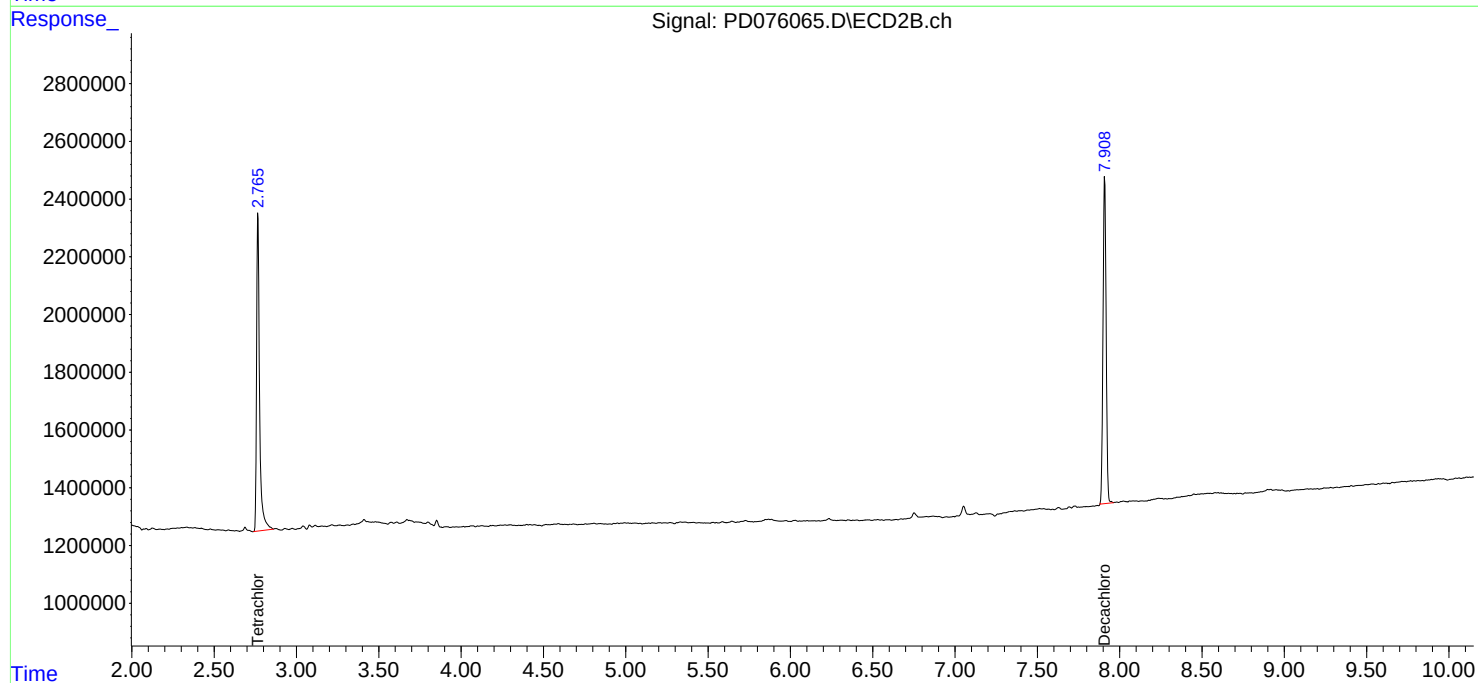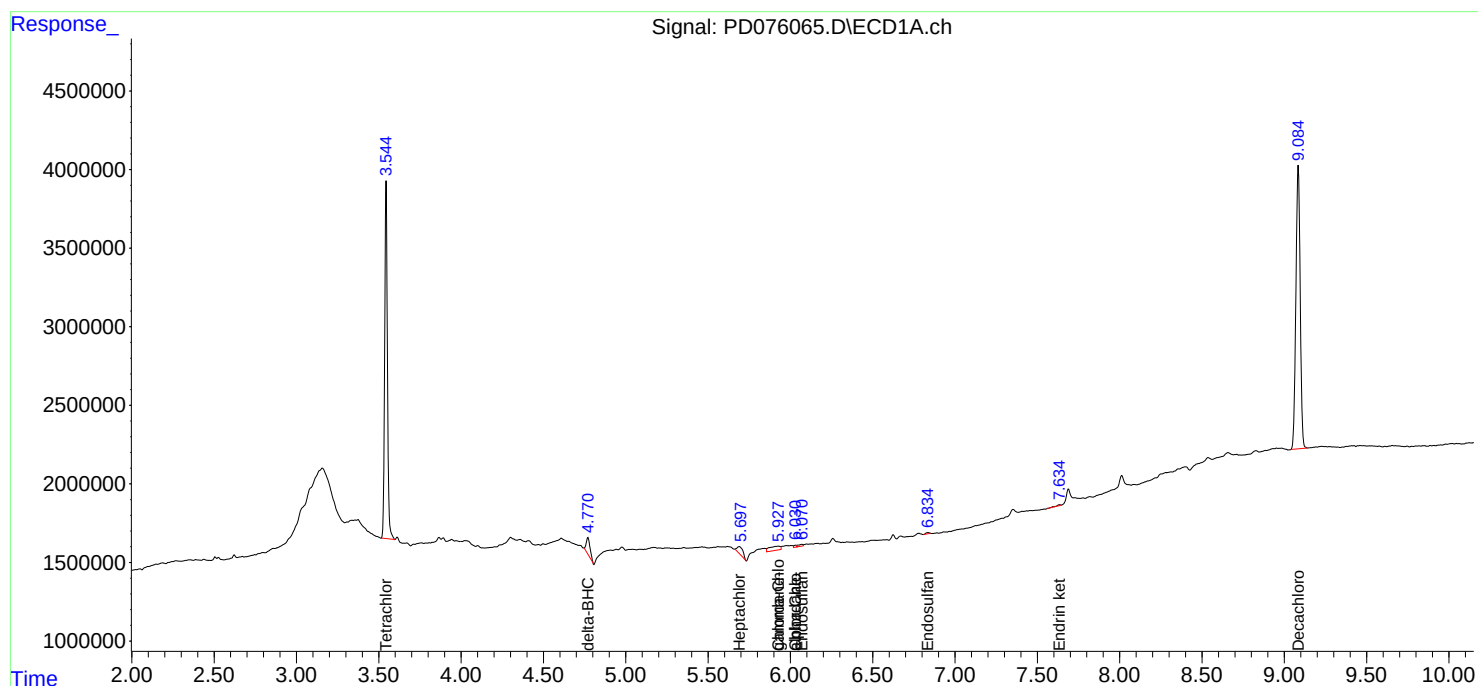


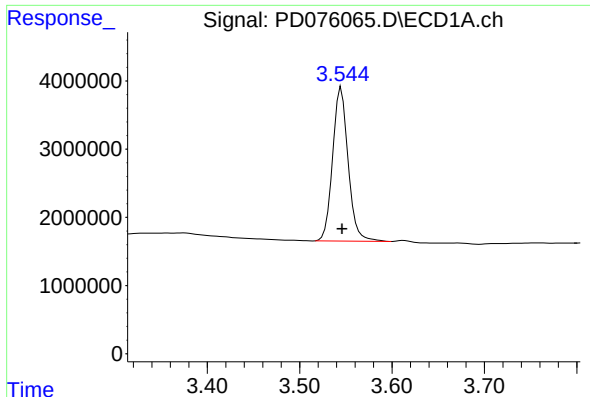

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 26302715
Conc: 12.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-11

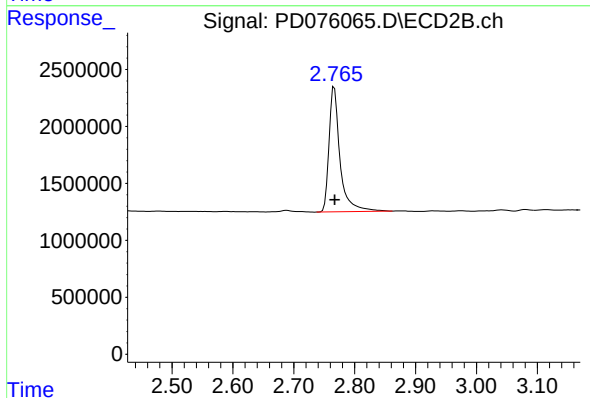


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 13816767
Conc: 12.74 ng/ml

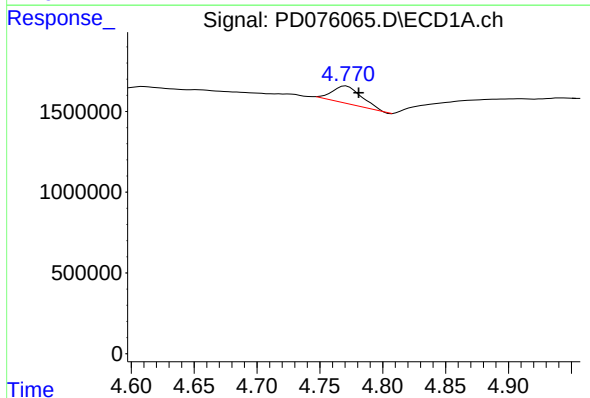


#7 delta-BHC

R.T.: 4.771 min
Delta R.T.: -0.010 min
Response: 1768410
Conc: 0.53 ng/ml

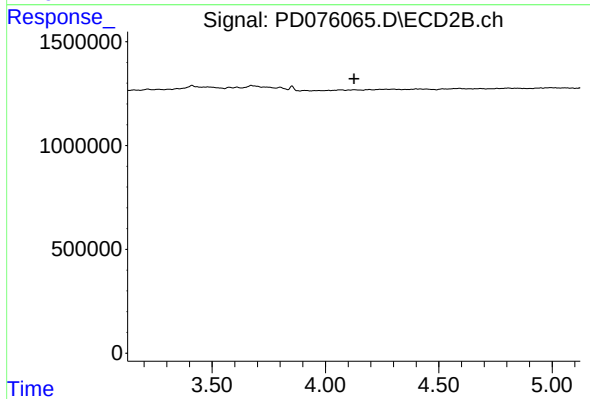

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

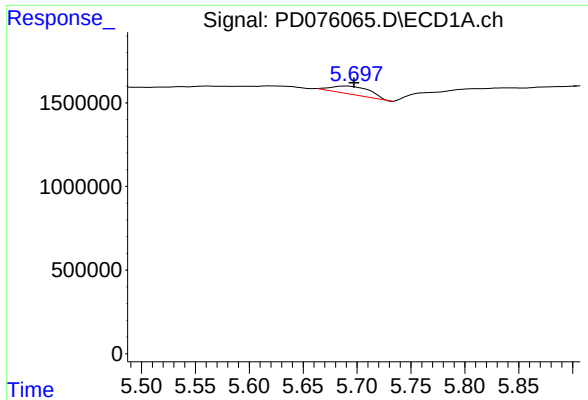

#8 Heptachlor epoxide


R.T.: 5.691 min
Delta R.T.: -0.007 min
Response: 1214405
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-11

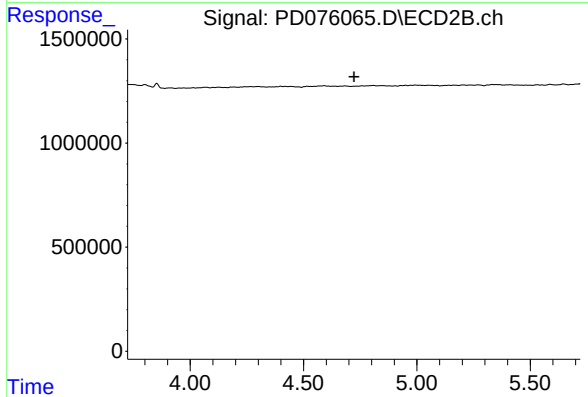


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

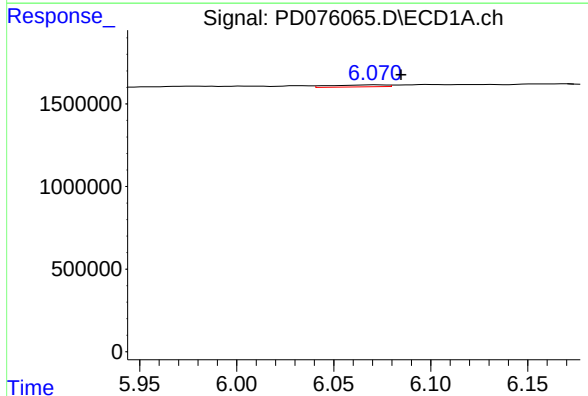


#9 Endosulfan I

R.T.: 6.071 min
Delta R.T.: -0.013 min
Response: 233950
Conc: 0.08 ng/ml

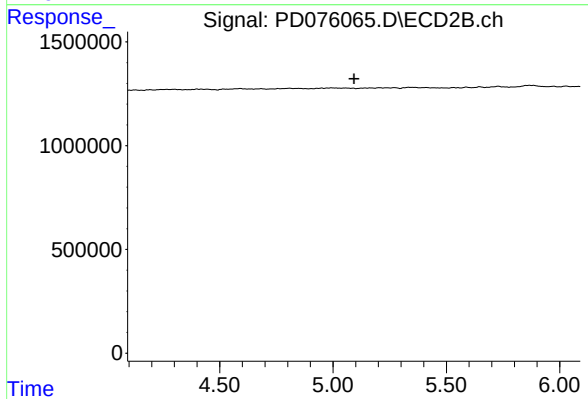

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

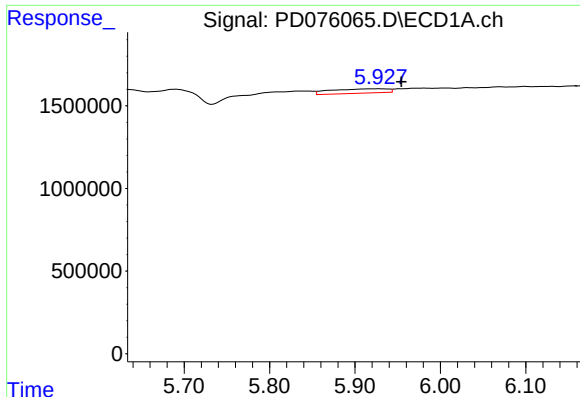

#10 gamma-Chlordane


R.T.: 5.929 min
Delta R.T.: -0.026 min
Response: 1226724
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-11

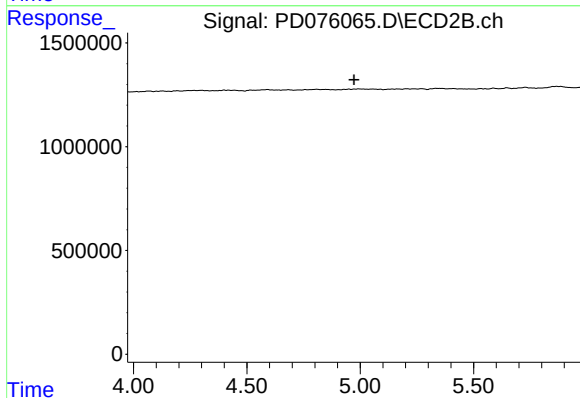


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

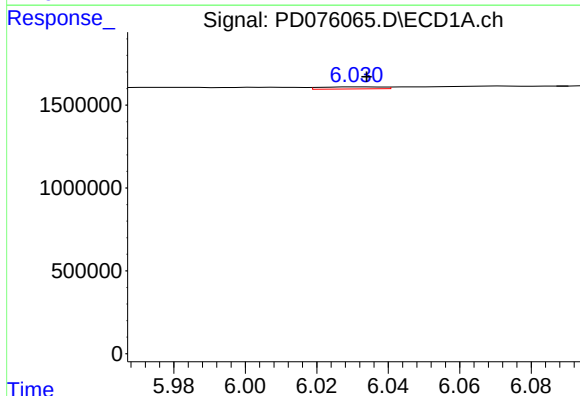


#11 alpha-Chlordane

R.T.: 6.032 min
Delta R.T.: -0.002 min
Response: 149815
Conc: 0.05 ng/ml

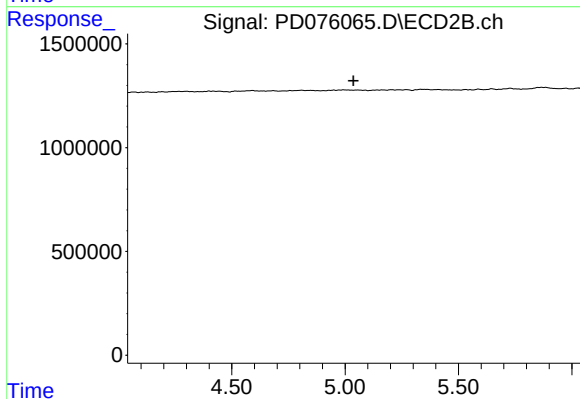

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

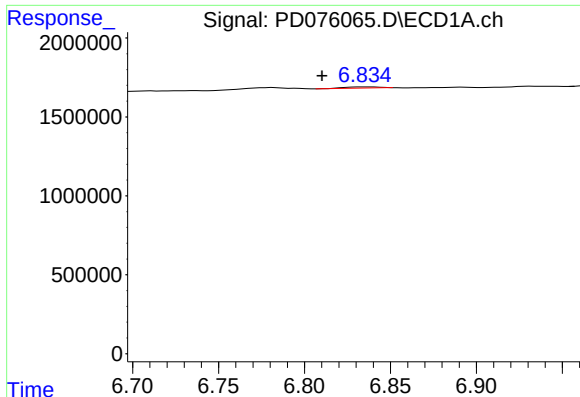

#15 Endosulfan II


R.T.: 6.835 min
Delta R.T.: 0.025 min
Response: 123306
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-11

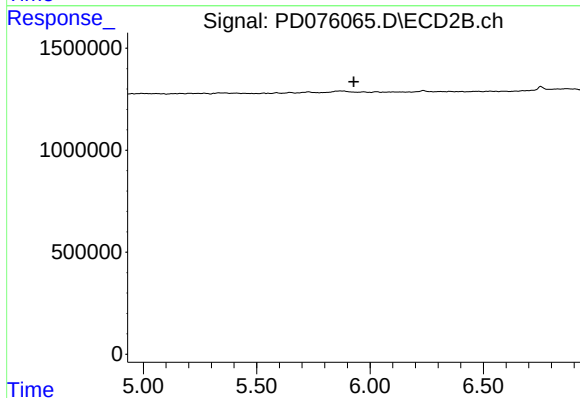


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

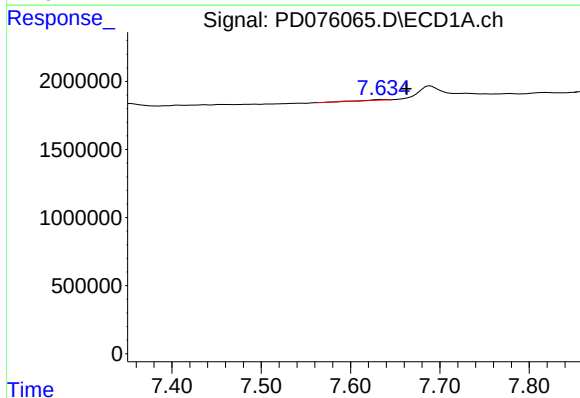


#21 Endrin ketone

R.T.: 7.637 min
Delta R.T.: -0.026 min
Response: 78434
Conc: 0.03 ng/ml

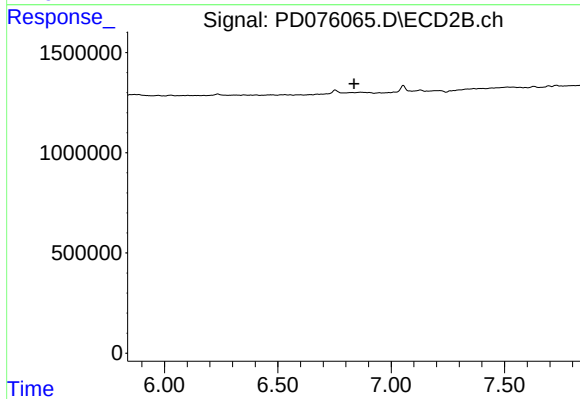

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

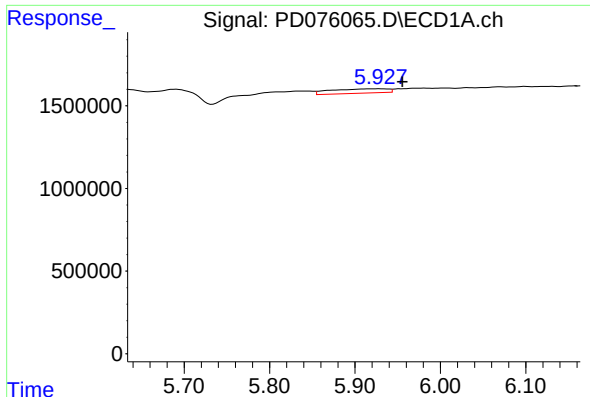

#25 Chlordane-3


R.T.: 5.929 min
Delta R.T.: -0.027 min
Response: 1226724
Conc: 2.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-11

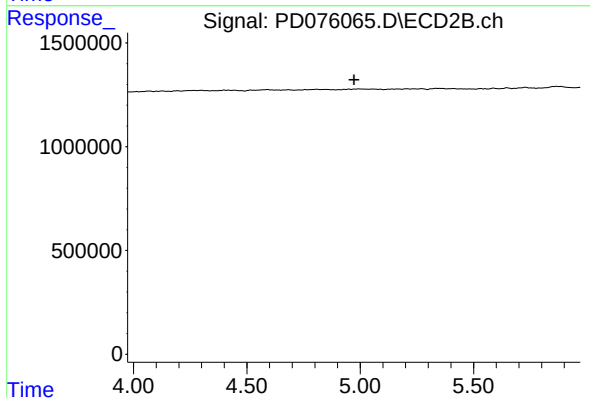


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

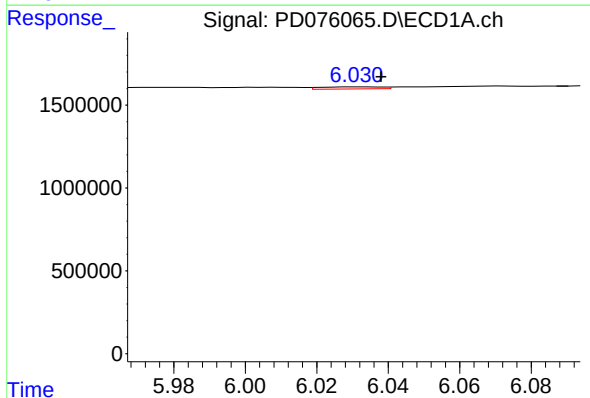


#26 Chlordane-4

R.T.: 6.032 min
Delta R.T.: -0.006 min
Response: 149815
Conc: 0.24 ng/ml

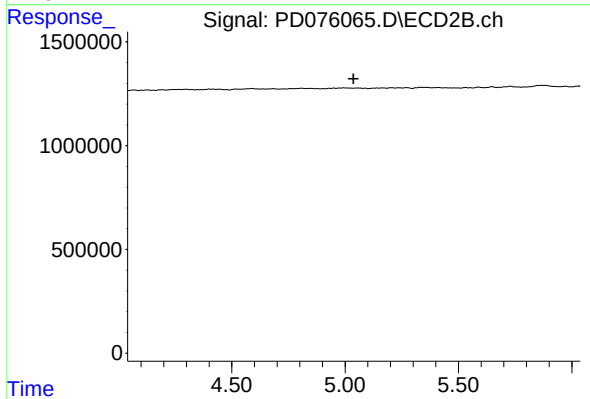

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

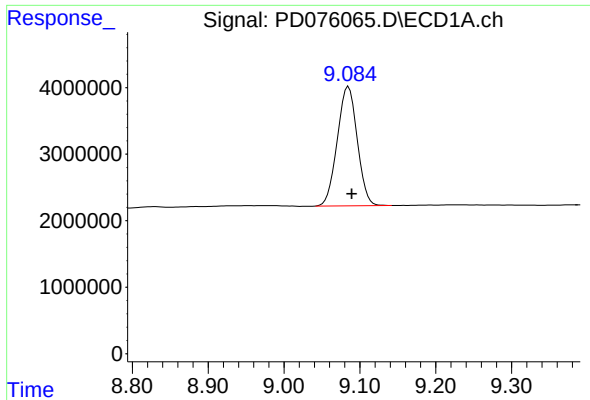

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.004 min
Response: 32855336
Conc: 12.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-11

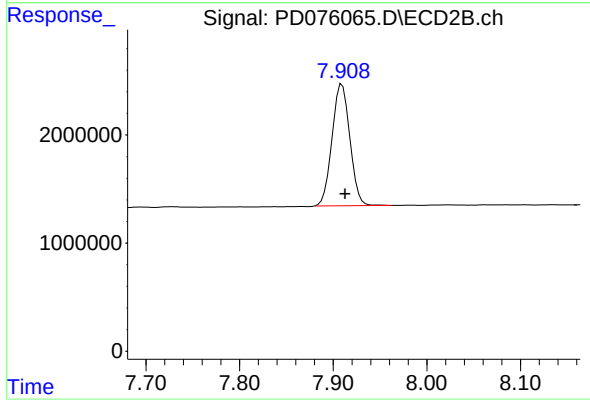

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.003 min
Response: 14911689
Conc: 15.25 ng/ml