

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 14:07
 Operator : AR\AJ
 Sample : 03329-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMPOSIT-SW01-0-8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/23/2023
 Supervised By :Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:15:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	50446246	26257919	23.682	24.202
28)	SA Decachlor...	9.083	7.909	67011538	28600735	26.452	29.250
Target Compounds							
10)	B gamma-Chl...	5.952	4.970	37122791	9080199	11.524	6.618m#
11)	B alpha-Chl...	6.035	5.033	57460310	15255106	17.774	11.121m#
17)	MA 4,4'-DDT	7.035	6.027	14849240	20336750	6.544m	25.036 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 14:07
Operator : AR\AJ
Sample : 03329-13
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMPOSIT-SW01-0-8


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/23/2023
Supervised By : Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:15:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

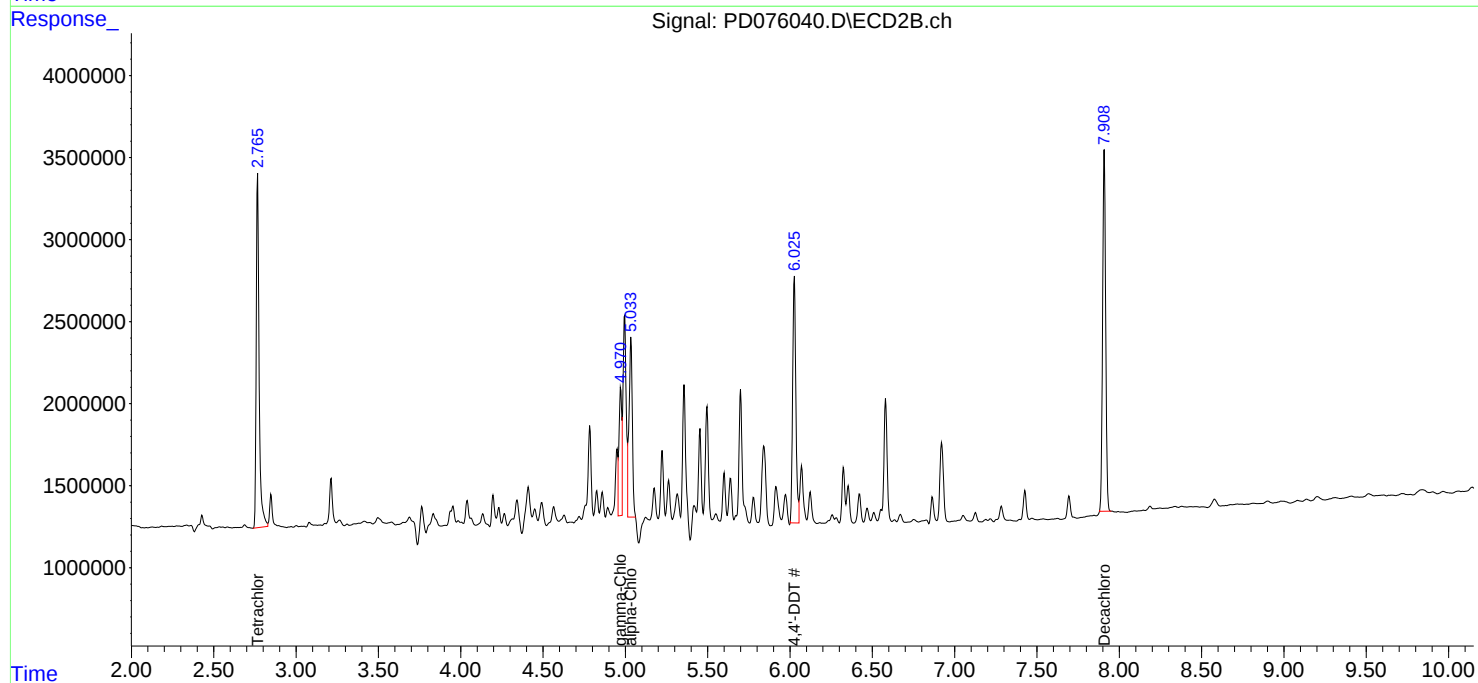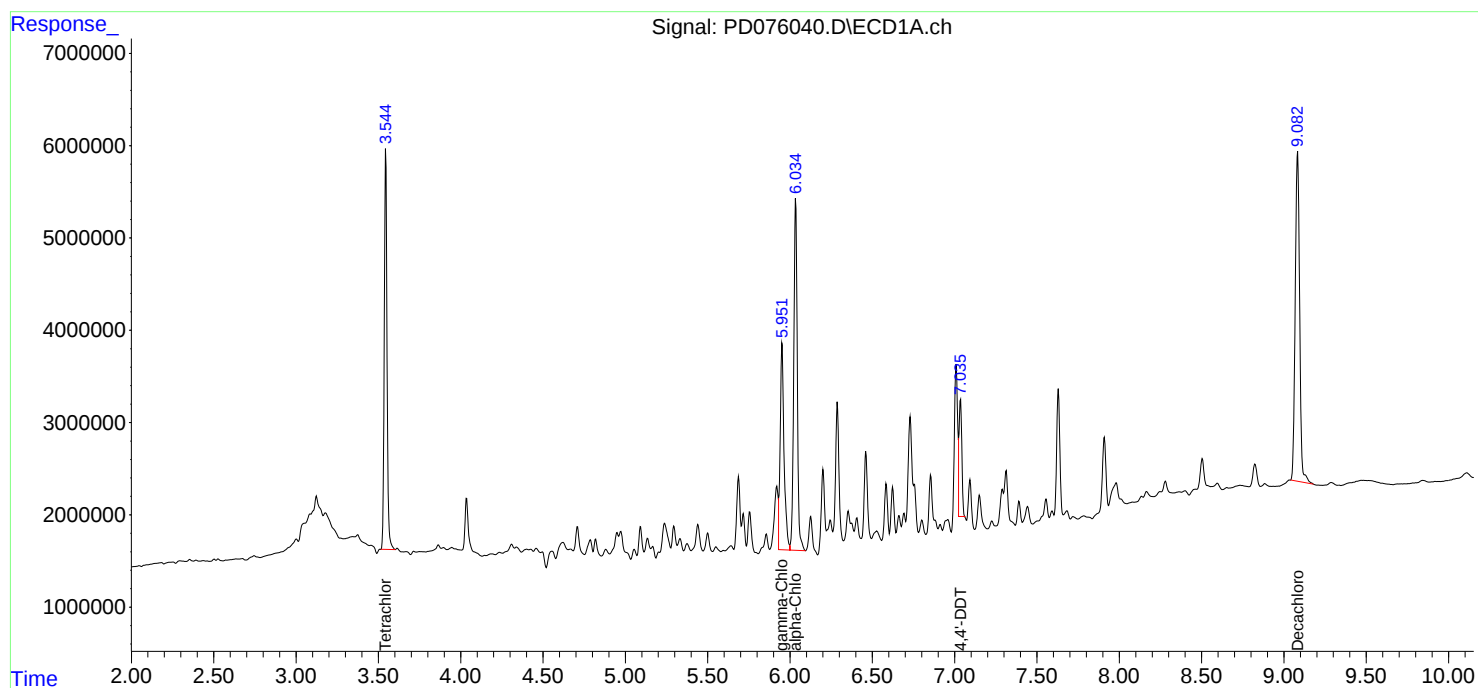

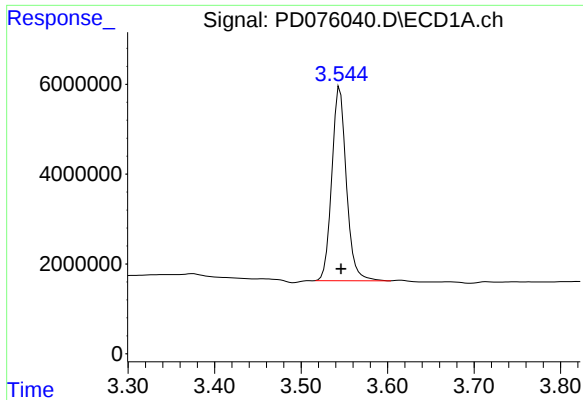


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: -0.001 min
Response: 50446246
Conc: 23.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSIT-SW01-0-8


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

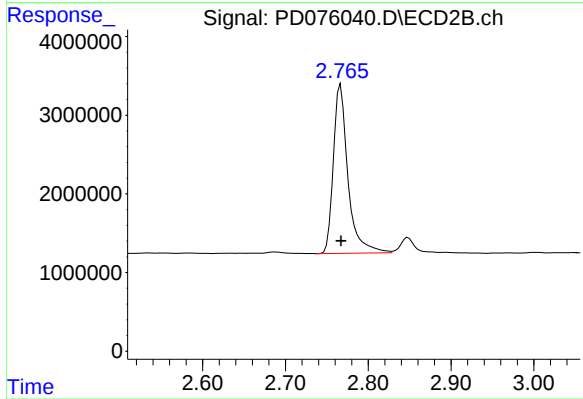


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 26257919
Conc: 24.20 ng/ml

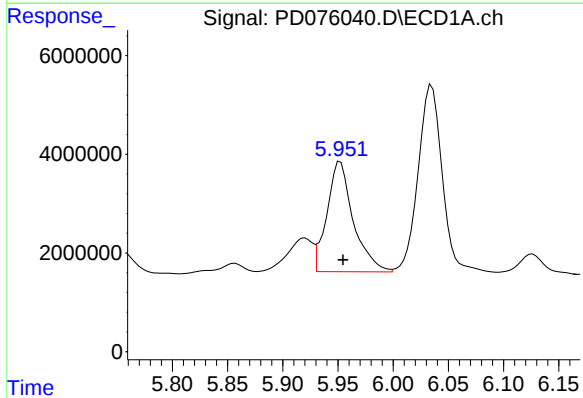


#10 gamma-Chlordane

R.T.: 5.952 min
Delta R.T.: -0.002 min
Response: 37122791
Conc: 11.52 ng/ml

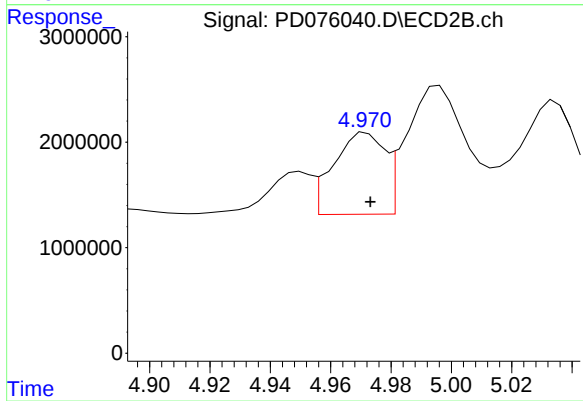

#10 gamma-Chlordane

R.T.: 4.970 min
Delta R.T.: -0.003 min
Response: 9080199
Conc: 6.62 ng/ml m

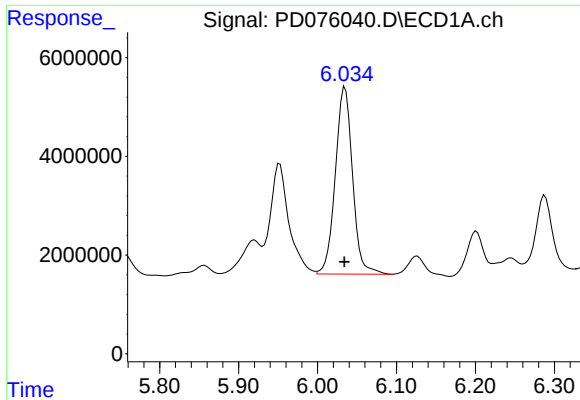


#11 alpha-Chlordane

R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 57460310
Conc: 17.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSIT-SW01-0-8


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

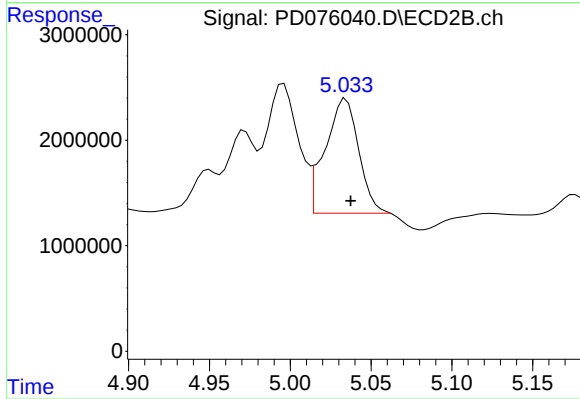


#11 alpha-Chlordane

R.T.: 5.033 min
Delta R.T.: -0.004 min
Response: 15255106
Conc: 11.12 ng/ml m

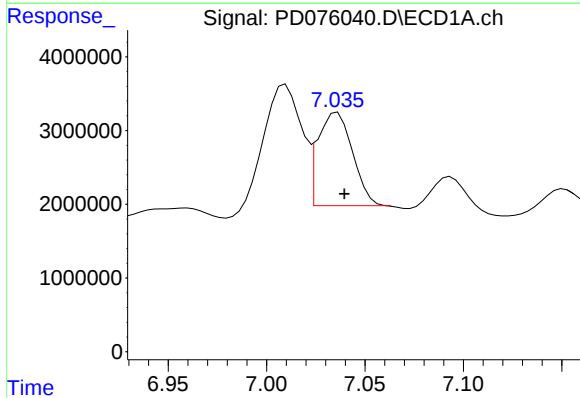


#17 4,4'-DDT

R.T.: 7.035 min
Delta R.T.: -0.005 min
Response: 14849240
Conc: 6.54 ng/ml m

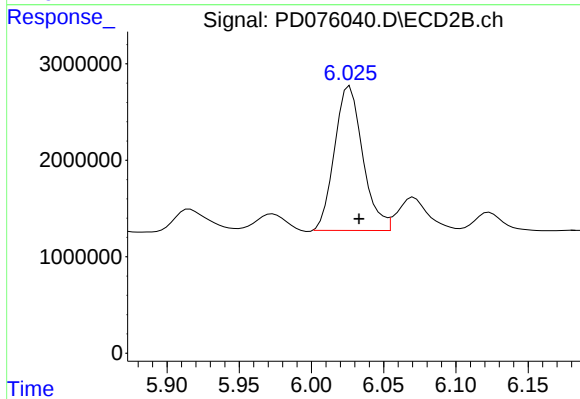

#17 4,4'-DDT

R.T.: 6.027 min
Delta R.T.: -0.006 min
Response: 20336750
Conc: 25.04 ng/ml

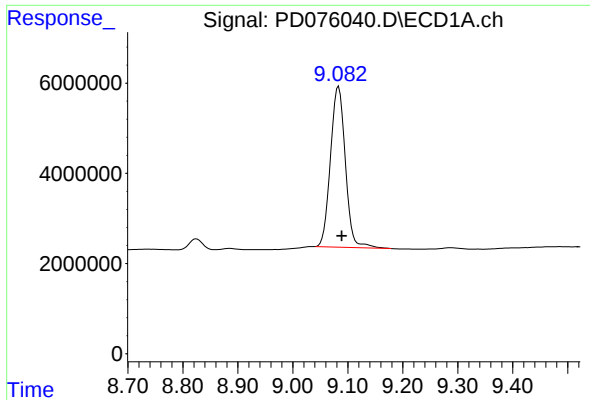


#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.006 min
Response: 67011538
Conc: 26.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSIT-SW01-0-8

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

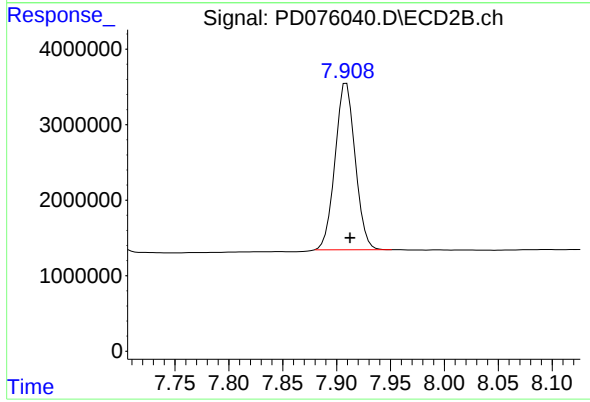

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.004 min
Response: 28600735
Conc: 29.25 ng/ml