

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 15:15
 Operator : AR\AJ
 Sample : 03331-20
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMPOSITE-SB30-35

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/23/2023
 Supervised By :Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:18:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.766	27435997	13436381	12.880	12.385
2)	SA Decachlor...	9.084	7.908	36897082	16821595	14.564	17.204m
Target Compounds							
11)	B alpha-Chl...	6.035	5.031	19020087	4904843	5.883	3.576m#
12)	B 4,4'-DDE	6.202	5.223	15195531	3493966	5.317	3.130m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 15:15
Operator : AR\AJ
Sample : 03331-20
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMPOSITE-SB30-35


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/23/2023
Supervised By : Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:18:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

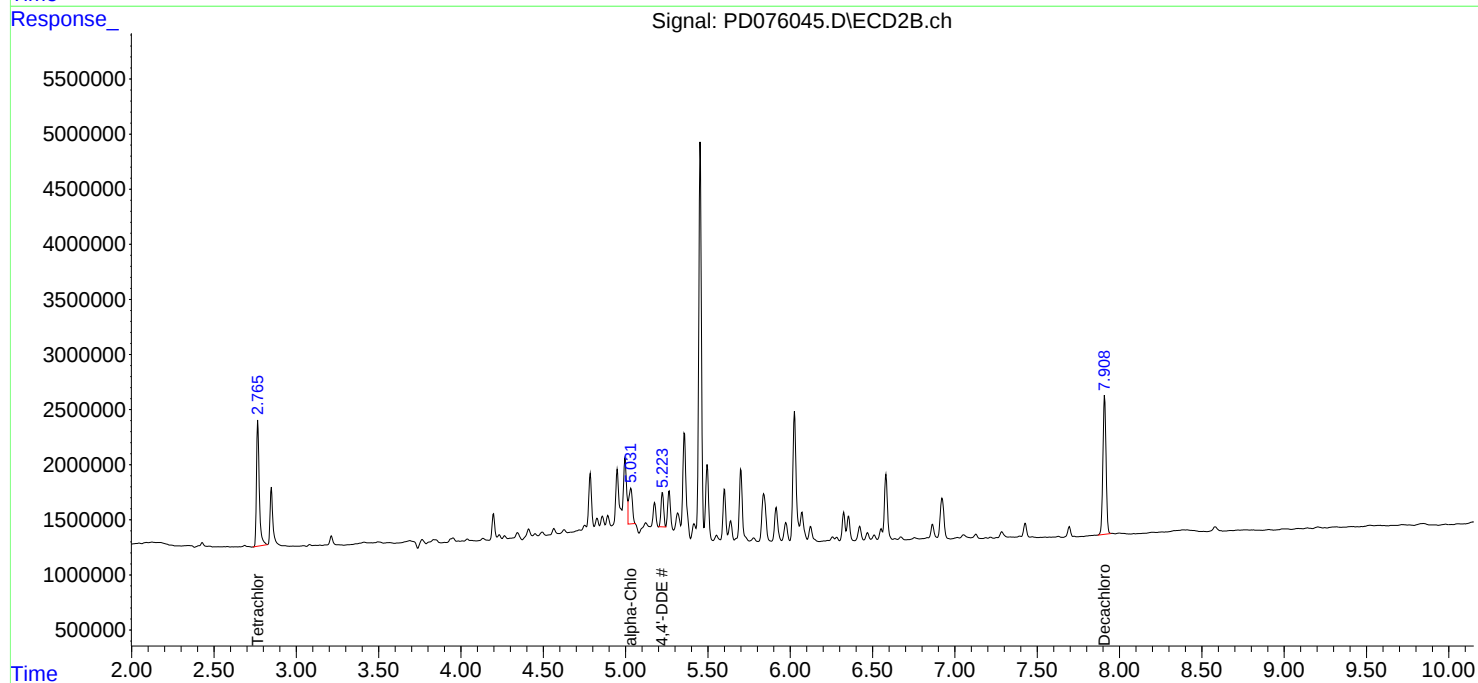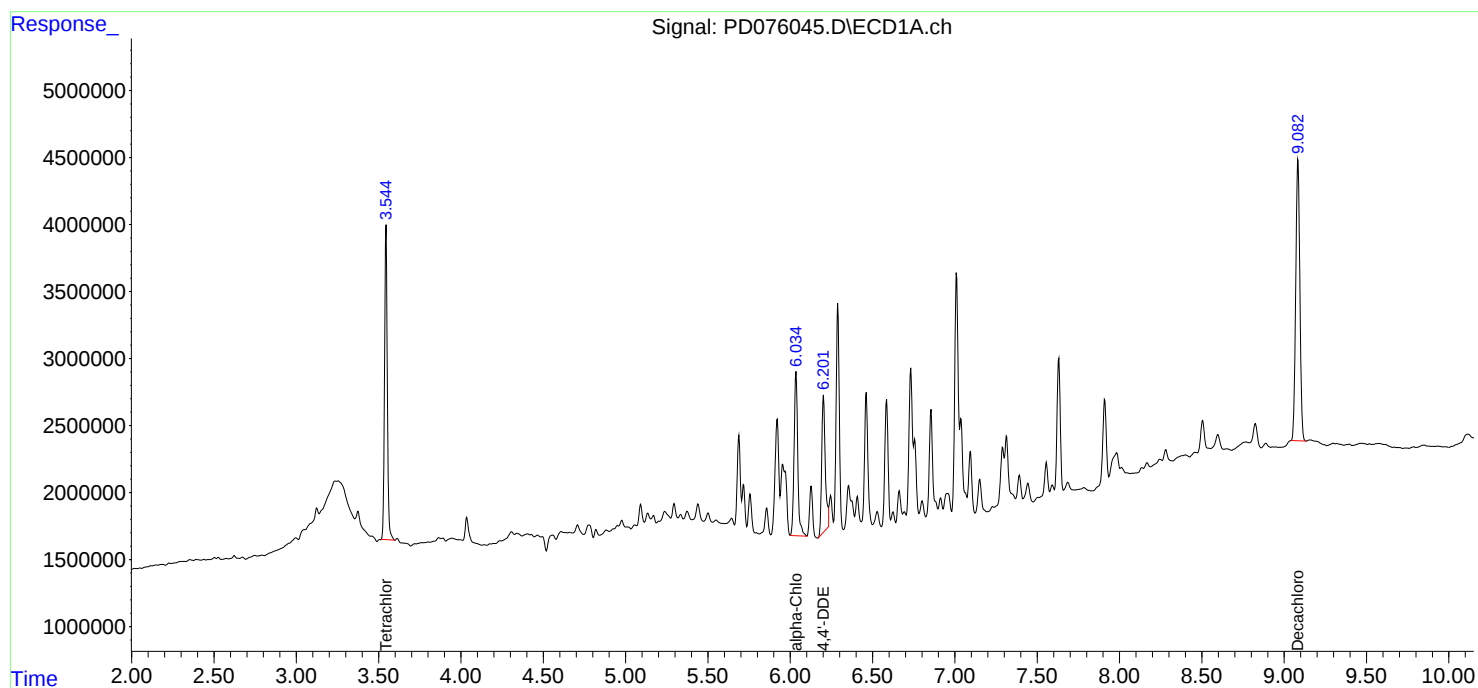

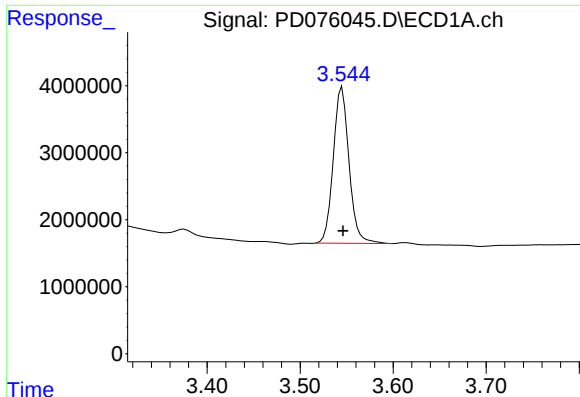


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 27435997
Conc: 12.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSITE-SB30-35


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

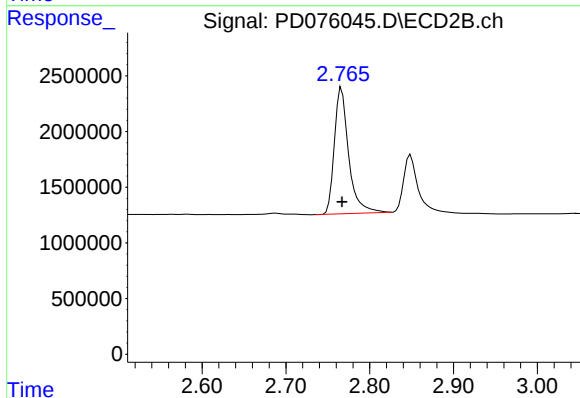


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 13436381
Conc: 12.38 ng/ml

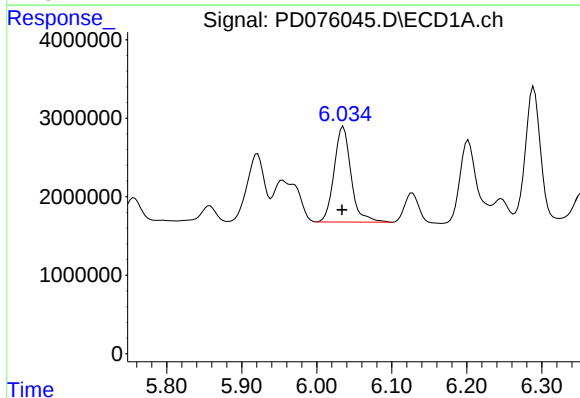


#11 alpha-Chlordane

R.T.: 6.035 min
Delta R.T.: 0.002 min
Response: 19020087
Conc: 5.88 ng/ml

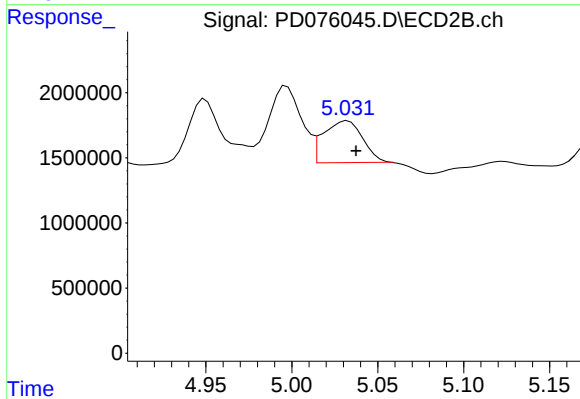

#11 alpha-Chlordane

R.T.: 5.031 min
Delta R.T.: -0.006 min
Response: 4904843
Conc: 3.58 ng/ml m

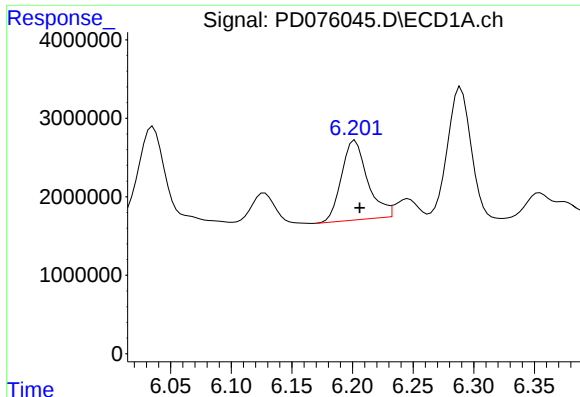


#12 4,4'-DDE

R.T.: 6.202 min
Delta R.T.: -0.004 min
Response: 15195531
Conc: 5.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSITE-SB30-35


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

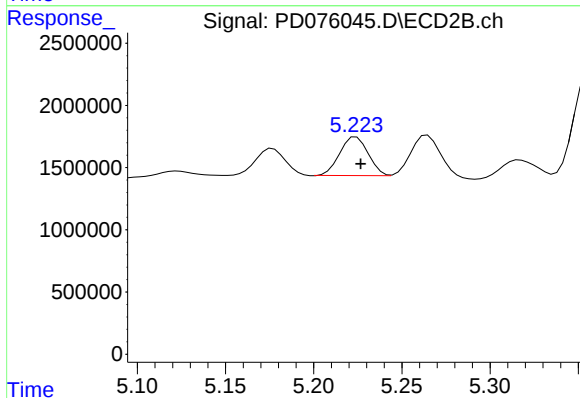


#12 4,4'-DDE

R.T.: 5.223 min
Delta R.T.: -0.004 min
Response: 3493966
Conc: 3.13 ng/ml m

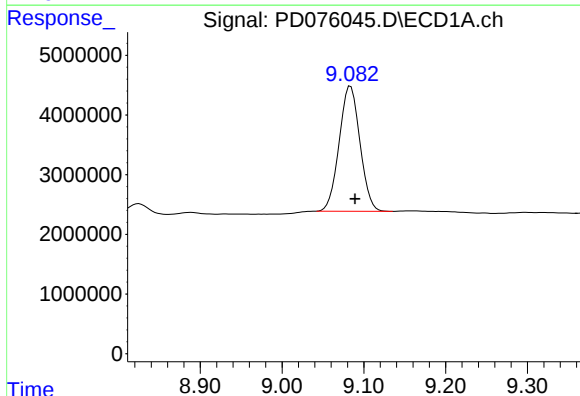

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.005 min
Response: 36897082
Conc: 14.56 ng/ml

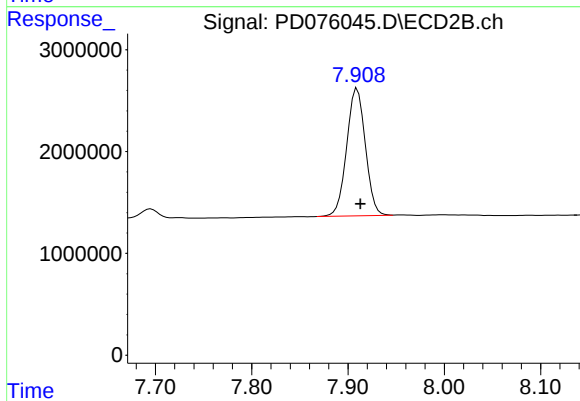

#28 Decachlorobiphenyl

R.T.: 7.908 min
Delta R.T.: -0.004 min
Response: 16821595
Conc: 17.20 ng/ml m