

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2023 16:10
 Operator : AR\AJ
 Sample : 03330-13
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMPOSITE-MC02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/23/2023
 Supervised By :Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 22:20:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	28363117	14377656	13.315	13.252
2)	SA Decachlor...	9.084	7.910	36060679	15902338	14.234	16.263
Target Compounds							
11)	B alpha-Chl...	6.036	5.033	7652037	1292283	2.367	0.942m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2023 16:10
Operator : AR\AJ
Sample : 03330-13
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMPOSITE-MC02


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/23/2023
Supervised By : Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 22:20:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

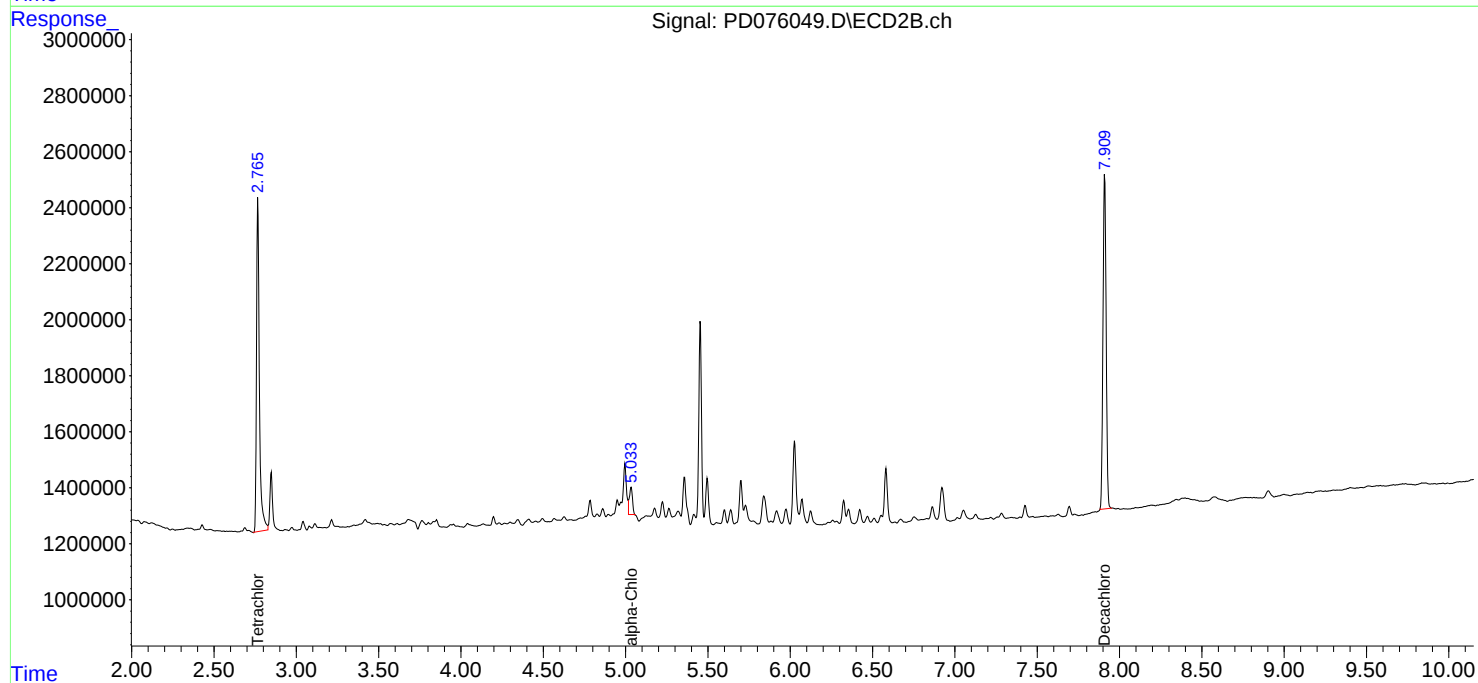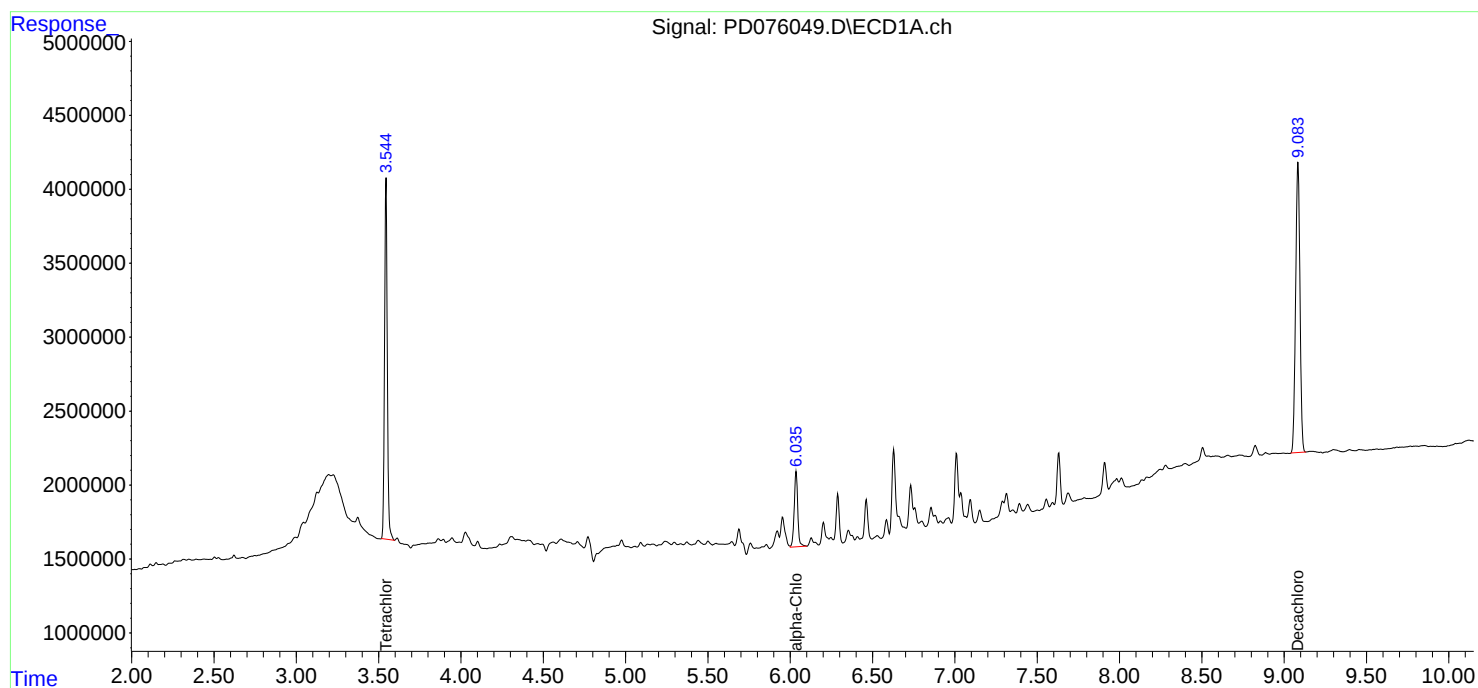

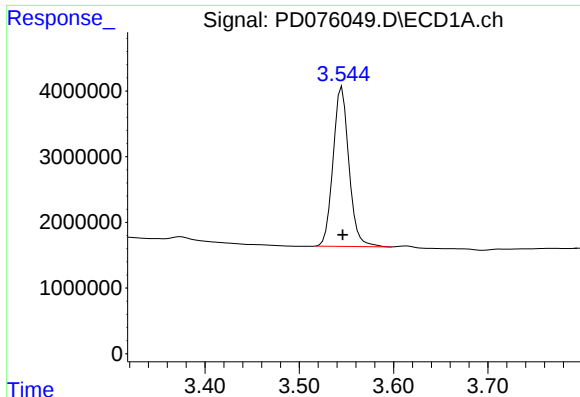

#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 28363117
Conc: 13.32 ng/ml

Instrument :

ECD_D

ClientSampleId :


COMPOSITE-MC02

Manual Integrations

APPROVED


Reviewed By :Abdul Mirza 06/23/2023

Supervised By :Ankita Jodhani 06/23/2023

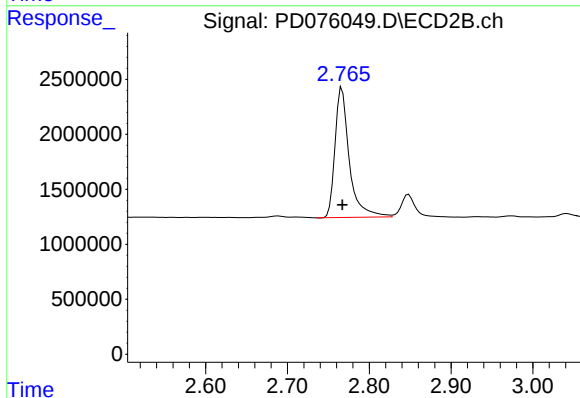


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 14377656
Conc: 13.25 ng/ml

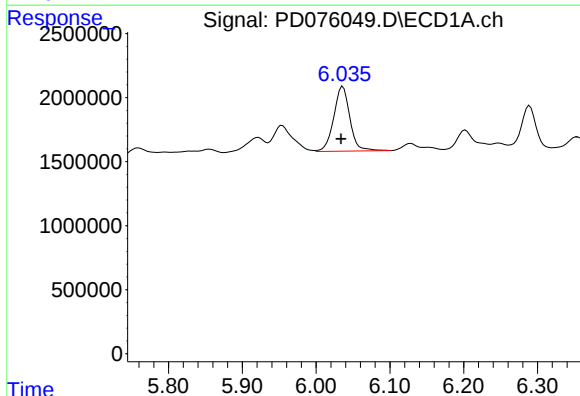


#11 alpha-Chlordane

R.T.: 6.036 min
Delta R.T.: 0.002 min
Response: 7652037
Conc: 2.37 ng/ml

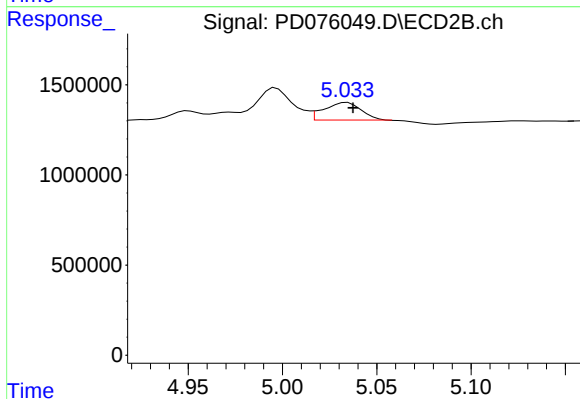

#11 alpha-Chlordane

R.T.: 5.033 min
Delta R.T.: -0.004 min
Response: 1292283
Conc: 0.94 ng/ml m

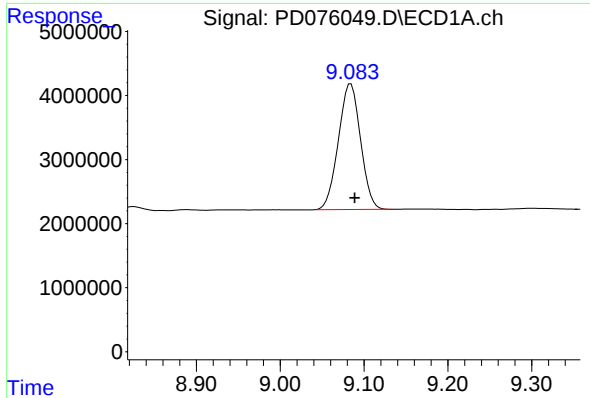


#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.005 min
Response: 36060679
Conc: 14.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSITE-MC02

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

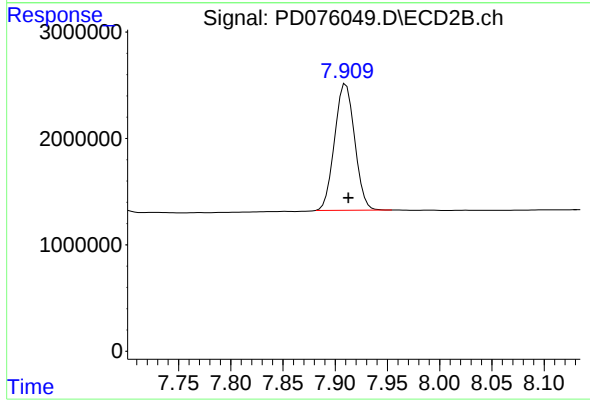

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.002 min
Response: 15902338
Conc: 16.26 ng/ml