

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD062423\  
 Data File : PD076050.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 22 Jun 2023 16:23  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 22 22:20:50 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD061523.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Jun 16 10:43:19 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.546 | 2.767 | 42348471 | 21263071 | 19.881 | 19.599 |
| 28)                         | SA Decachlor... | 9.085 | 7.910 | 49020350 | 21663271 | 19.350 | 22.155 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD062423\  
Data File : PD076050.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 22 Jun 2023 16:23  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 22 22:20:50 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD061523.M  
Quant Title : GC Extractables  
QLast Update : Fri Jun 16 10:43:19 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

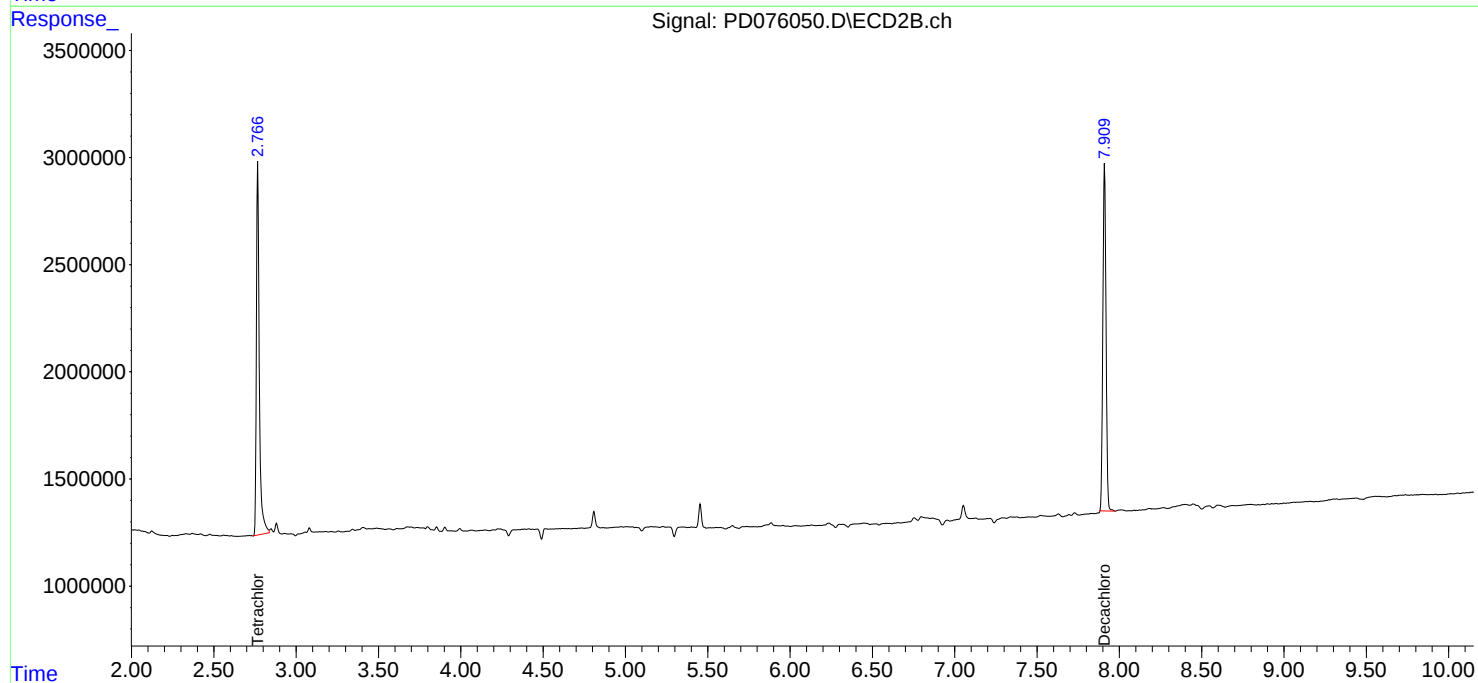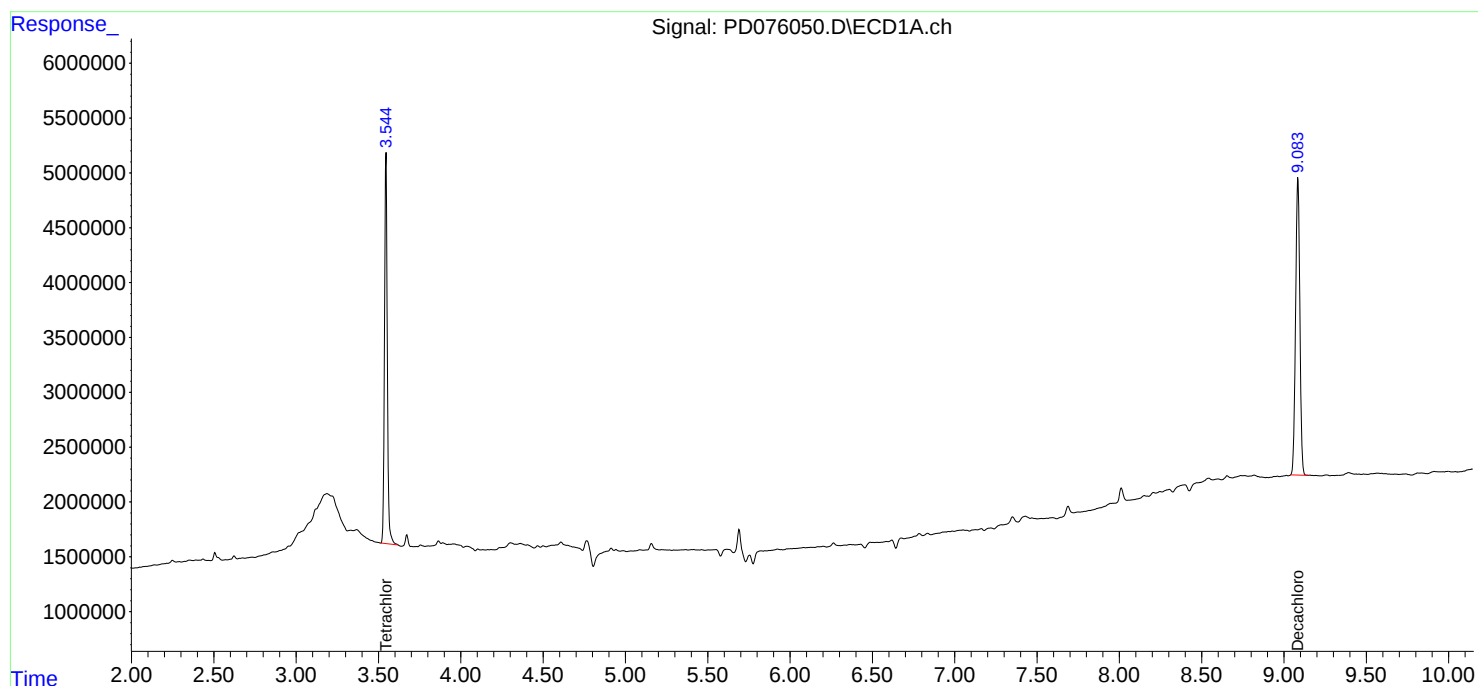


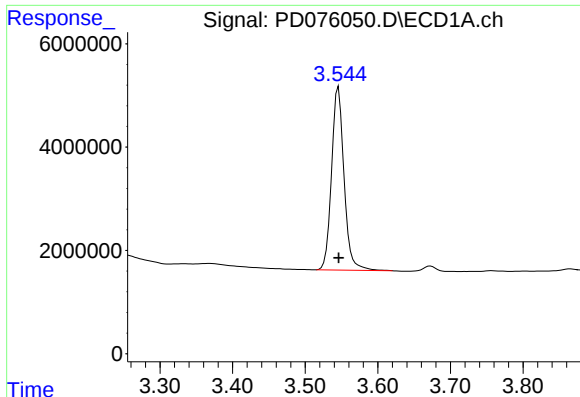

#1 Tetrachloro-m-xylene


R.T.: 3.546 min  
Delta R.T.: 0.000 min  
Response: 42348471  
Conc: 19.88 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

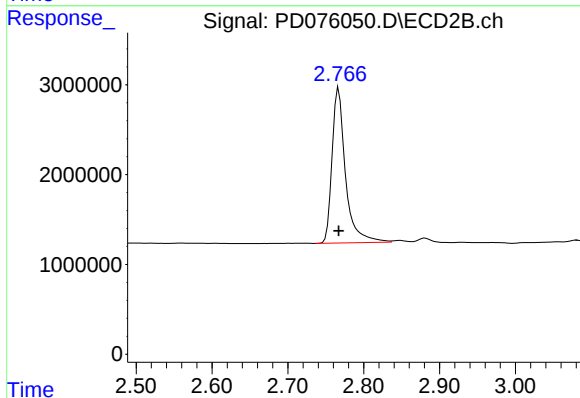


#1 Tetrachloro-m-xylene

R.T.: 2.767 min  
Delta R.T.: 0.000 min  
Response: 21263071  
Conc: 19.60 ng/ml

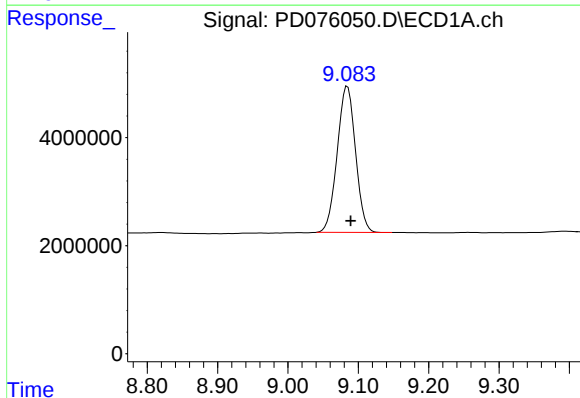

#28 Decachlorobiphenyl

R.T.: 9.085 min  
Delta R.T.: -0.005 min  
Response: 49020350  
Conc: 19.35 ng/ml

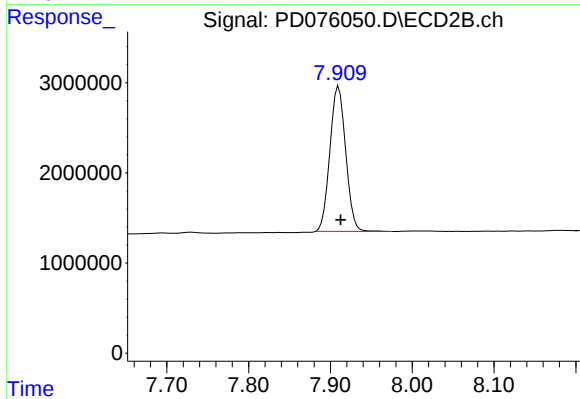

#28 Decachlorobiphenyl

R.T.: 7.910 min  
Delta R.T.: -0.002 min  
Response: 21663271  
Conc: 22.16 ng/ml