

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
 Data File : PD076080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 00:08
 Operator : AR\AJ
 Sample : 03358-12
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DUP-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/23/2023
 Supervised By :Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 07:39:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.767	23178281	11896366	10.881	10.965
28)	SA Decachlor...	9.084	7.910	27297153	12423277	10.775	12.705
Target Compounds							
11)	B alpha-Chl...	6.036	5.034	5796508	911776	1.793	0.665m#
12)	B 4,4'-DDE	6.203	5.225	8715879	3700710	3.049	3.316
16)	A 4,4'-DDD	6.726	5.780	1510534	523472	0.664	0.594
17)	MA 4,4'-DDT	7.037	6.031	10854452	4553790	4.783	5.606

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062423\
Data File : PD076080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 00:08
Operator : AR\AJ
Sample : 03358-12
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/23/2023
Supervised By : Ankita Jodhani 06/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 07:39:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

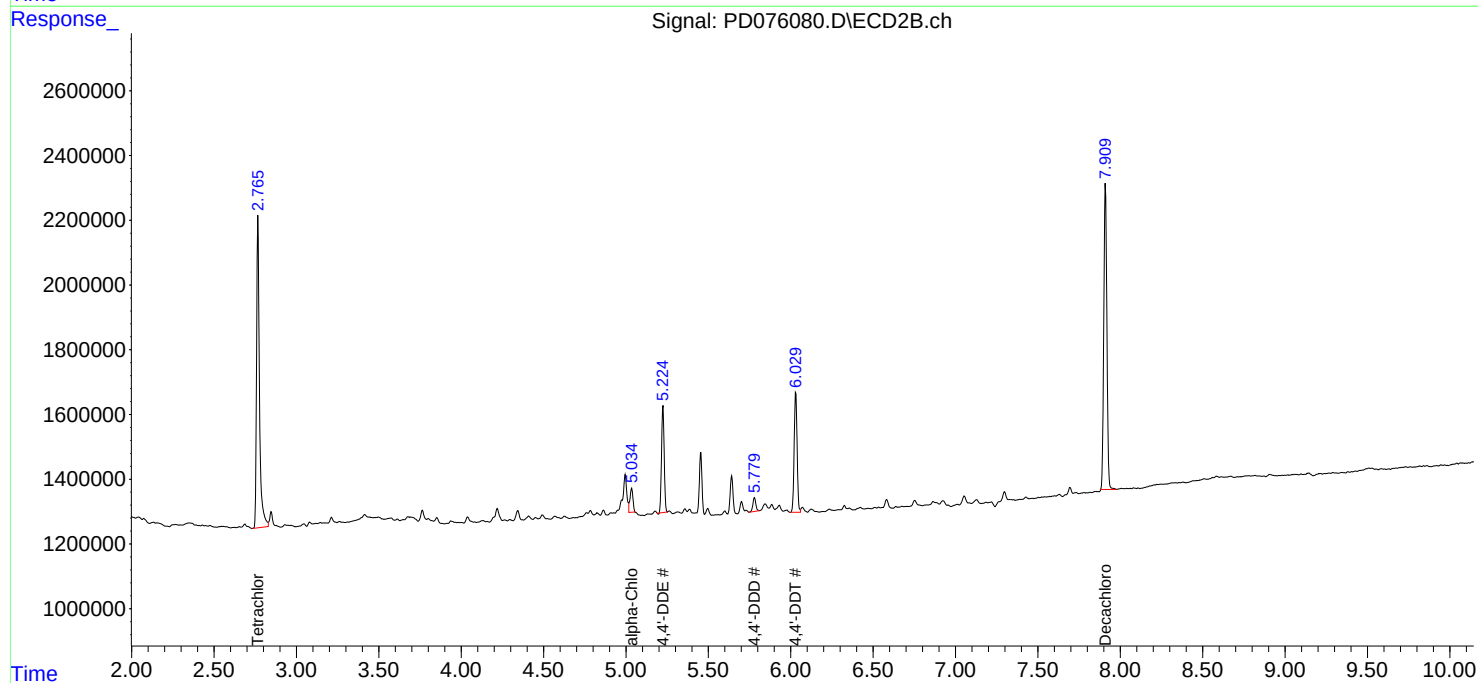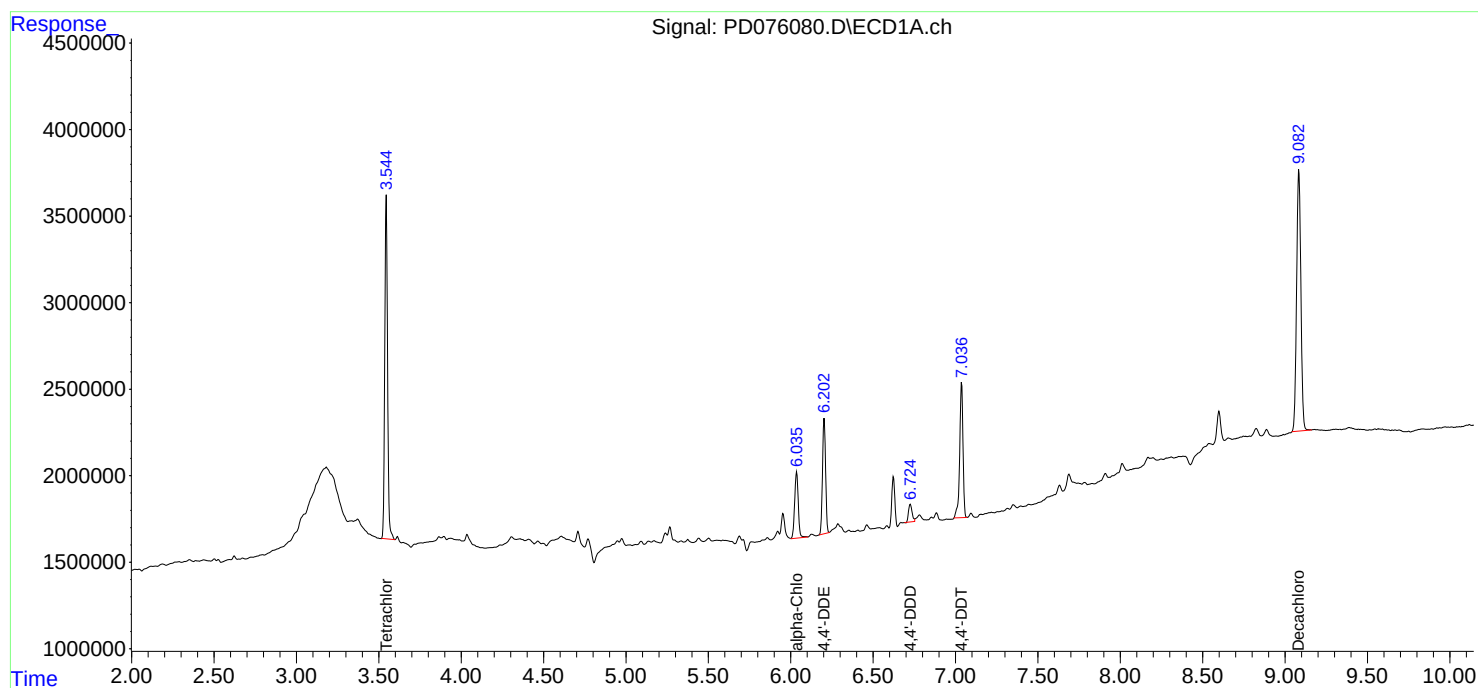

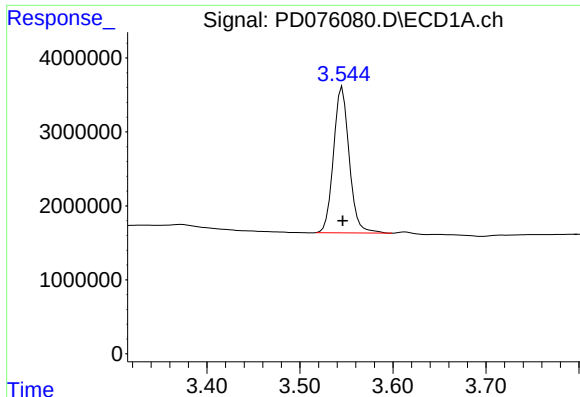


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 23178281
Conc: 10.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

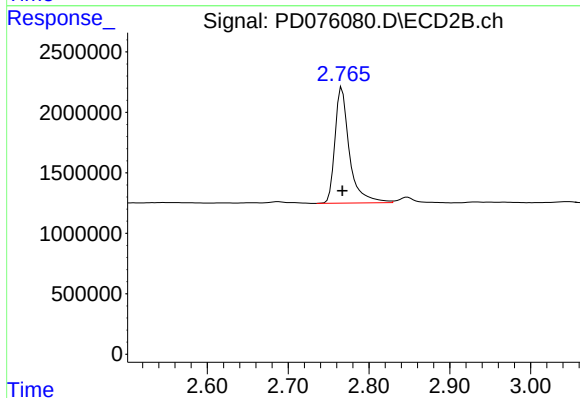


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 11896366
Conc: 10.97 ng/ml

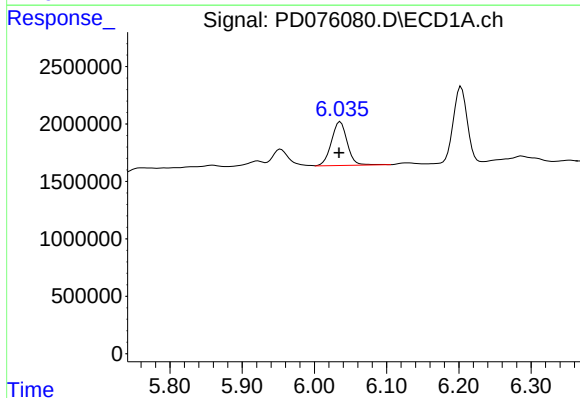


#11 alpha-Chlordane

R.T.: 6.036 min
Delta R.T.: 0.002 min
Response: 5796508
Conc: 1.79 ng/ml

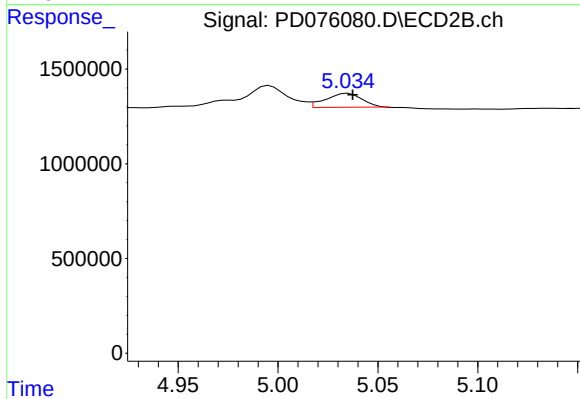

#11 alpha-Chlordane

R.T.: 5.034 min
Delta R.T.: -0.004 min
Response: 911776
Conc: 0.66 ng/ml m

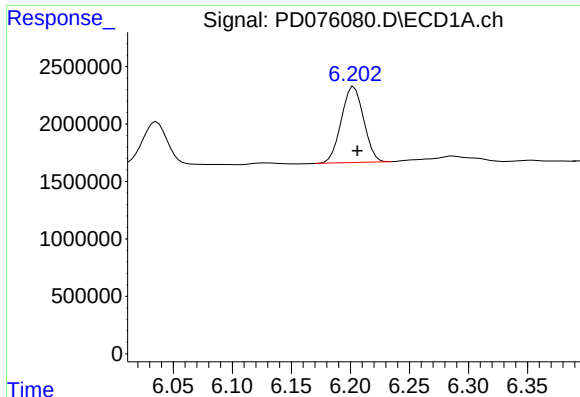


#12 4,4'-DDE

R.T.: 6.203 min
Delta R.T.: -0.003 min
Response: 8715879
Conc: 3.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

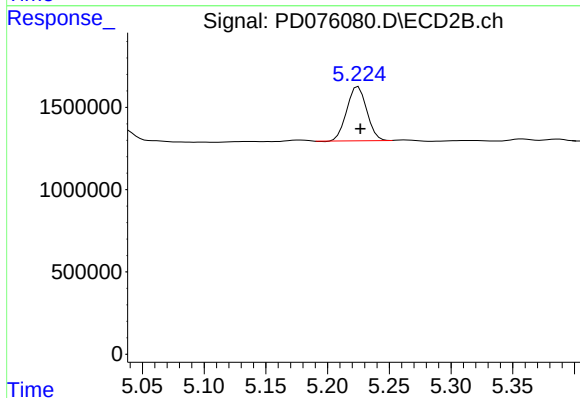


#12 4,4'-DDE

R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 3700710
Conc: 3.32 ng/ml

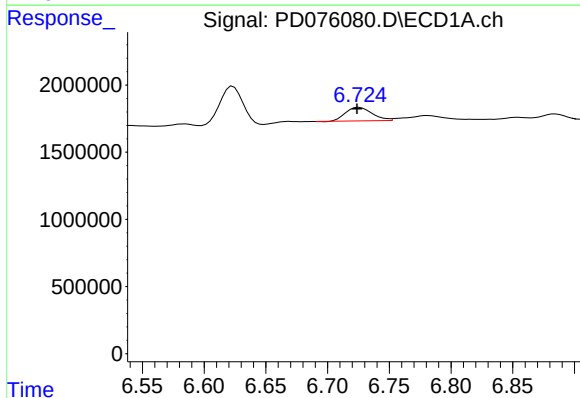


#16 4,4'-DDD

R.T.: 6.726 min
Delta R.T.: 0.002 min
Response: 1510534
Conc: 0.66 ng/ml

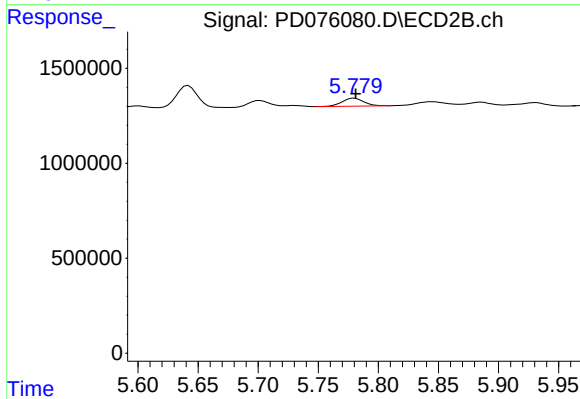

#16 4,4'-DDD

R.T.: 5.780 min
Delta R.T.: 0.000 min
Response: 523472
Conc: 0.59 ng/ml

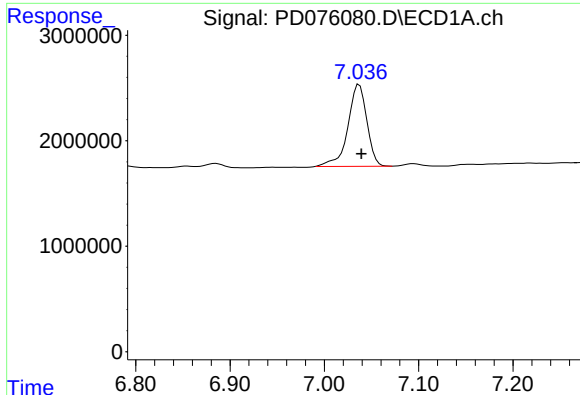


#17 4,4'-DDT

R.T.: 7.037 min
Delta R.T.: -0.003 min
Response: 10854452
Conc: 4.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
DUP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/23/2023
Supervised By :Ankita Jodhani 06/23/2023

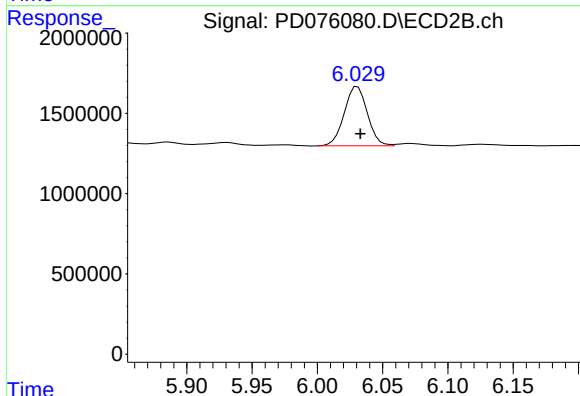


#17 4,4'-DDT

R.T.: 6.031 min
Delta R.T.: -0.002 min
Response: 4553790
Conc: 5.61 ng/ml

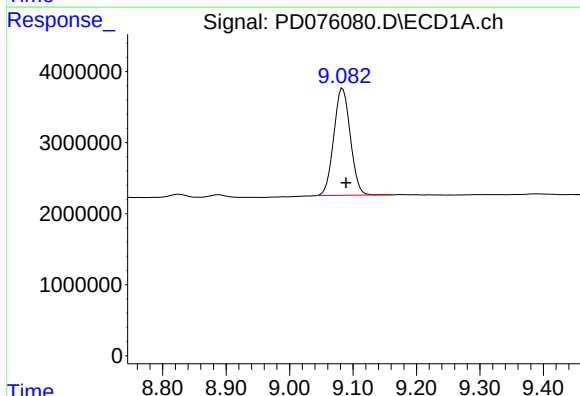

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.005 min
Response: 27297153
Conc: 10.78 ng/ml

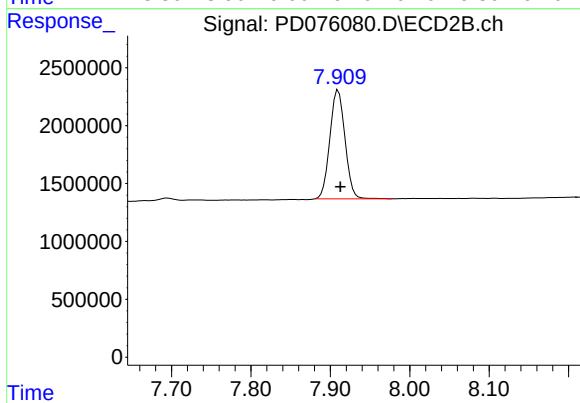

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.003 min
Response: 12423277
Conc: 12.71 ng/ml