

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
 Data File : PD083798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 15:34
 Operator : AR\AJ
 Sample : P2961-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:37:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.563	2.773	20226427	106.9E6	15.495	19.611 #
27)	SA Decachlor...	9.119	7.899	37985656	127.0E6	19.535	20.922
Target Compounds							
10)	B trans-Chl...	0.000	5.010f	0 28774780	N.D.	3.962	
11)	B cis-Chlor...	0.000	5.010	0 28774780	N.D.	3.908	
22)	Toxaphene-1	5.844f	5.010	2036992 28774780	336.413	794.683	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
Data File : PD083798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 15:34
Operator : AR\AJ
Sample : P2961-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:37:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

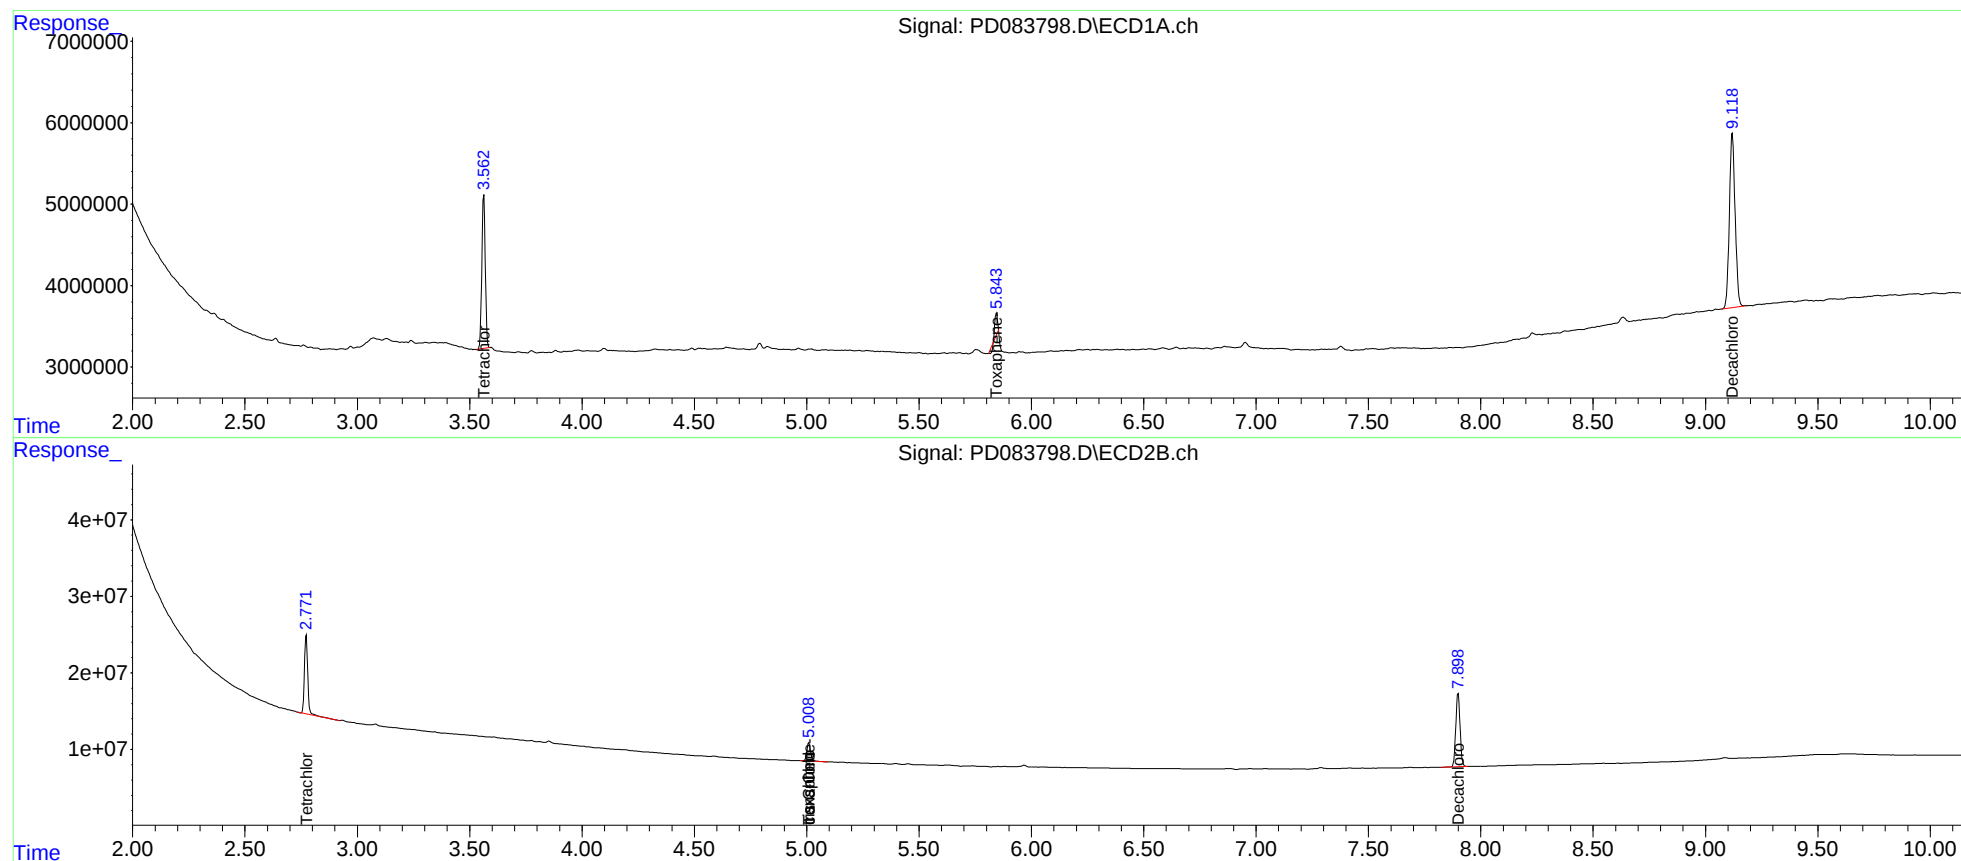

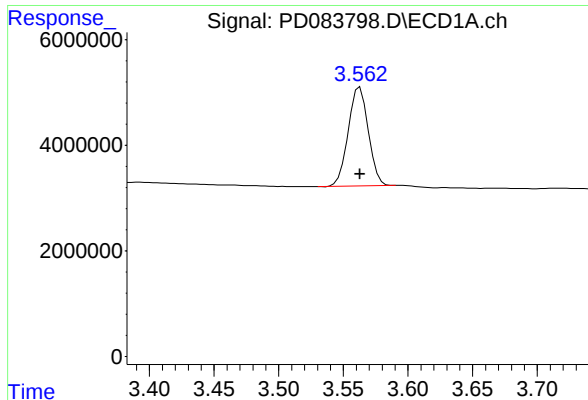


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 20226427
Conc: 15.50 ng/ml

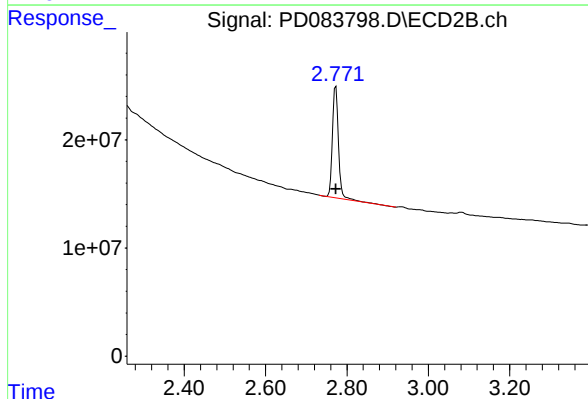


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 106901896
Conc: 19.61 ng/ml

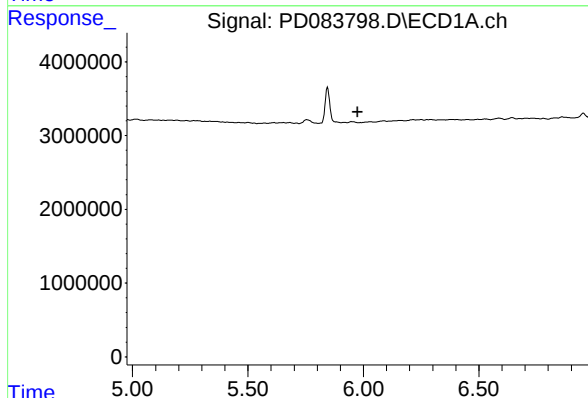


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.975 min
Response: 0
Conc: N.D.

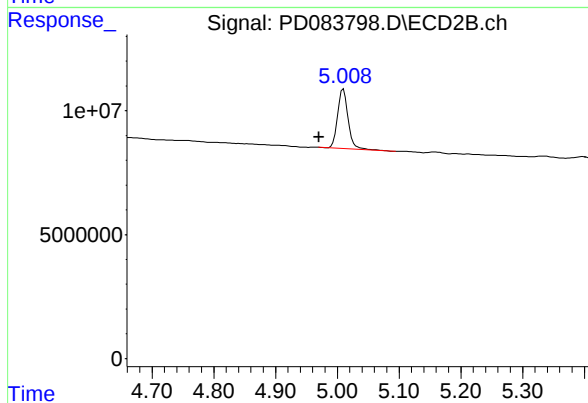


#10 trans-Chlordane

R.T.: 5.010 min
Delta R.T.: 0.040 min
Response: 28774780
Conc: 3.96 ng/ml

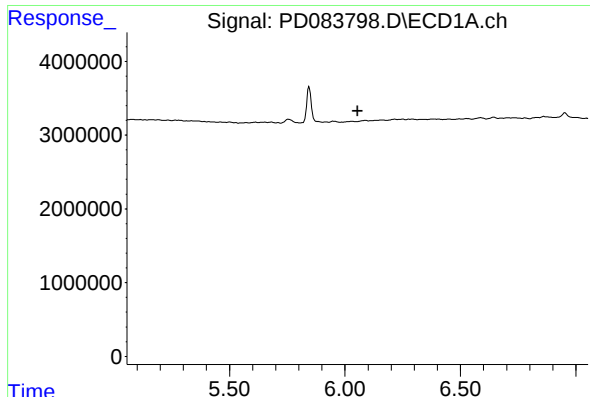


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.055 min
Response: 0
Conc: N.D.

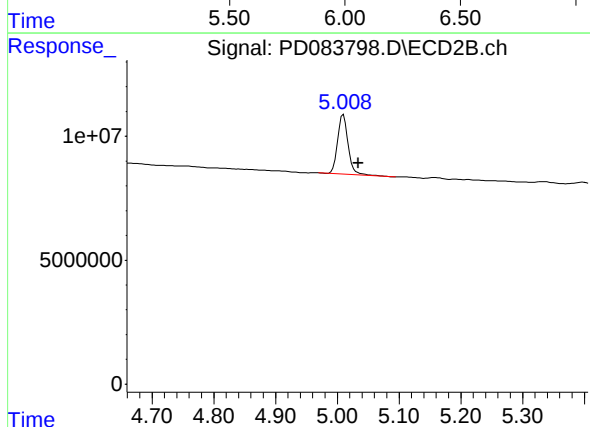


#11 cis-Chlordane

R.T.: 5.010 min
Delta R.T.: -0.024 min
Response: 28774780
Conc: 3.91 ng/ml

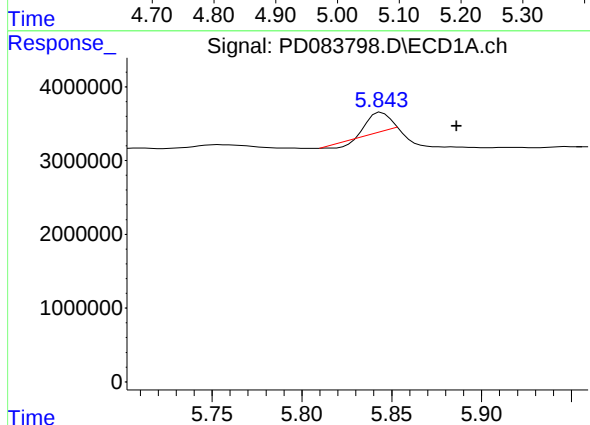


#22 Toxaphene-1

R.T.: 5.844 min
Delta R.T.: -0.042 min
Response: 2036992
Conc: 336.41 ng/ml

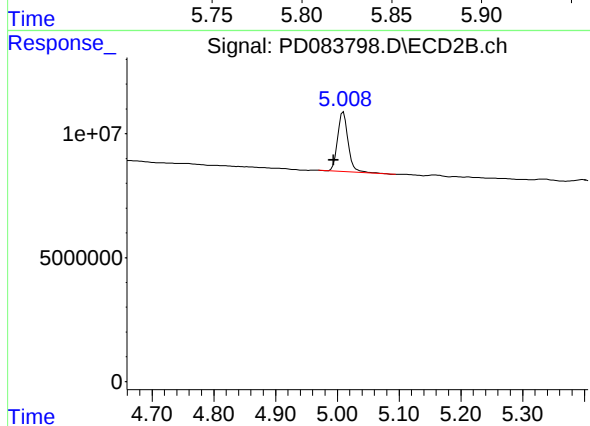


#22 Toxaphene-1

R.T.: 5.010 min
Delta R.T.: 0.015 min
Response: 28774780
Conc: 794.68 ng/ml

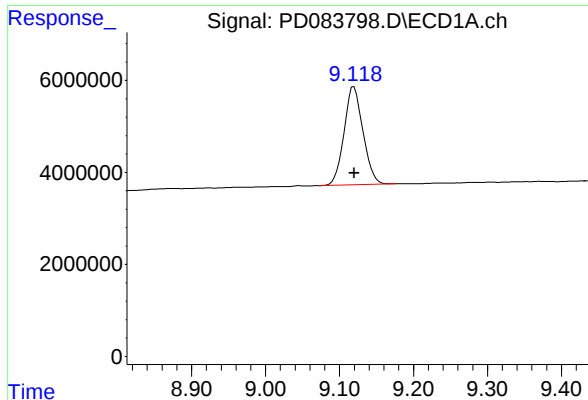

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.000 min
Response: 37985656
Conc: 19.53 ng/ml

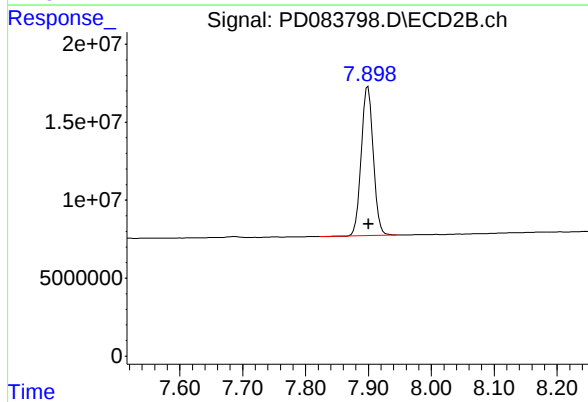

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.001 min
Response: 127042512
Conc: 20.92 ng/ml