

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
 Data File : PD083799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 15:47
 Operator : AR\AJ
 Sample : P2961-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:37:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.771	21152741	111.6E6	16.205	20.465 #
27)	SA Decachlor...	9.120	7.898	38746947	128.0E6	19.926	21.081
Target Compounds							
10)	B trans-Chl...	0.000	5.009f	0 16908551	N.D.		2.328
11)	B cis-Chlor...	0.000	5.009	0 16908551	N.D.		2.297
22)	Toxaphene-1	5.844f	5.009	718667 16908551	118.689		466.969 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
Data File : PD083799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 15:47
Operator : AR\AJ
Sample : P2961-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:37:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

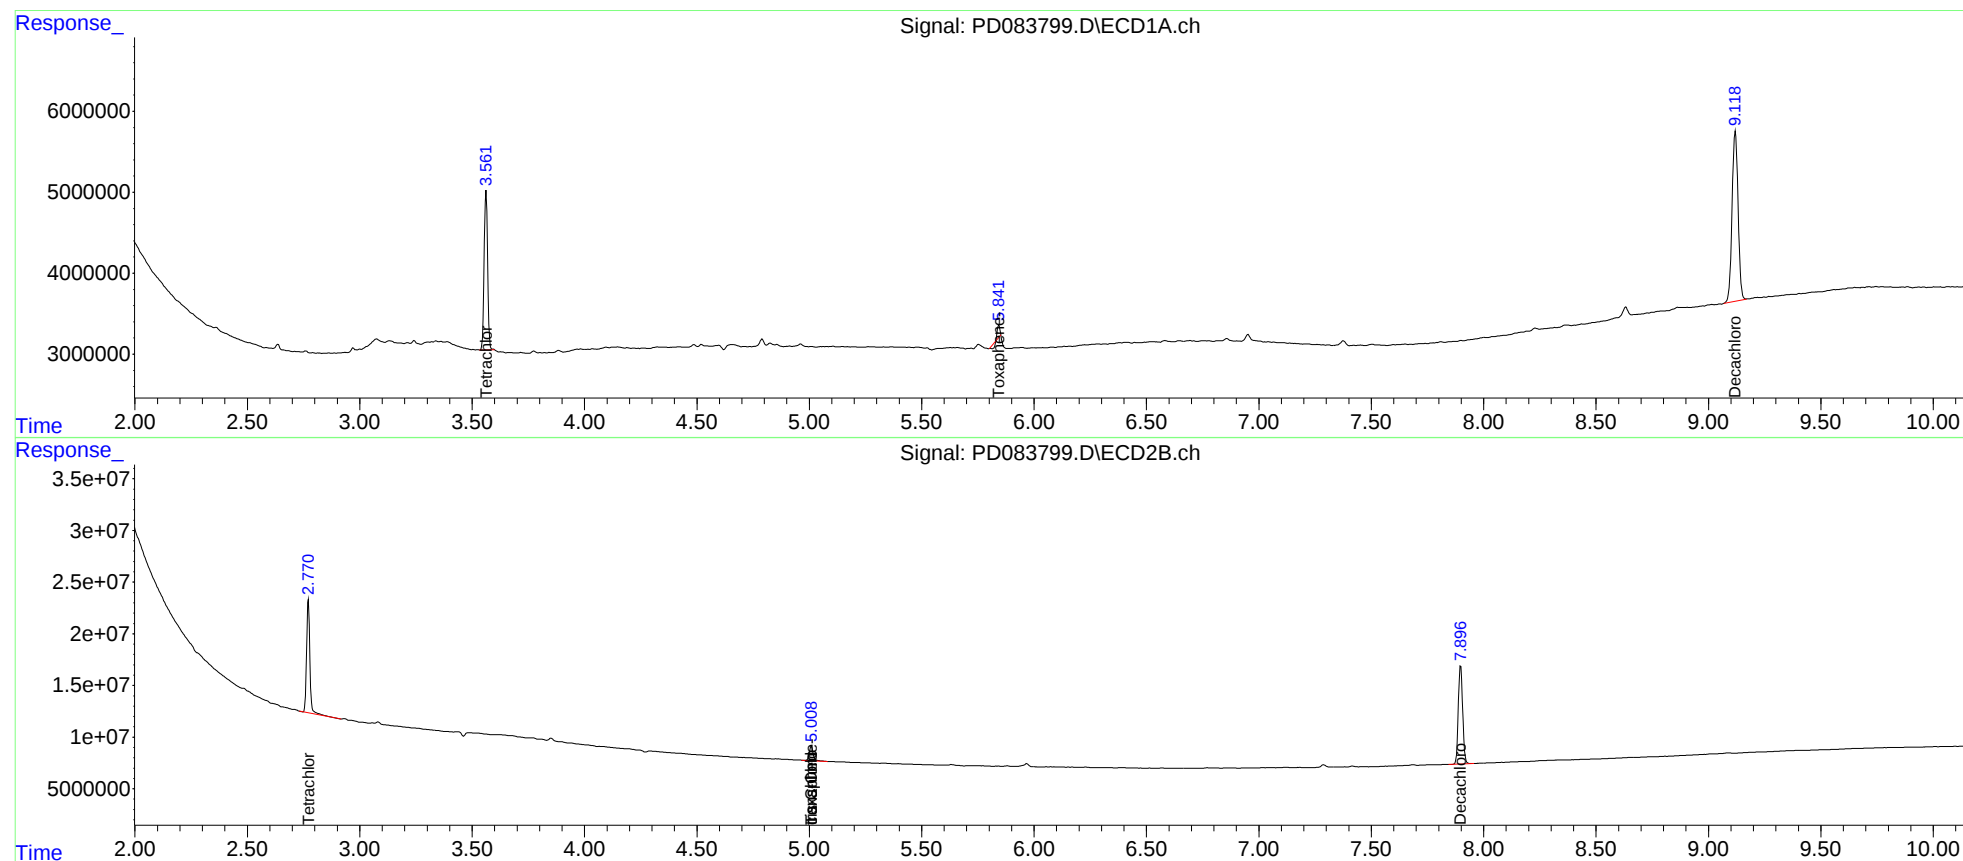

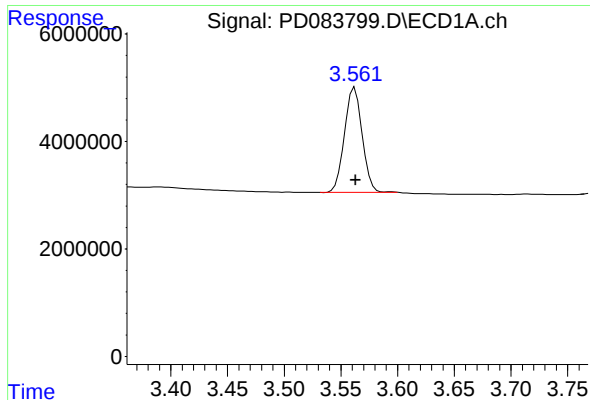


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 21152741
Conc: 16.21 ng/ml

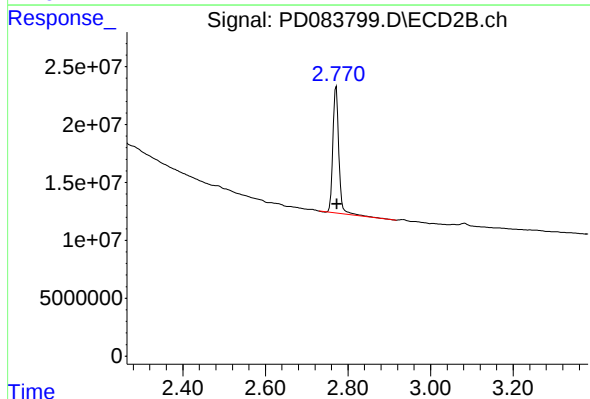


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.002 min
Response: 111556306
Conc: 20.47 ng/ml

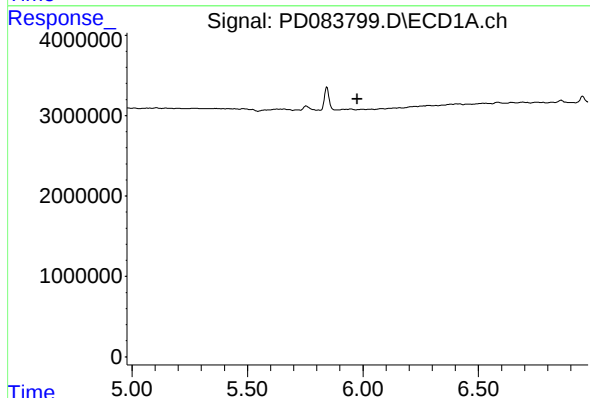


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.975 min
Response: 0
Conc: N.D.

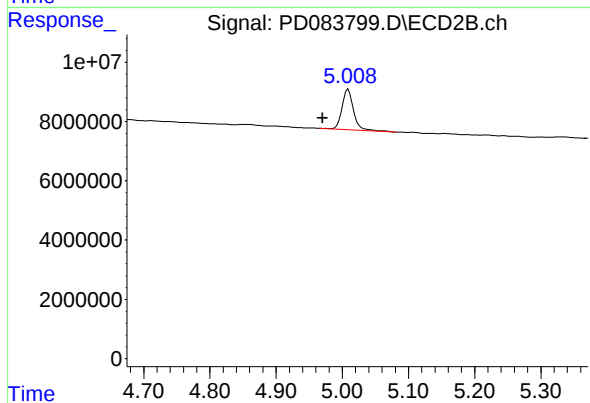


#10 trans-Chlordane

R.T.: 5.009 min
Delta R.T.: 0.039 min
Response: 16908551
Conc: 2.33 ng/ml

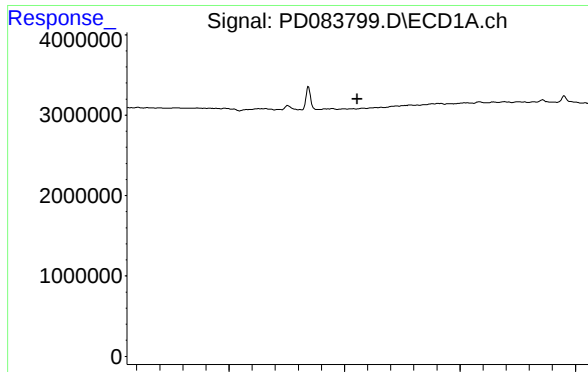


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.055 min
Response: 0
Conc: N.D.

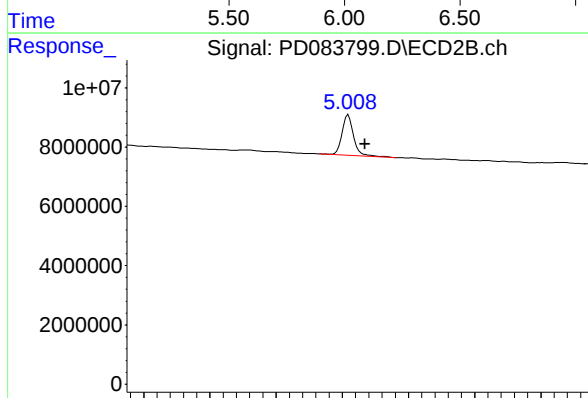


#11 cis-Chlordane

R.T.: 5.009 min
Delta R.T.: -0.025 min
Response: 16908551
Conc: 2.30 ng/ml

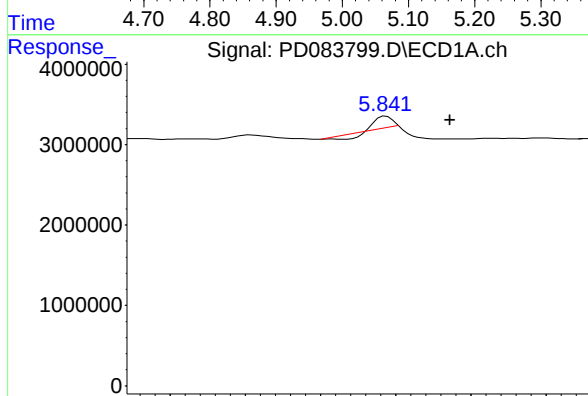


#22 Toxaphene-1

R.T.: 5.844 min
Delta R.T.: -0.043 min
Response: 718667
Conc: 118.69 ng/ml

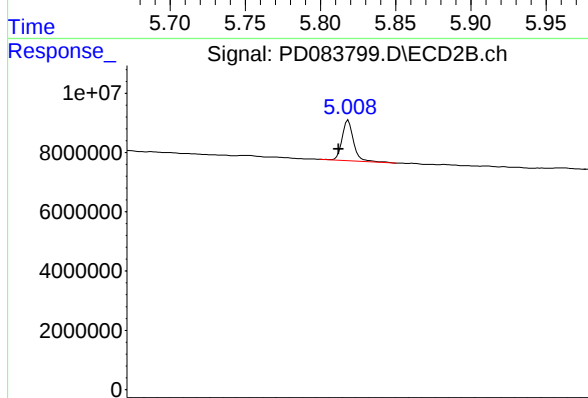


#22 Toxaphene-1

R.T.: 5.009 min
Delta R.T.: 0.015 min
Response: 16908551
Conc: 466.97 ng/ml

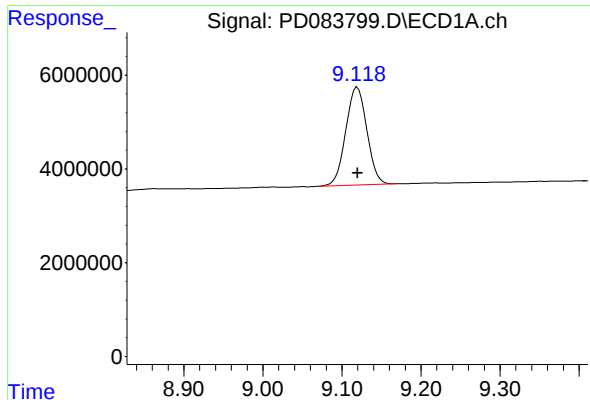

#27 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: 0.000 min
Response: 38746947
Conc: 19.93 ng/ml

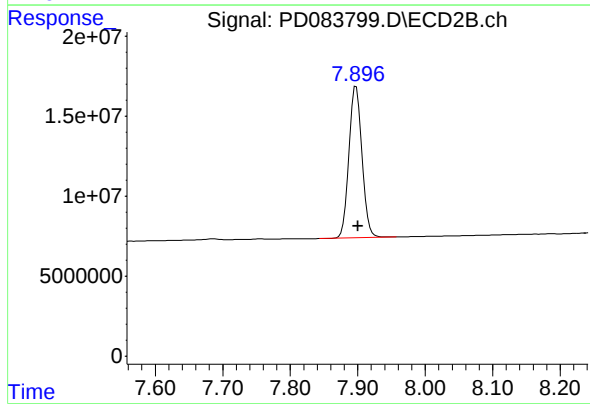

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.003 min
Response: 128005216
Conc: 21.08 ng/ml