

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
 Data File : PD083801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 16:14
 Operator : AR\AJ
 Sample : P2961-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:37:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.771	20533242	131.2E6	15.731	24.064 #
27)	SA Decachlor...	9.121	7.899	37896123	125.9E6	19.489	20.732
Target Compounds							
4)	MA Heptachlor	4.933	0.000	3541732	0	1.458	N.D. #
5)	MB Aldrin	0.000	4.238	0	36537211	N.D.	4.728
6)	B beta-BHC	0.000	3.851f	0	222.8E6	N.D.	62.441
7)	B delta-BHC	4.790	0.000	76574519	0	29.150	N.D. #
10)	B trans-Chl...	0.000	5.009f	0	16871867	N.D.	2.323
11)	B cis-Chlor...	0.000	5.009	0	16871867	N.D.	2.292
22)	Toxaphene-1	5.844f	5.009	1040586	16871867	171.855	465.956 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
Data File : PD083801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 16:14
Operator : AR\AJ
Sample : P2961-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:37:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

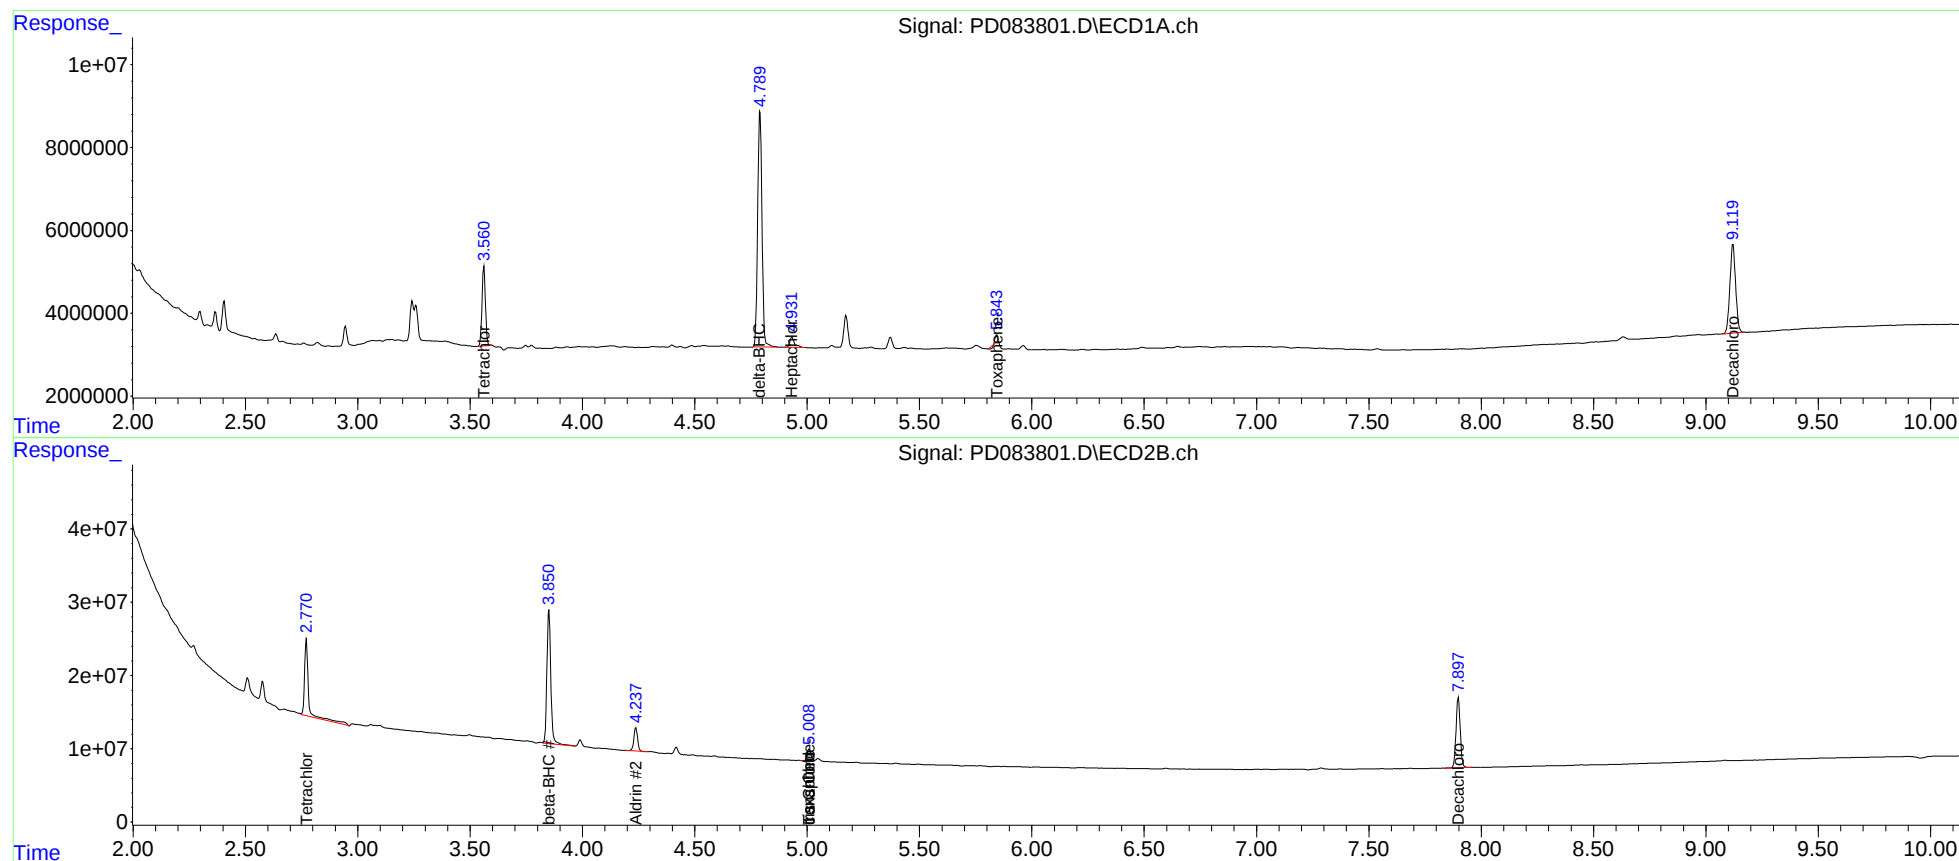

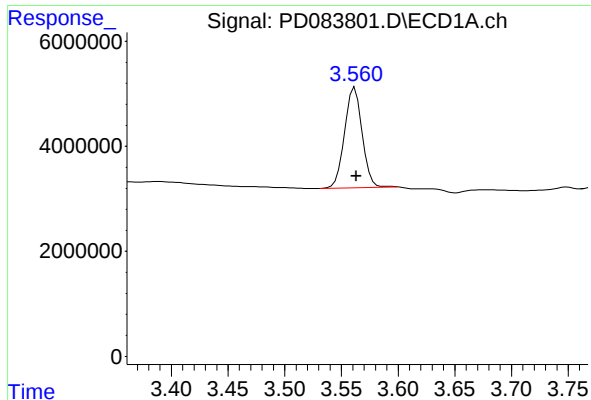


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.001 min
Response: 20533242
Conc: 15.73 ng/ml

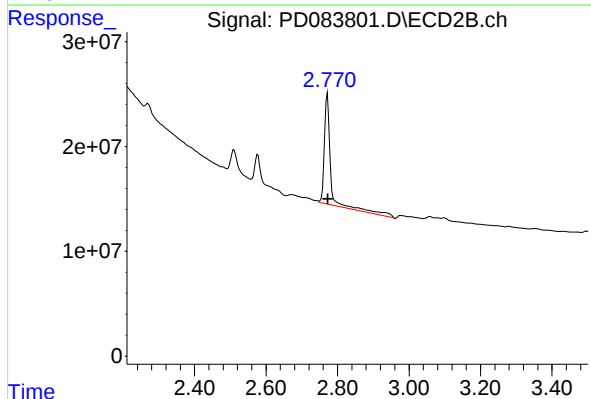


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.002 min
Response: 131174832
Conc: 24.06 ng/ml

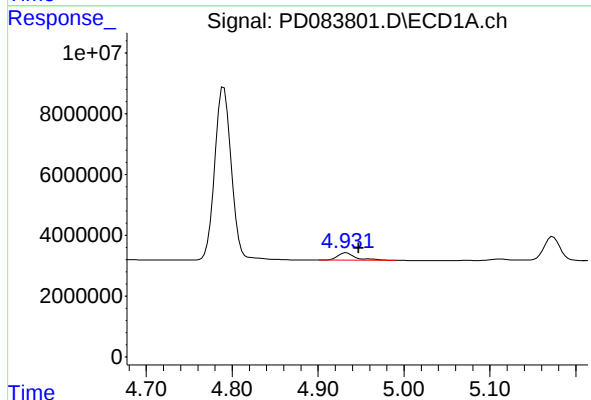


#4 Heptachlor

R.T.: 4.933 min
Delta R.T.: -0.015 min
Response: 3541732
Conc: 1.46 ng/ml

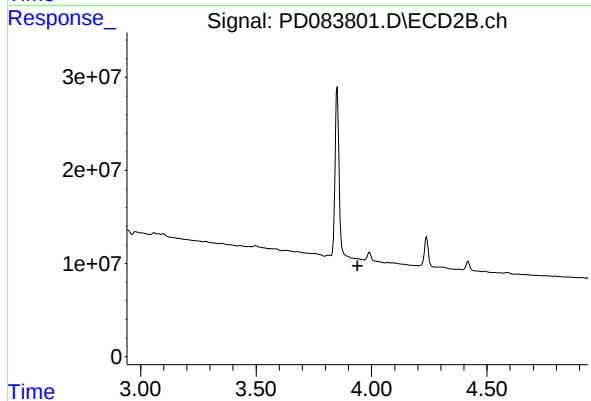


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 3.940 min
Response: 0
Conc: N.D.

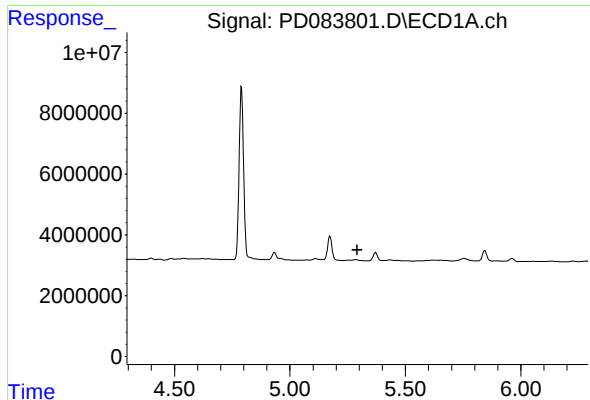


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.291 min
Response: 0
Conc: N.D.

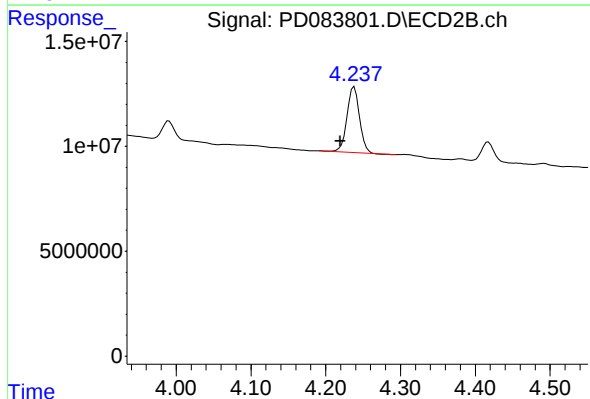


#5 Aldrin

R.T.: 4.238 min
Delta R.T.: 0.019 min
Response: 36537211
Conc: 4.73 ng/ml

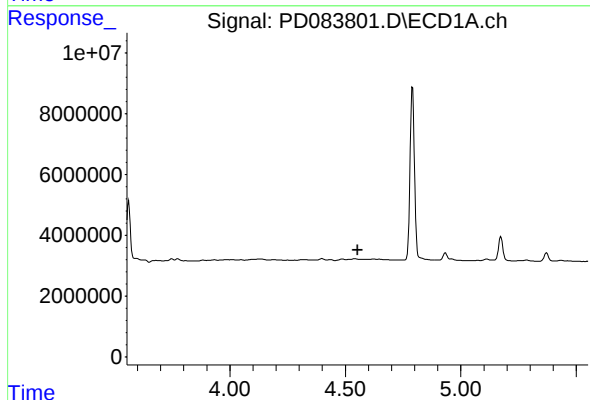


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.552 min
Response: 0
Conc: N.D.

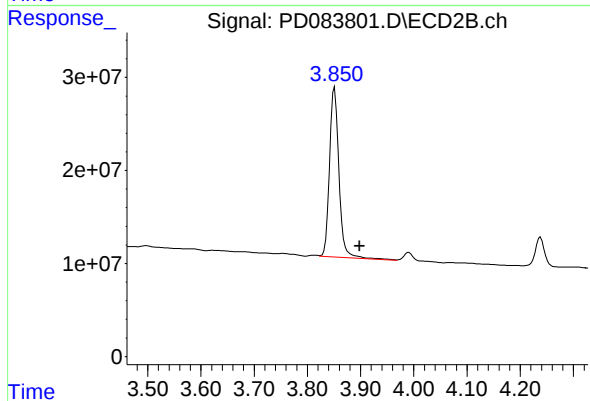


#6 beta-BHC

R.T.: 3.851 min
Delta R.T.: -0.047 min
Response: 222803434
Conc: 62.44 ng/ml

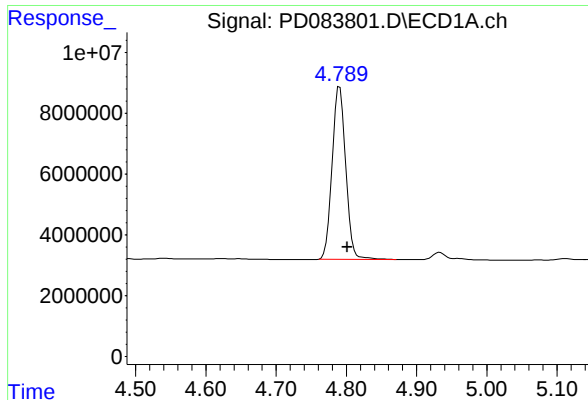


#7 delta-BHC

R.T.: 4.790 min
Delta R.T.: -0.011 min
Response: 76574519
Conc: 29.15 ng/ml

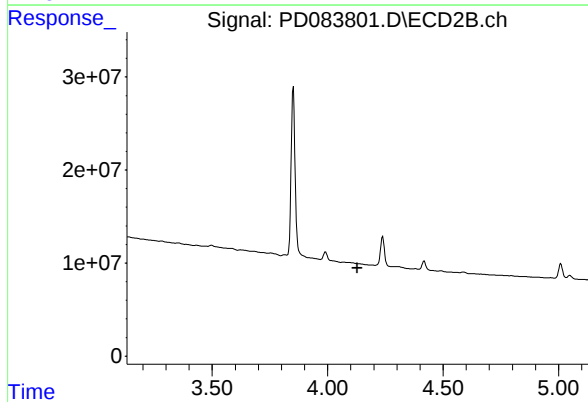


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.128 min
Response: 0
Conc: N.D.

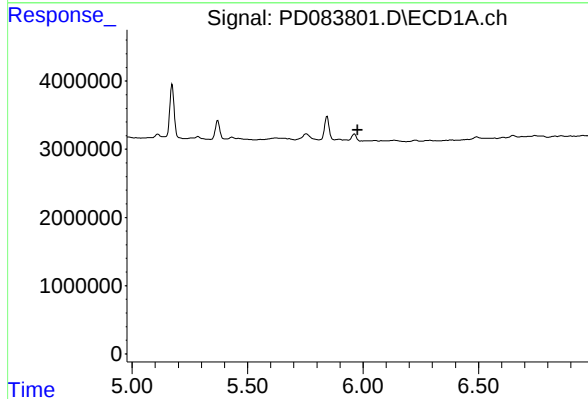


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.975 min
Response: 0
Conc: N.D.

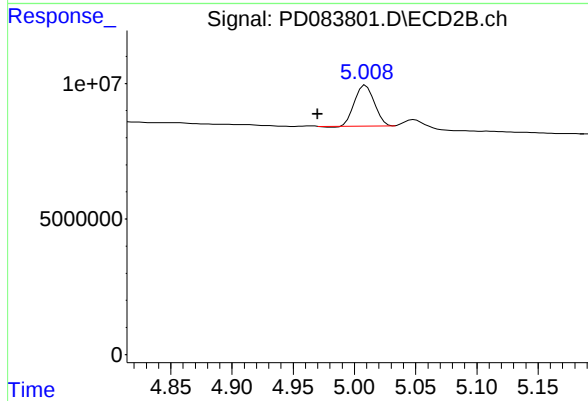


#10 trans-Chlordane

R.T.: 5.009 min
Delta R.T.: 0.039 min
Response: 16871867
Conc: 2.32 ng/ml

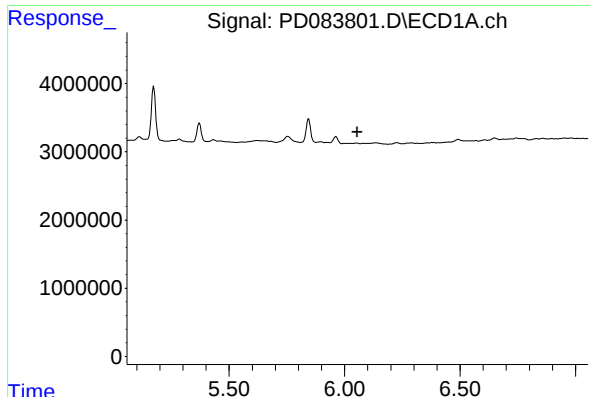


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.055 min
Response: 0
Conc: N.D.

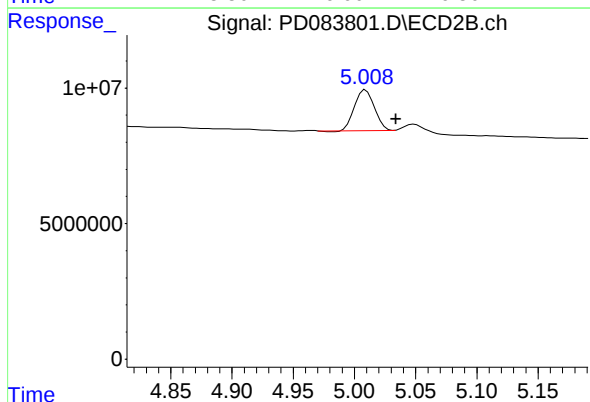


#11 cis-Chlordane

R.T.: 5.009 min
Delta R.T.: -0.025 min
Response: 16871867
Conc: 2.29 ng/ml

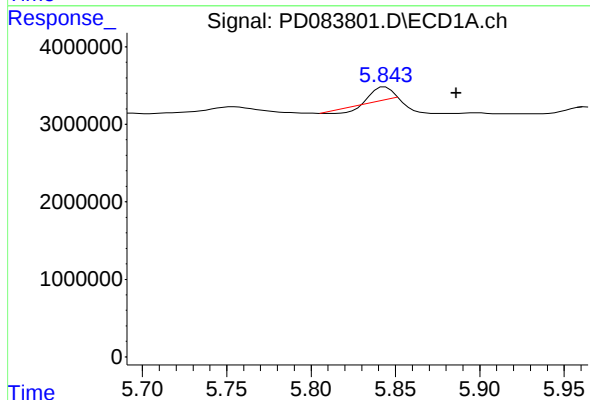


#22 Toxaphene-1

R.T.: 5.844 min
Delta R.T.: -0.042 min
Response: 1040586
Conc: 171.85 ng/ml

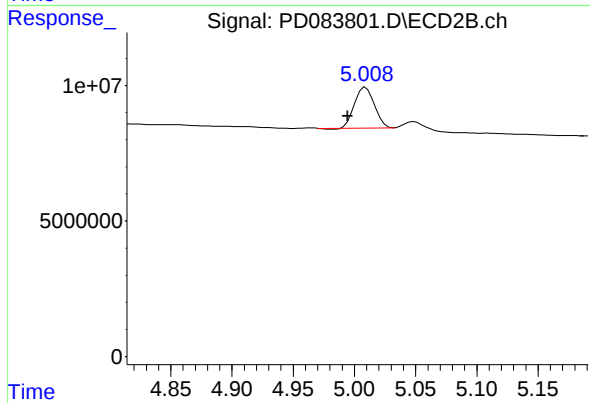


#22 Toxaphene-1

R.T.: 5.009 min
Delta R.T.: 0.015 min
Response: 16871867
Conc: 465.96 ng/ml

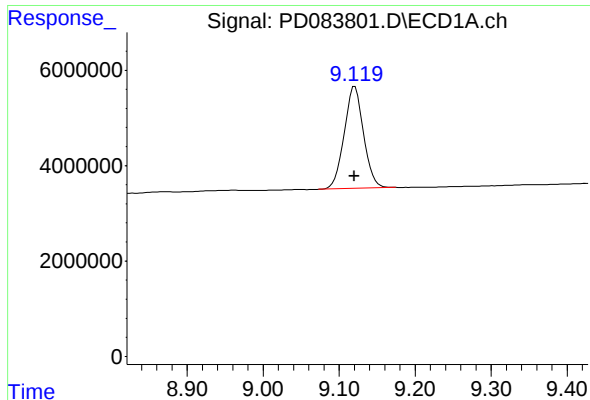

#27 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 37896123
Conc: 19.49 ng/ml

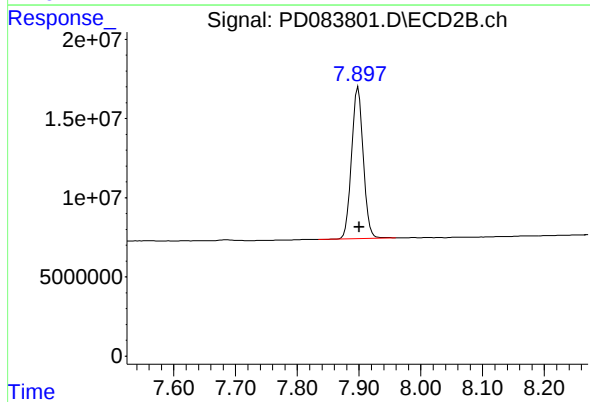

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.002 min
Response: 125886196
Conc: 20.73 ng/ml