

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
 Data File : PD083808.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2024 17:34
 Operator : AR\AJ
 Sample : P2961-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:38:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.562	2.772	20386809	108.7E6	15.618	19.934 #
27)	SA Decachlor...	9.118	7.898	27242850	89592401	14.010	14.755
Target Compounds							
10)	B trans-Chl...	0.000	5.009f	0	9787928	N.D.	1.348
11)	B cis-Chlor...	0.000	5.009	0	9787928	N.D.	1.329
22)	Toxaphene-1	5.843f	5.009	668279	9787928	110.368	270.317 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
Data File : PD083808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 17:34
Operator : AR\AJ
Sample : P2961-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:38:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

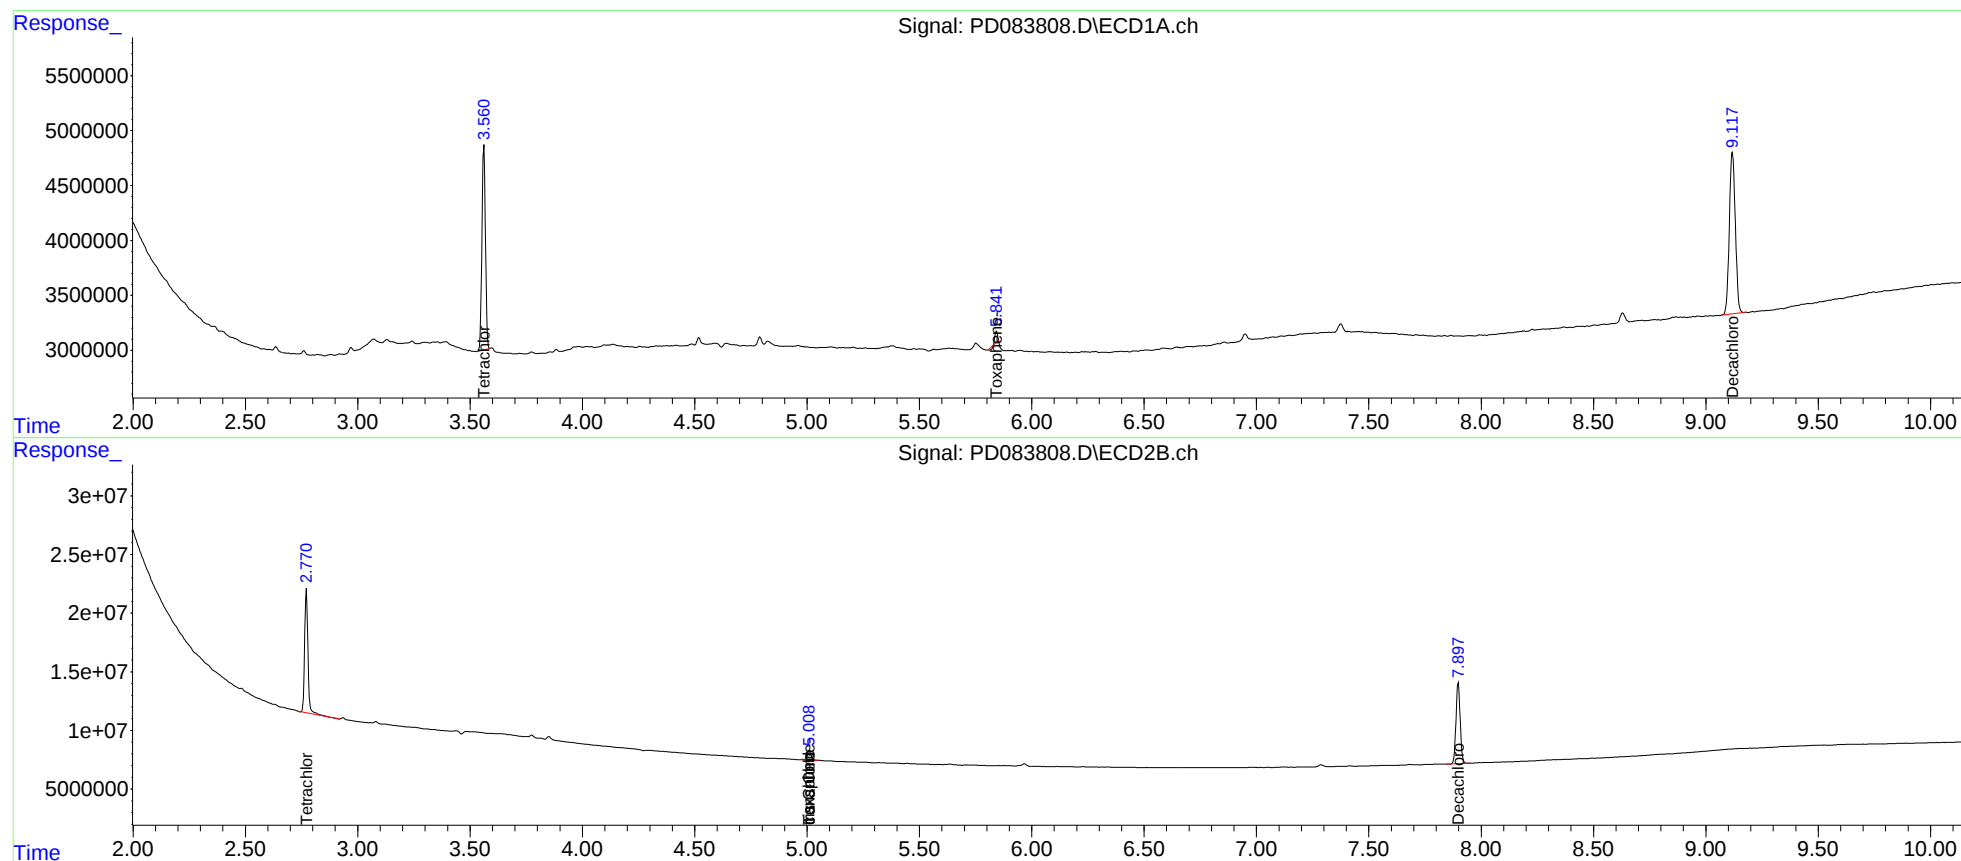

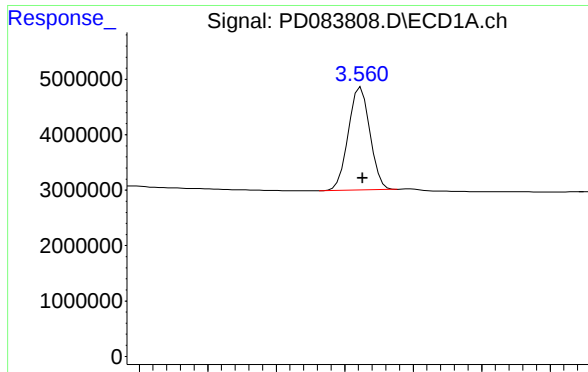


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.001 min
Response: 20386809
Conc: 15.62 ng/ml

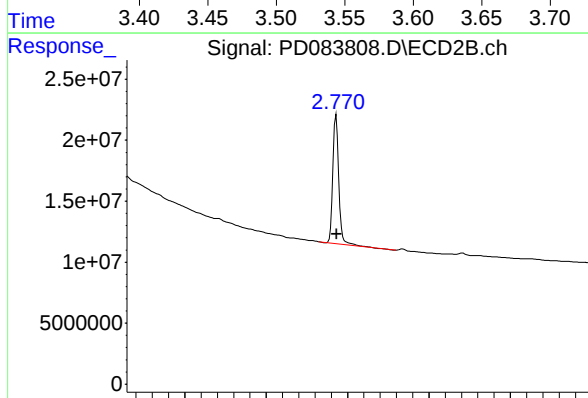


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.002 min
Response: 108662575
Conc: 19.93 ng/ml

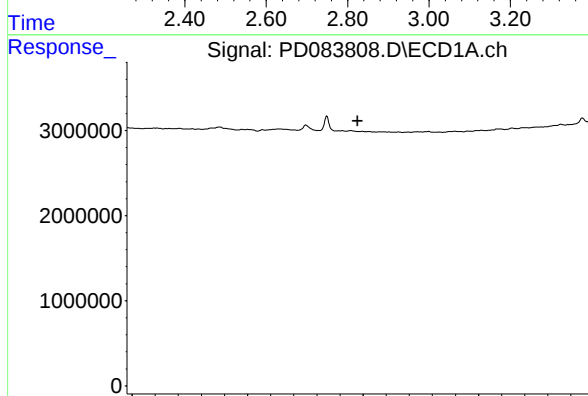


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.975 min
Response: 0
Conc: N.D.

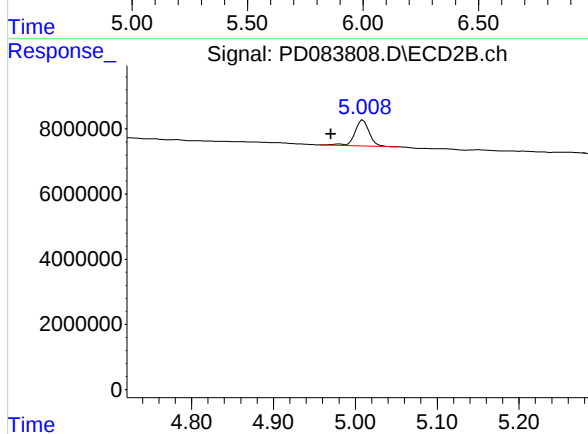


#10 trans-Chlordane

R.T.: 5.009 min
Delta R.T.: 0.039 min
Response: 9787928
Conc: 1.35 ng/ml

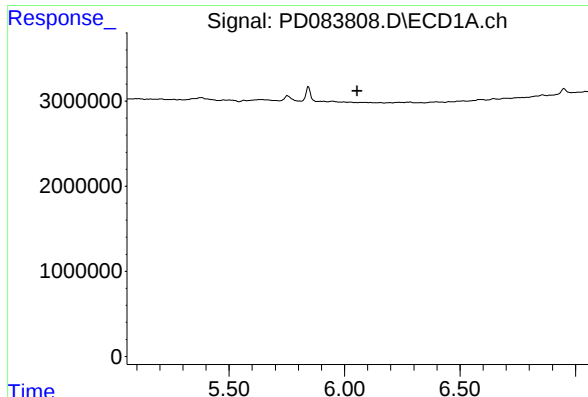


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.055 min
Response: 0
Conc: N.D.

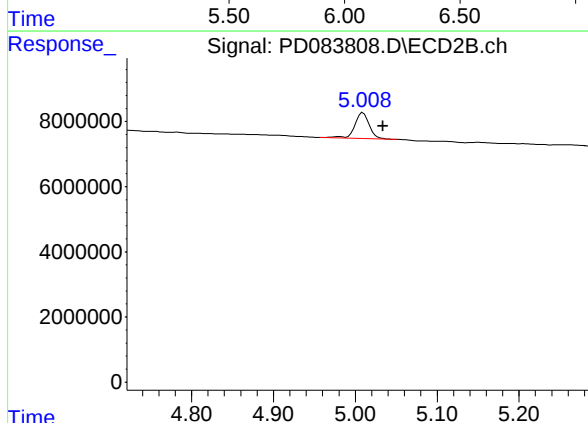


#11 cis-Chlordane

R.T.: 5.009 min
Delta R.T.: -0.024 min
Response: 9787928
Conc: 1.33 ng/ml

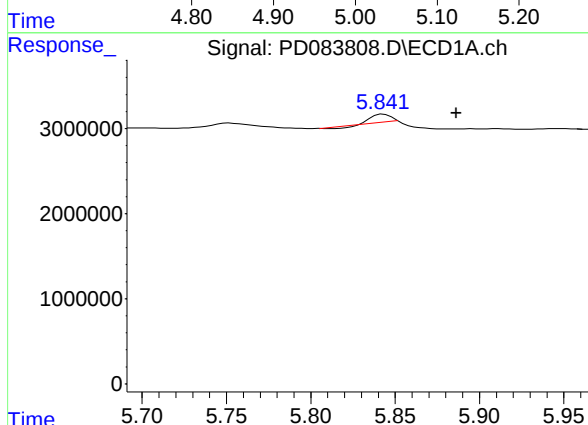


#22 Toxaphene-1

R.T.: 5.843 min
Delta R.T.: -0.043 min
Response: 668279
Conc: 110.37 ng/ml

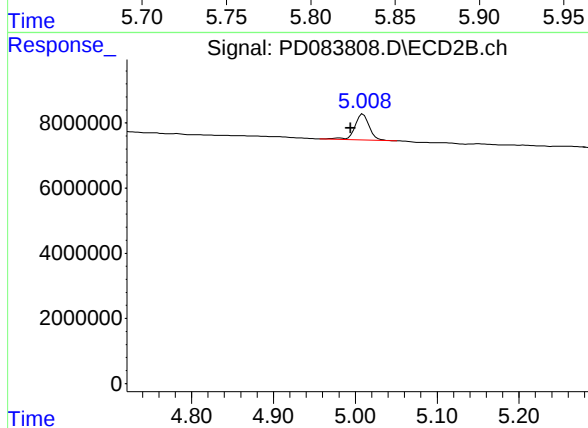


#22 Toxaphene-1

R.T.: 5.009 min
Delta R.T.: 0.015 min
Response: 9787928
Conc: 270.32 ng/ml

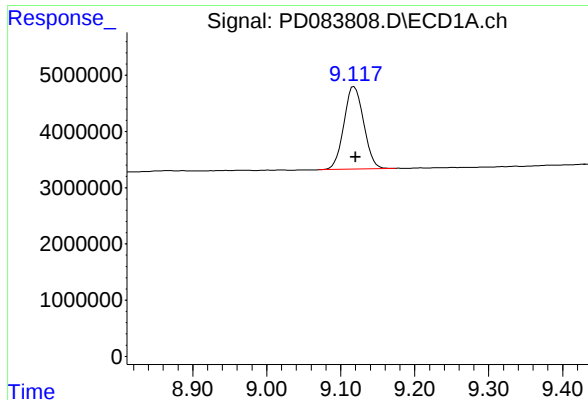

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.002 min
Response: 27242850
Conc: 14.01 ng/ml

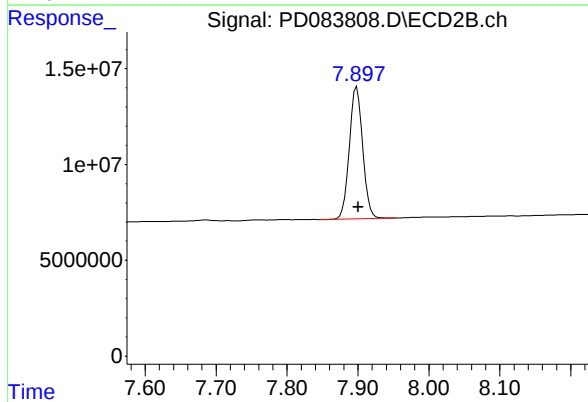

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.002 min
Response: 89592401
Conc: 14.75 ng/ml