

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
Data File : PD083795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 14:54
Operator : AR\AJ
Sample : PB161663BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PBLK663

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 06/25/2024
Supervised By :Ankita Jodhani 06/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:36:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

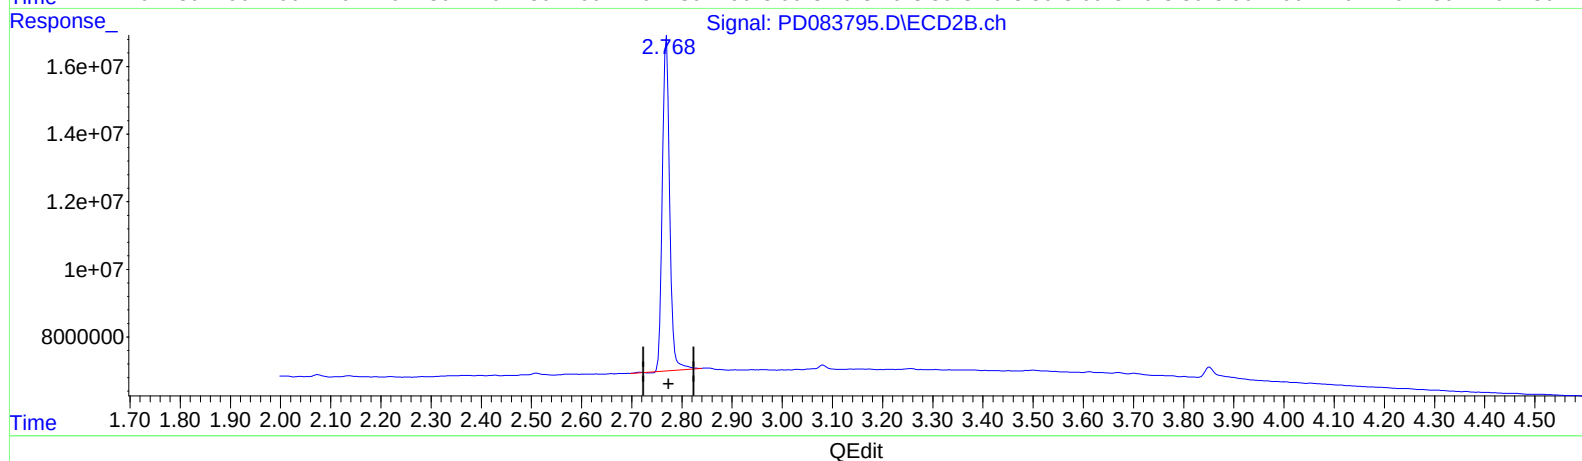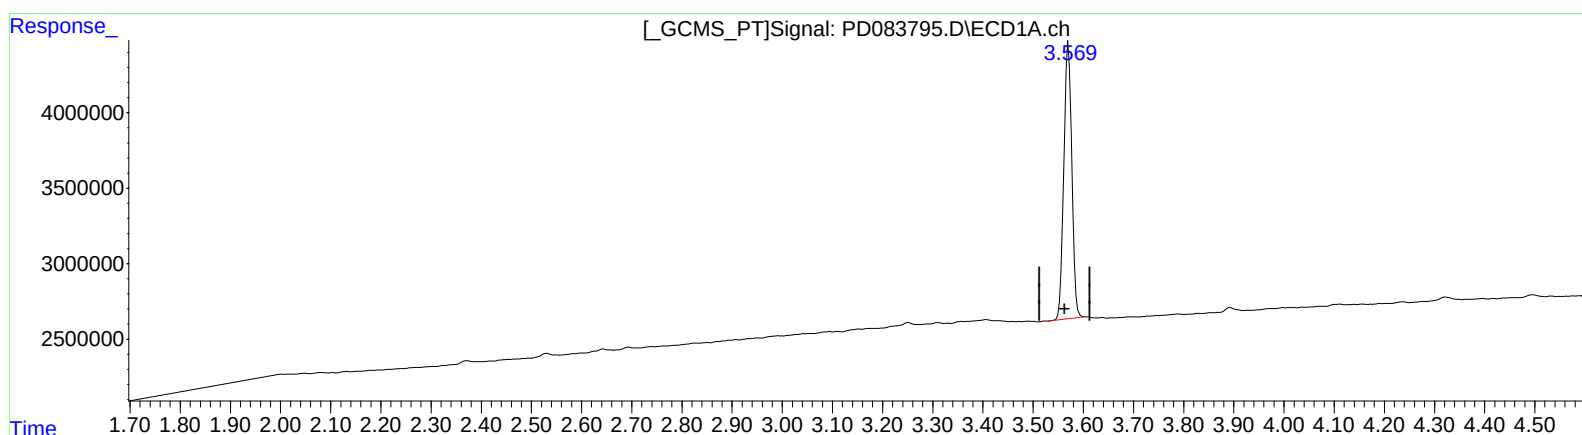

(1) Tetrachloro-m-xylene (SA)

3.571min 15.463 ng/ml

response 20183984

(1) Tetrachloro-m-xylene #2 (SA)

2.769min 18.432 ng/ml

response 100469838

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062424\
Data File : PD083795.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2024 14:54
Operator : AR\AJ
Sample : PB161663BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

PBLK663



Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 06/25/2024

Supervised By :Ankita Jodhani 06/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:36:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

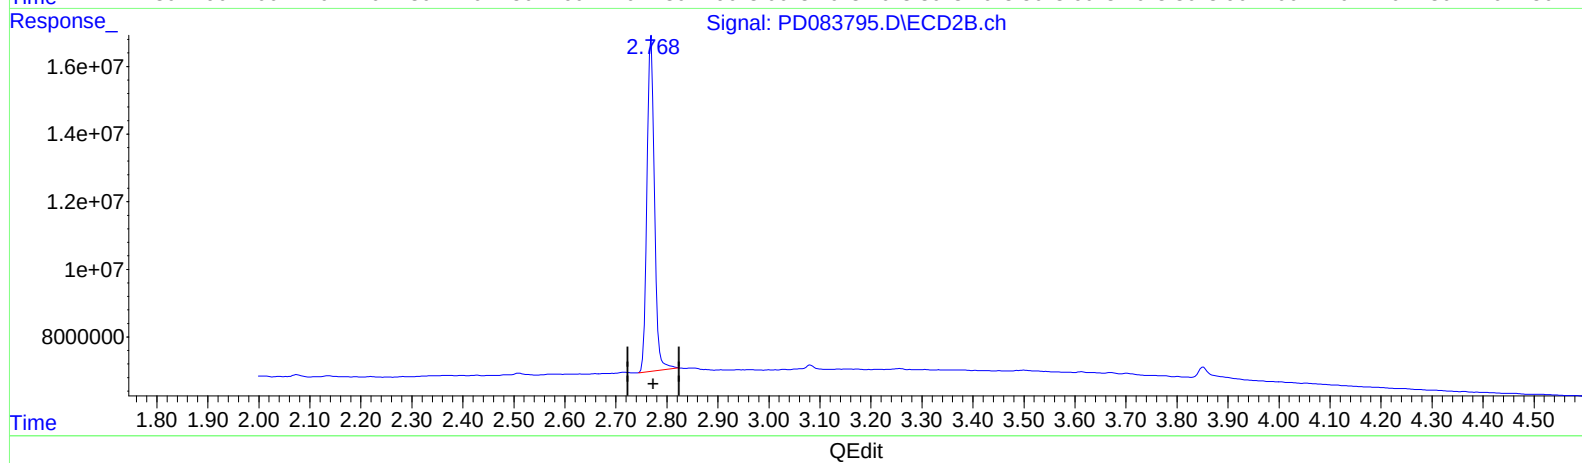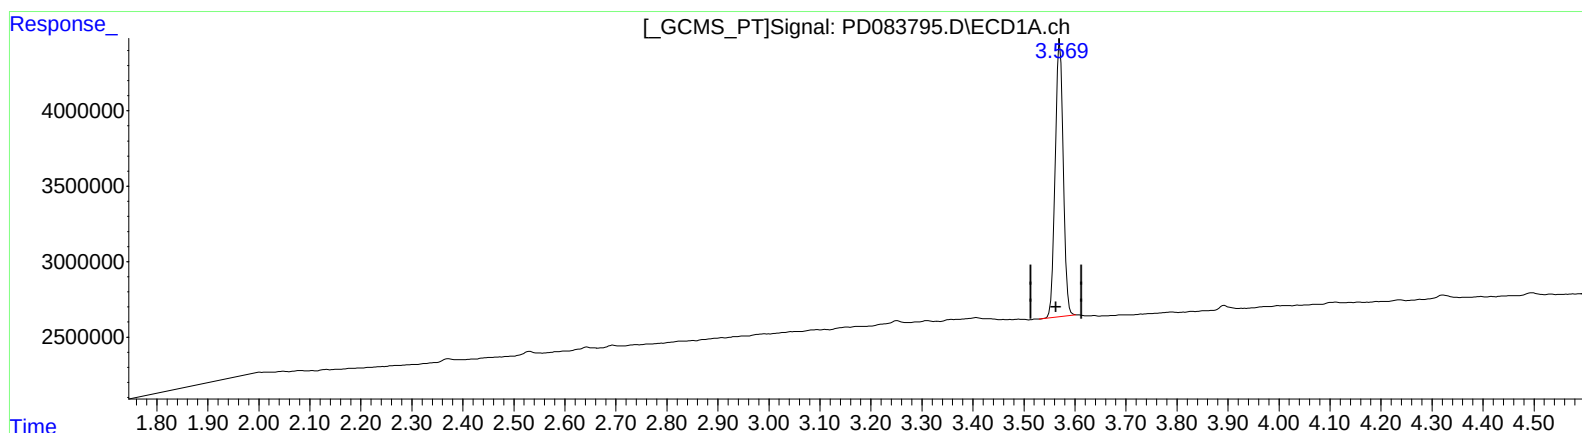

(1) Tetrachloro-m-xylene (SA)

3.571min 15.463 ng/ml

response 20183984

(1) Tetrachloro-m-xylene #2 (SA)

2.768min 18.463 ng/ml m

response 100641753