

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
 Data File : PD076115.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 18:56
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 22:53:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	43960074	23208289	20.637	21.392
28)	SA Decachlor...	9.084	7.910	48364854	20284798	19.091	20.745
Target Compounds							
2)	A alpha-BHC	4.001	3.269	35406891	16199512	9.590	10.126
3)	MA gamma-BHC...	4.335	3.599	33386335	15089792	9.922	10.241
4)	MA Heptachlor	4.941	0.000	1295121	0	0.361	N.D. #
6)	B beta-BHC	4.531	3.896	15333783	7543989	10.665	11.835
7)	B delta-BHC	4.762f	0.000	1022798	0	0.308	N.D. #
8)	B Heptachlo...	5.690	0.000	2216112	0	0.688	N.D. #
9)	A Endosulfan I	6.110f	0.000	41428	0	0.014	N.D. #
10)	B gamma-Chl...	5.923f	0.000	359269	0	0.112	N.D. #
11)	B alpha-Chl...	6.052f	0.000	86716	0	0.027	N.D. #
12)	B 4,4'-DDE	6.206	0.000	177407	0	0.062	N.D. #
13)	MA Dieldrin	6.381f	0.000	319129	0	0.102	N.D. #
14)	MA Endrin	6.589	5.632	115.9E6	60095295	43.331	49.380
15)	B Endosulfa...	6.824	5.941	1177953	304958	0.456	0.283 #
16)	A 4,4'-DDD	6.722	5.780	6510767	3374220	2.861	3.829 #
17)	MA 4,4'-DDT	7.037	6.031	229.3E6	111.5E6	101.041	137.291 #
18)	B Endrin al...	6.938	6.107	2549765	2089411	1.271	2.414 #
20)	A Methoxychlor	7.513	6.607	322.0E6	147.9E6	248.747	319.463 #
21)	B Endrin ke...	7.659	6.835	8311981	4390366	2.984	3.614
24)	Chlordane-2	0.000	4.369f	0	1105622	N.D.	20.854 #
26)	Chlordane-4	6.052	0.000	86716	0	0.138	N.D. #
27)	Chlordane-5	0.000	5.941	0	304958	N.D.	6.305 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
Data File : PD076115.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 18:56
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PEM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 22:53:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

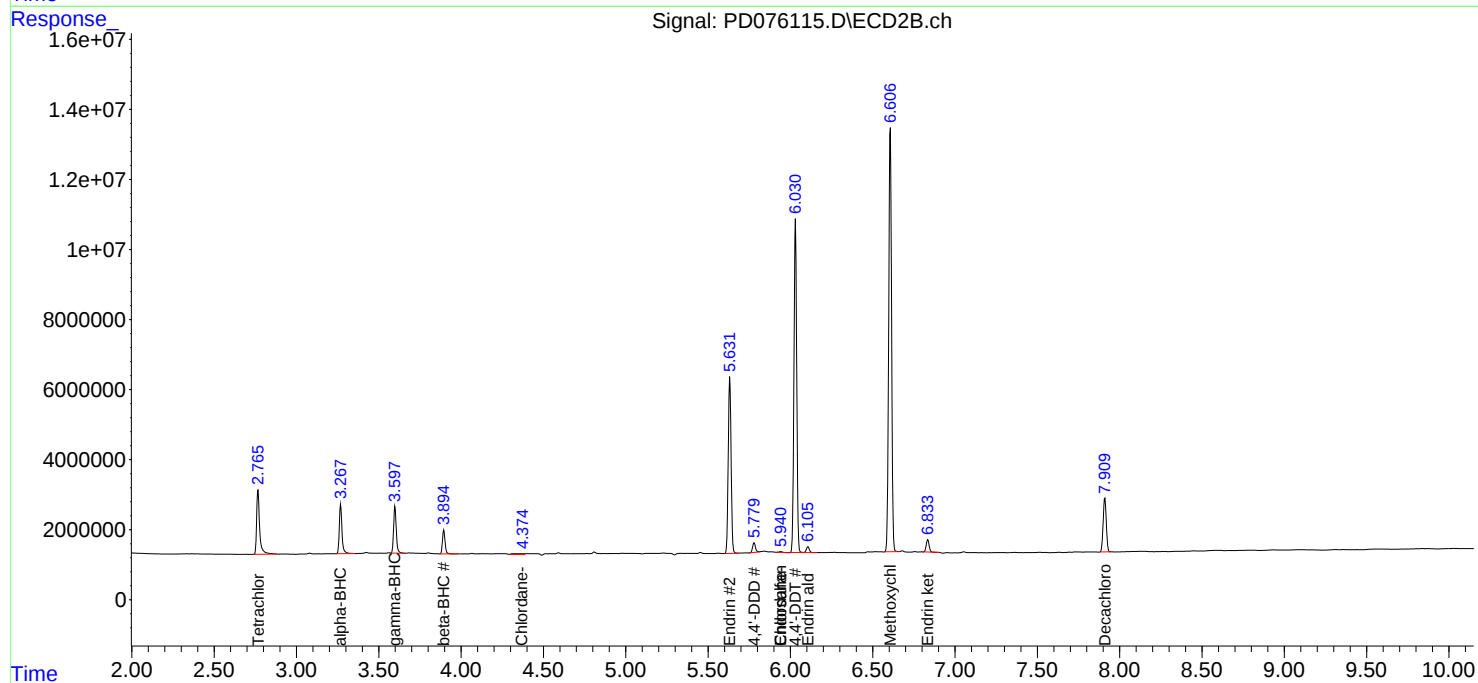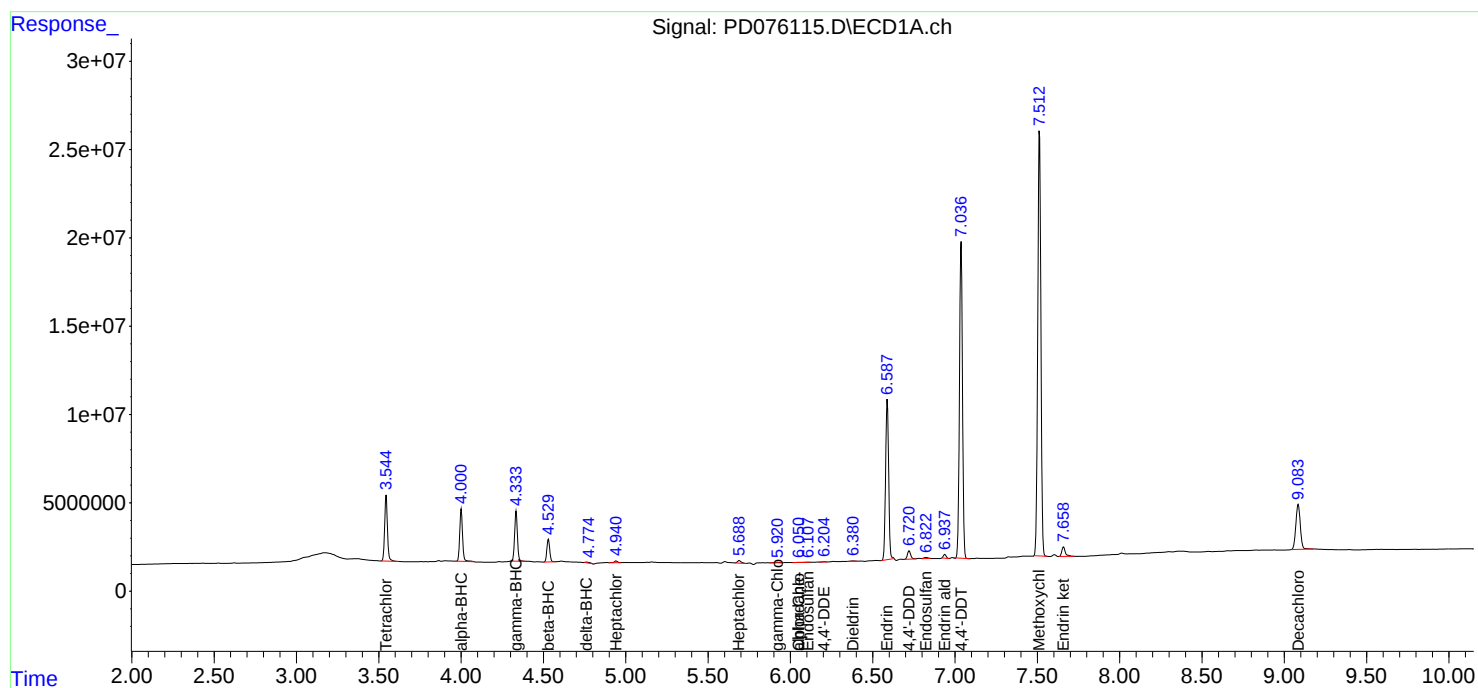


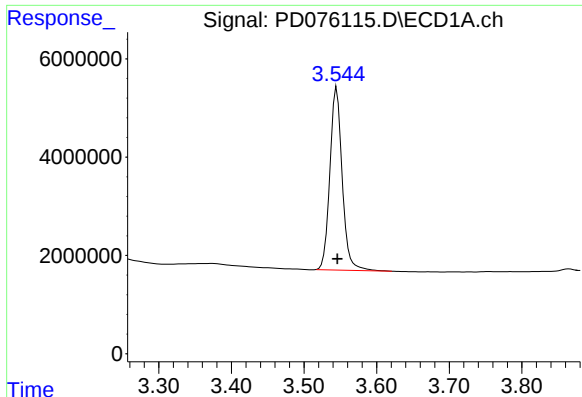

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 43960074
Conc: 20.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

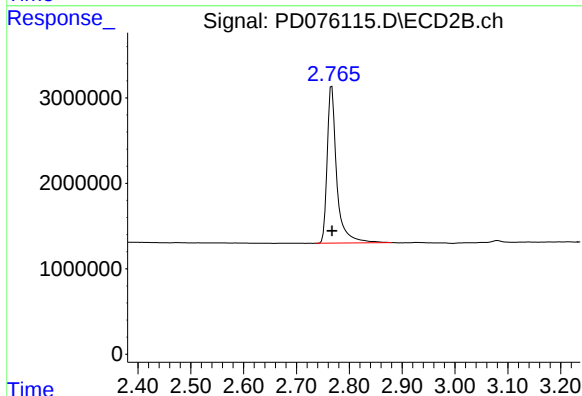


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 23208289
Conc: 21.39 ng/ml

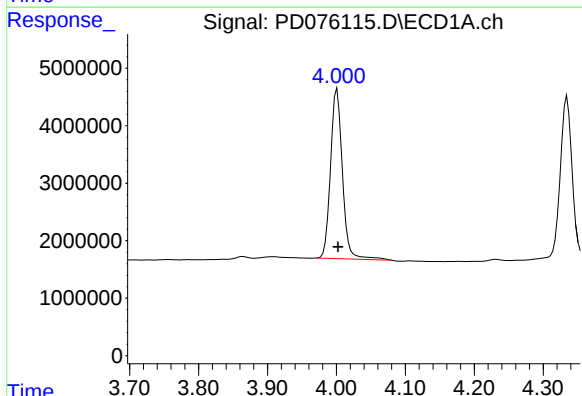


#2 alpha-BHC

R.T.: 4.001 min
Delta R.T.: -0.002 min
Response: 35406891
Conc: 9.59 ng/ml

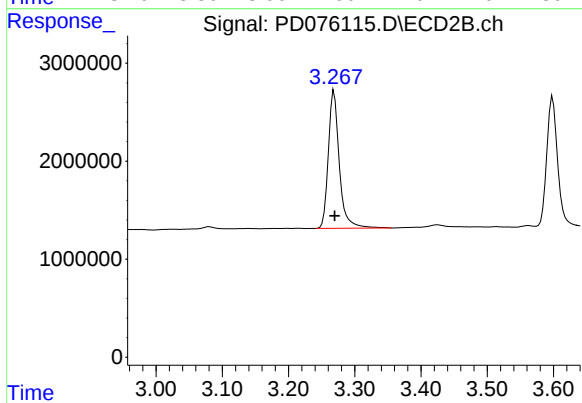

#2 alpha-BHC


R.T.: 3.269 min
Delta R.T.: 0.000 min
Response: 16199512
Conc: 10.13 ng/ml

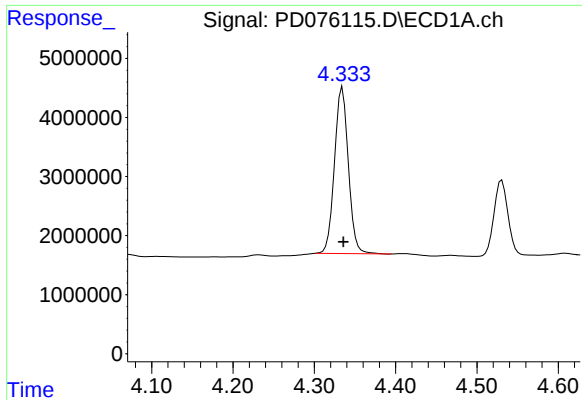

#3 gamma-BHC (Lindane)


R.T.: 4.335 min
Delta R.T.: -0.001 min
Response: 33386335
Conc: 9.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

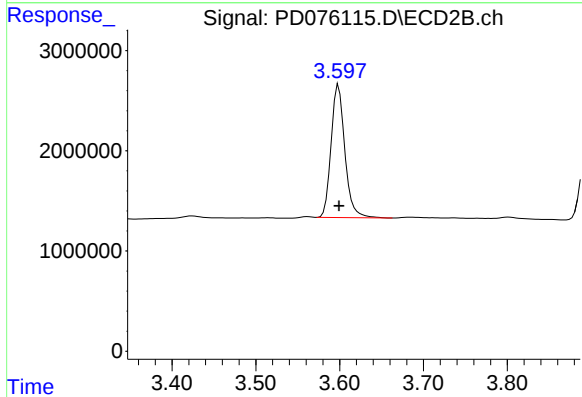


#3 gamma-BHC (Lindane)

R.T.: 3.599 min
Delta R.T.: 0.000 min
Response: 15089792
Conc: 10.24 ng/ml

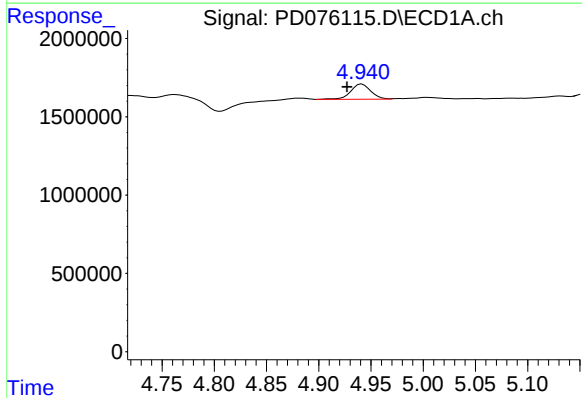


#4 Heptachlor

R.T.: 4.941 min
Delta R.T.: 0.014 min
Response: 1295121
Conc: 0.36 ng/ml

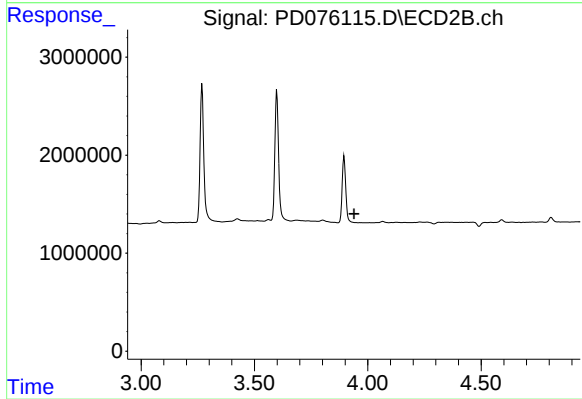

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

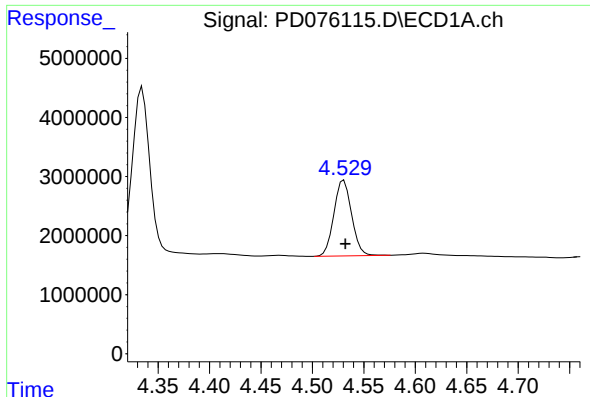

#6 beta-BHC


R.T.: 4.531 min
Delta R.T.: -0.002 min
Response: 15333783
Conc: 10.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

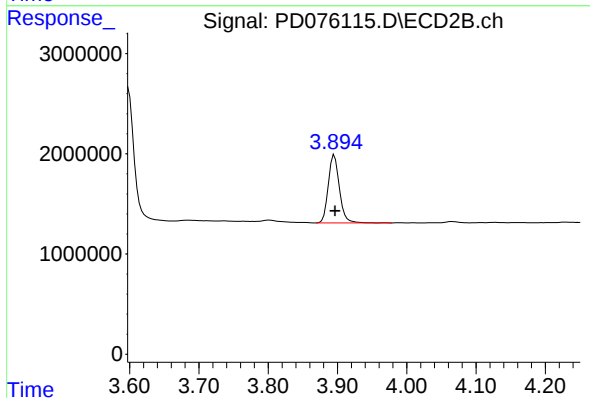


#6 beta-BHC

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 7543989
Conc: 11.84 ng/ml

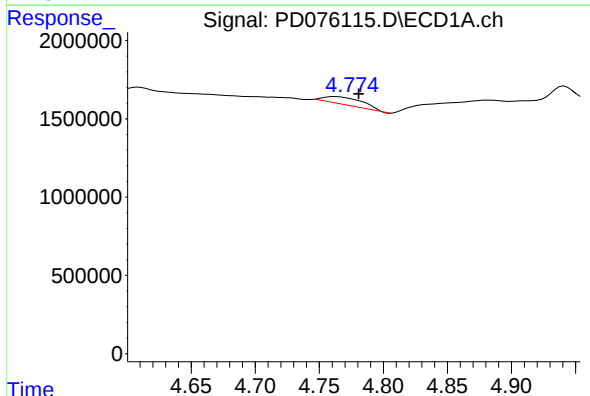


#7 delta-BHC

R.T.: 4.762 min
Delta R.T.: -0.019 min
Response: 1022798
Conc: 0.31 ng/ml

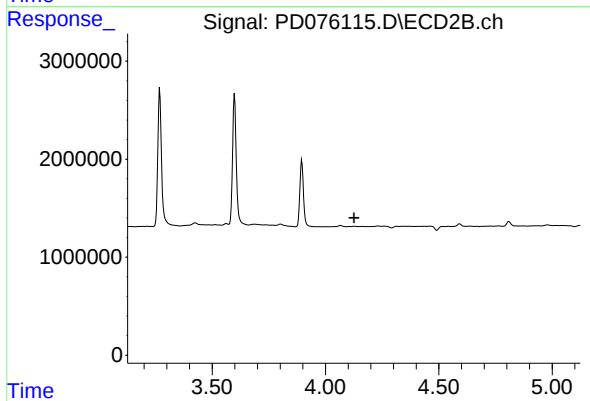

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

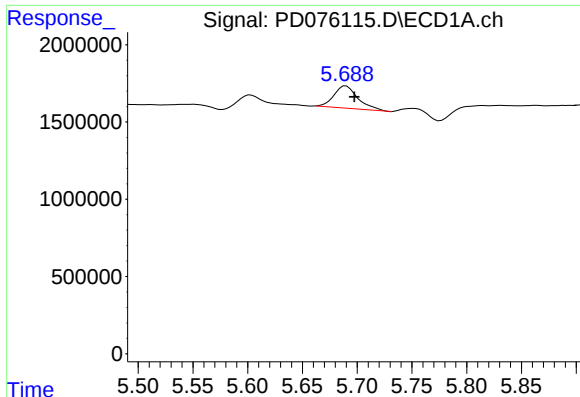

#8 Heptachlor epoxide


R.T.: 5.690 min
Delta R.T.: -0.008 min
Response: 2216112
Conc: 0.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

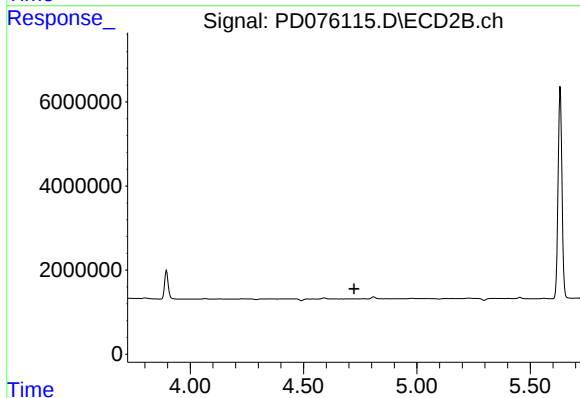


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

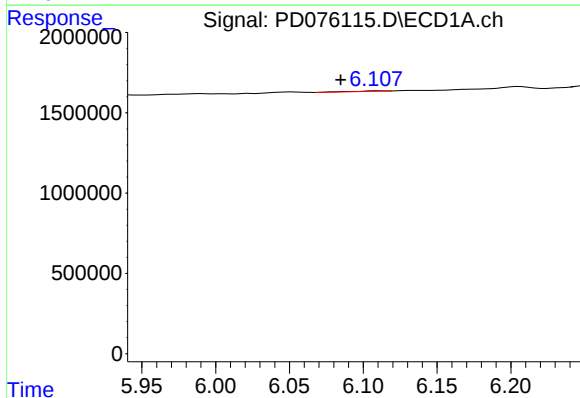


#9 Endosulfan I

R.T.: 6.110 min
Delta R.T.: 0.025 min
Response: 41428
Conc: 0.01 ng/ml

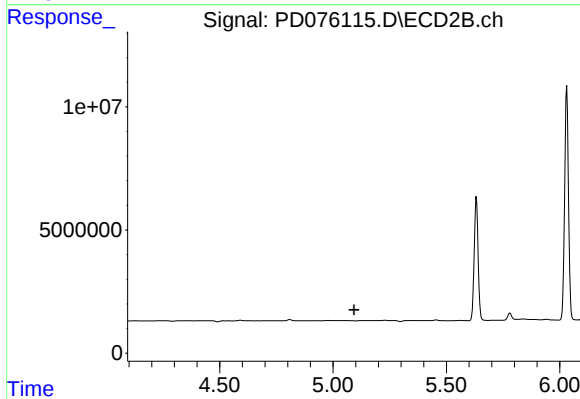

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

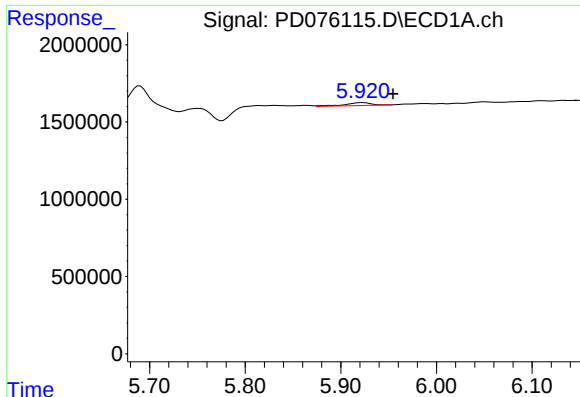

#10 gamma-Chlordane


R.T.: 5.923 min
Delta R.T.: -0.032 min
Response: 359269
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

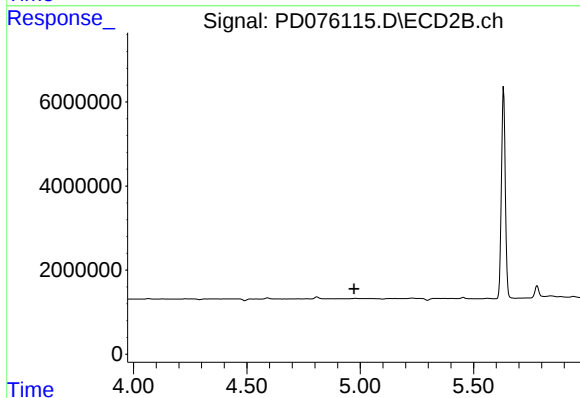


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

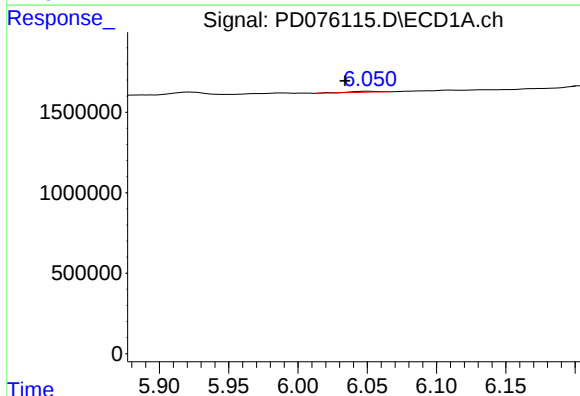


#11 alpha-Chlordane

R.T.: 6.052 min
Delta R.T.: 0.018 min
Response: 86716
Conc: 0.03 ng/ml

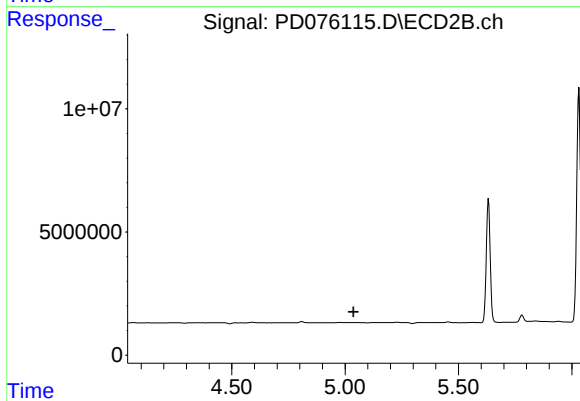

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

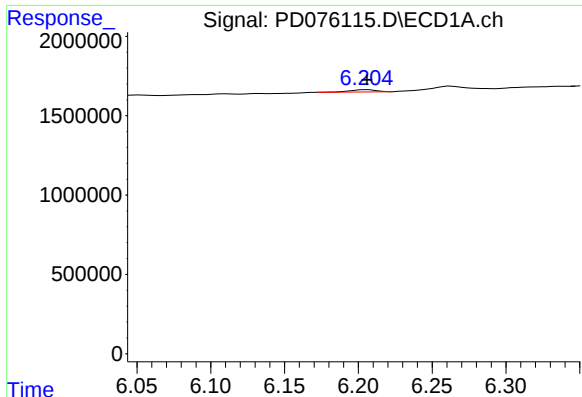

#12 4,4'-DDE


R.T.: 6.206 min
Delta R.T.: 0.000 min
Response: 177407
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

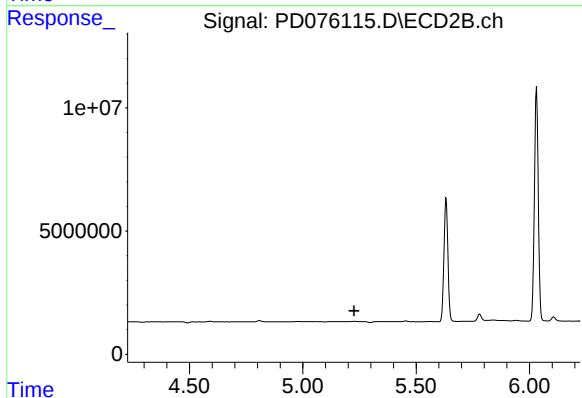


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.227 min
Response: 0
Conc: N.D.

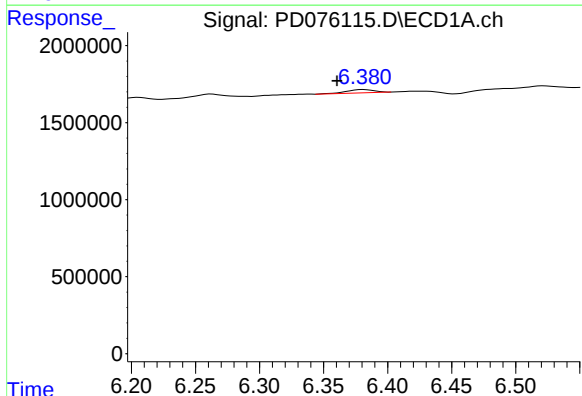


#13 Dieldrin

R.T.: 6.381 min
Delta R.T.: 0.021 min
Response: 319129
Conc: 0.10 ng/ml

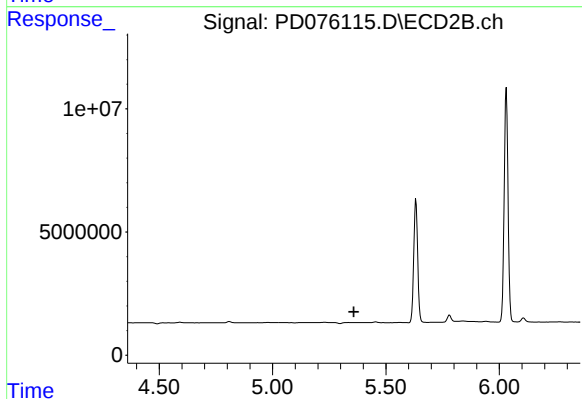

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

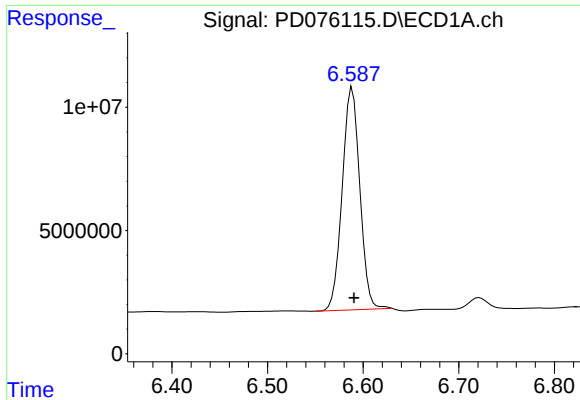

#14 Endrin


R.T.: 6.589 min
Delta R.T.: -0.002 min
Response: 115881714
Conc: 43.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

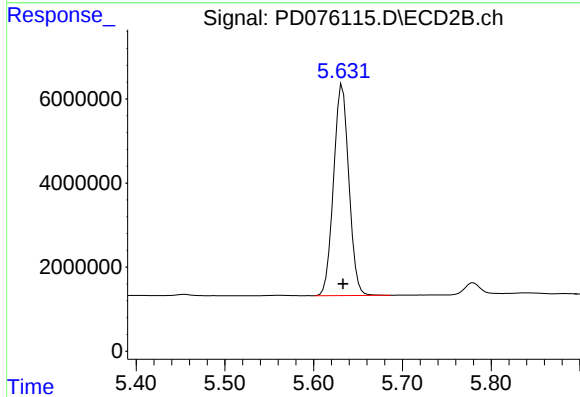


#14 Endrin

R.T.: 5.632 min
Delta R.T.: 0.000 min
Response: 60095295
Conc: 49.38 ng/ml

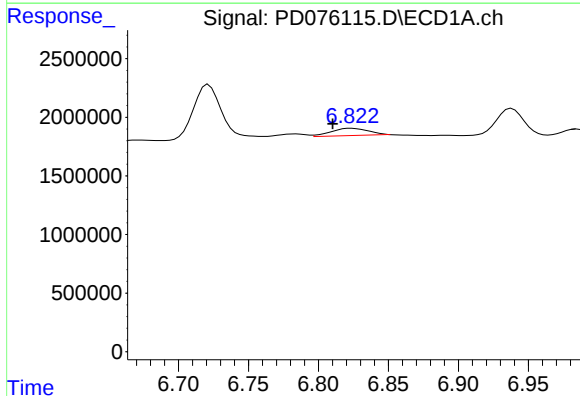


#15 Endosulfan II

R.T.: 6.824 min
Delta R.T.: 0.013 min
Response: 1177953
Conc: 0.46 ng/ml

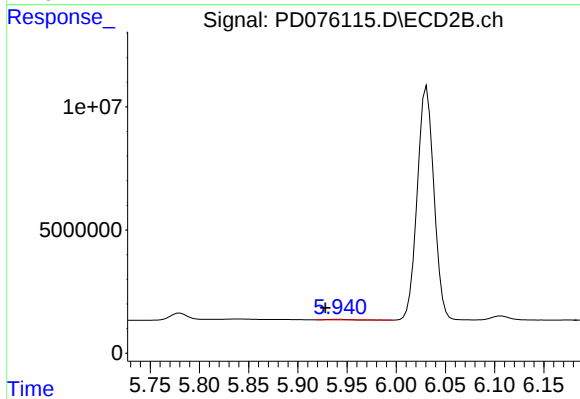

#15 Endosulfan II


R.T.: 5.941 min
Delta R.T.: 0.013 min
Response: 304958
Conc: 0.28 ng/ml

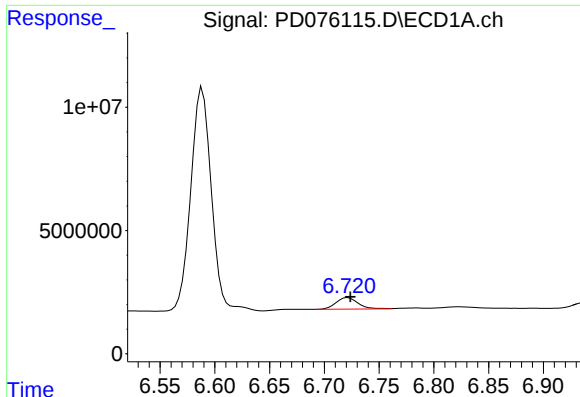

#16 4,4'-DDD


R.T.: 6.722 min
Delta R.T.: -0.002 min
Response: 6510767
Conc: 2.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

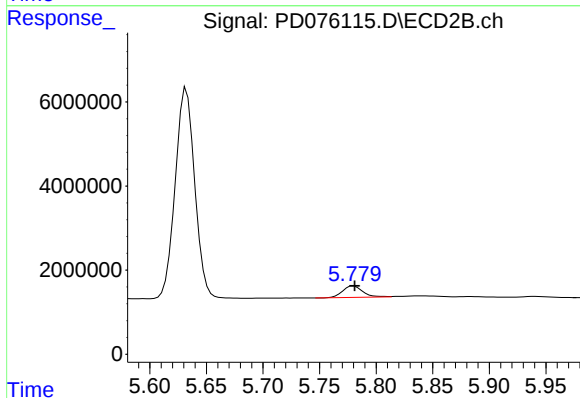


#16 4,4'-DDD

R.T.: 5.780 min
Delta R.T.: -0.001 min
Response: 3374220
Conc: 3.83 ng/ml

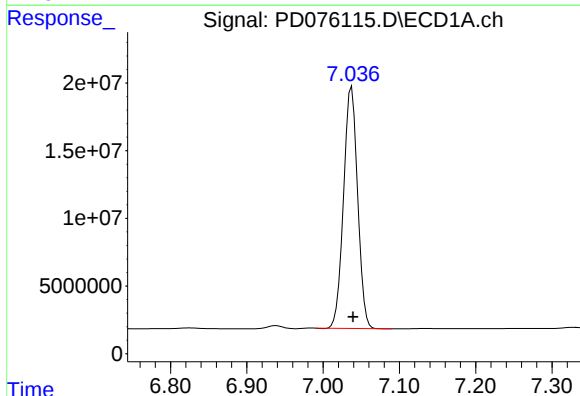


#17 4,4'-DDT

R.T.: 7.037 min
Delta R.T.: -0.002 min
Response: 229289485
Conc: 101.04 ng/ml

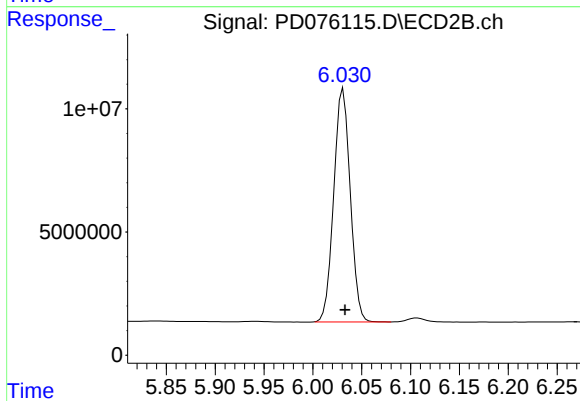

#17 4,4'-DDT


R.T.: 6.031 min
Delta R.T.: -0.002 min
Response: 111520503
Conc: 137.29 ng/ml

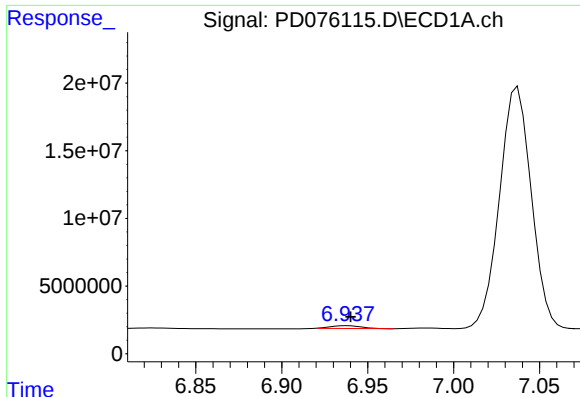

#18 Endrin aldehyde


R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 2549765
Conc: 1.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

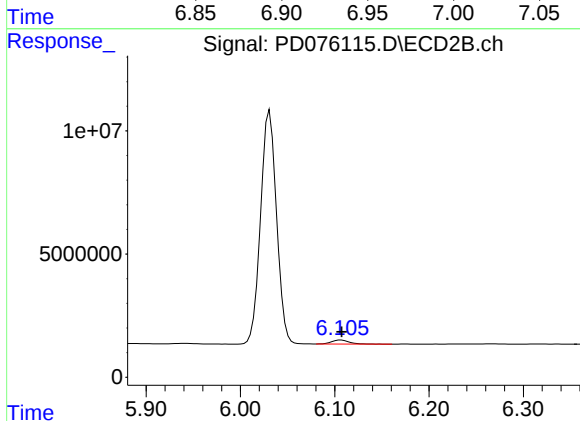


#18 Endrin aldehyde

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 2089411
Conc: 2.41 ng/ml

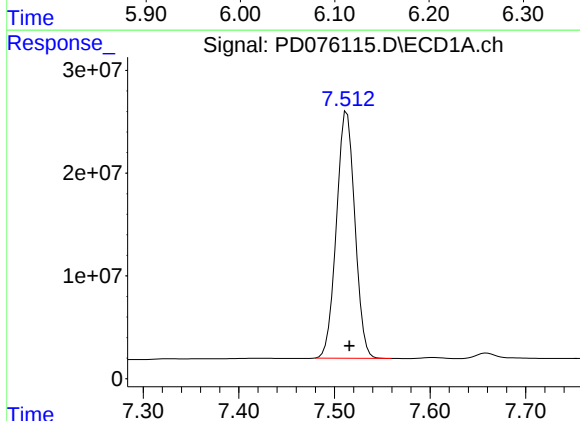


#20 Methoxychlor

R.T.: 7.513 min
Delta R.T.: -0.003 min
Response: 321976448
Conc: 248.75 ng/ml

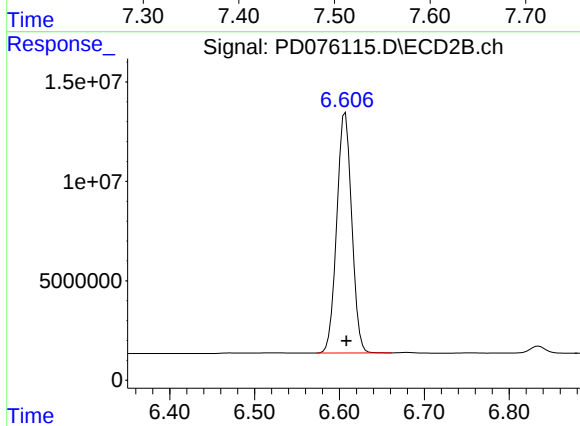

#20 Methoxychlor


R.T.: 6.607 min
Delta R.T.: -0.001 min
Response: 147861394
Conc: 319.46 ng/ml

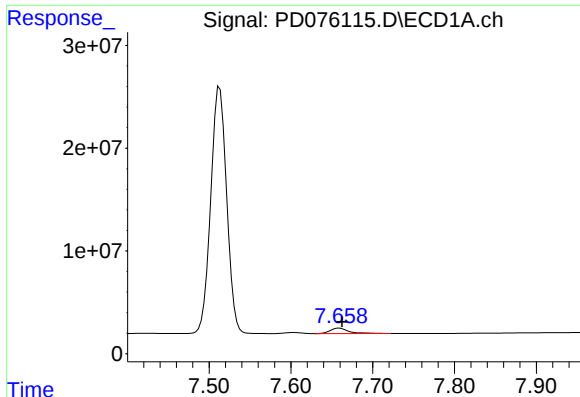

#21 Endrin ketone


R.T.: 7.659 min
Delta R.T.: -0.003 min
Response: 8311981
Conc: 2.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

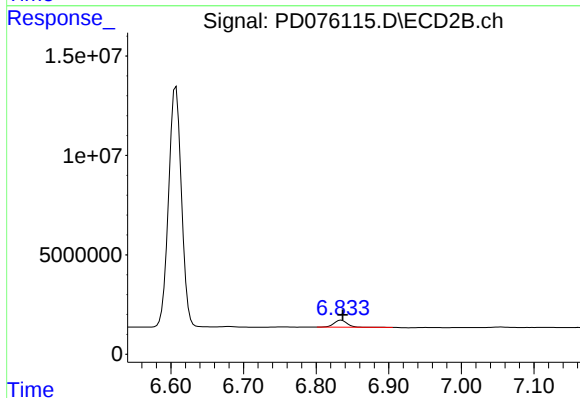


#21 Endrin ketone

R.T.: 6.835 min
Delta R.T.: -0.002 min
Response: 4390366
Conc: 3.61 ng/ml

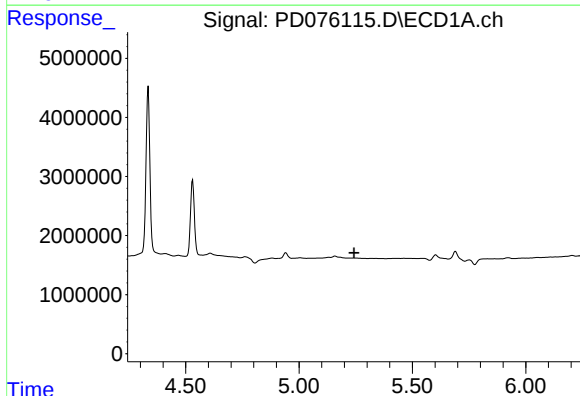


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.243 min
Response: 0
Conc: N.D.

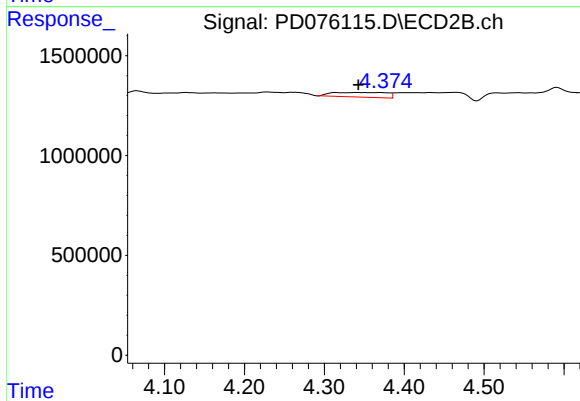

#24 Chlordane-2


R.T.: 4.369 min
Delta R.T.: 0.026 min
Response: 1105622
Conc: 20.85 ng/ml

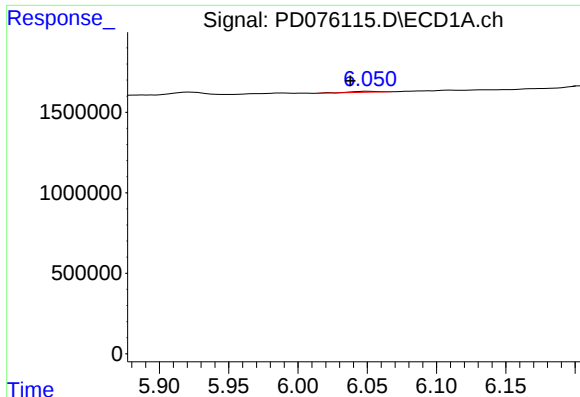

#26 Chlordane-4


R.T.: 6.052 min
Delta R.T.: 0.014 min
Response: 86716
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

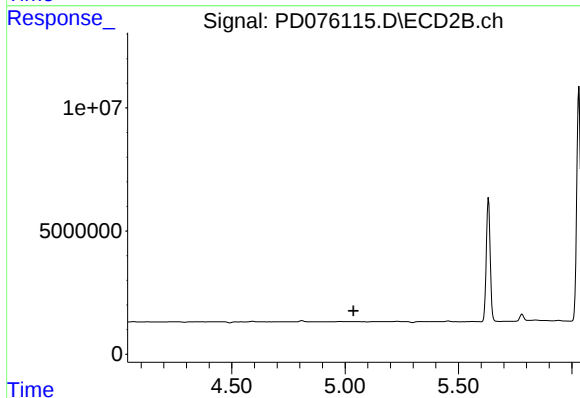


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

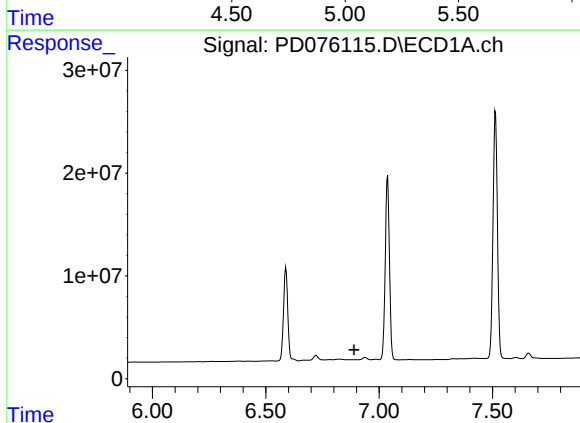


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.890 min
Response: 0
Conc: N.D.

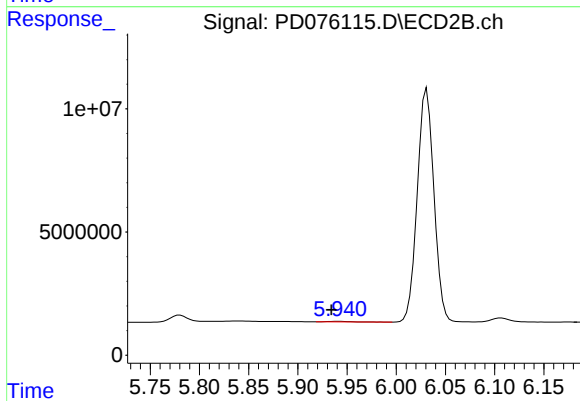

#27 Chlordane-5

R.T.: 5.941 min
Delta R.T.: 0.007 min
Response: 304958
Conc: 6.31 ng/ml

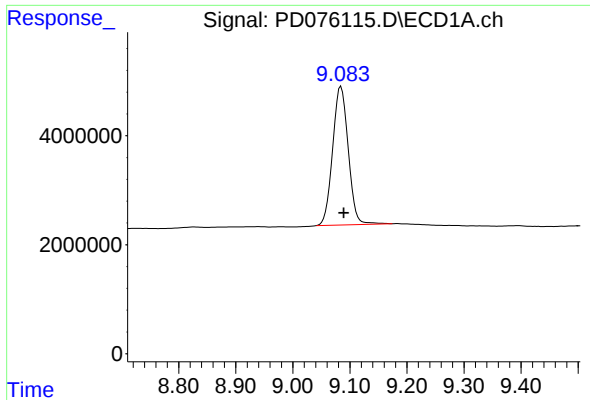

#28 Decachlorobiphenyl


R.T.: 9.084 min

Delta R.T.: -0.005 min

Response: 48364854

Conc: 19.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PEM

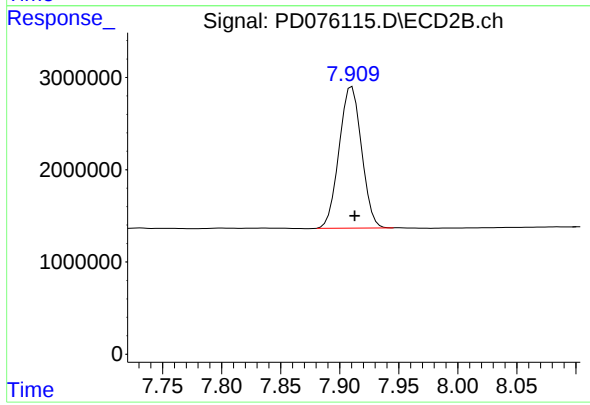

#28 Decachlorobiphenyl

R.T.: 7.910 min

Delta R.T.: -0.002 min

Response: 20284798

Conc: 20.75 ng/ml