

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
 Data File : PD076095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 10:31
 Operator : AR\AJ
 Sample : 03363-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/26/2023
 Supervised By :Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 16:33:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.766	19372195	10209905	9.094	9.411
28)	SA Decachlor...	9.089	7.913	21237851	8887595	8.383	9.089
Target Compounds							
12)	B 4,4'-DDE	6.205	5.224	2293141	837932	0.802	0.751m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
Data File : PD076095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 10:31
Operator : AR\AJ
Sample : 03363-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/26/2023
Supervised By : Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 16:33:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

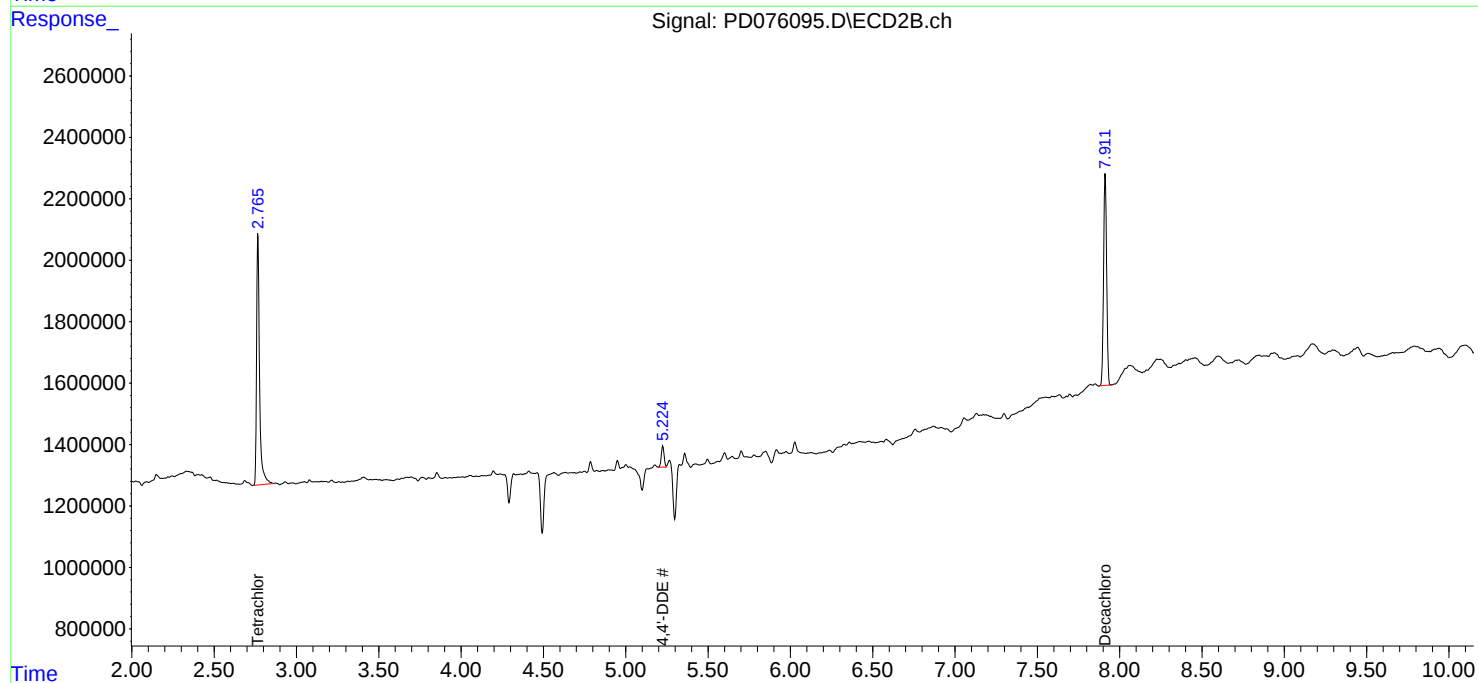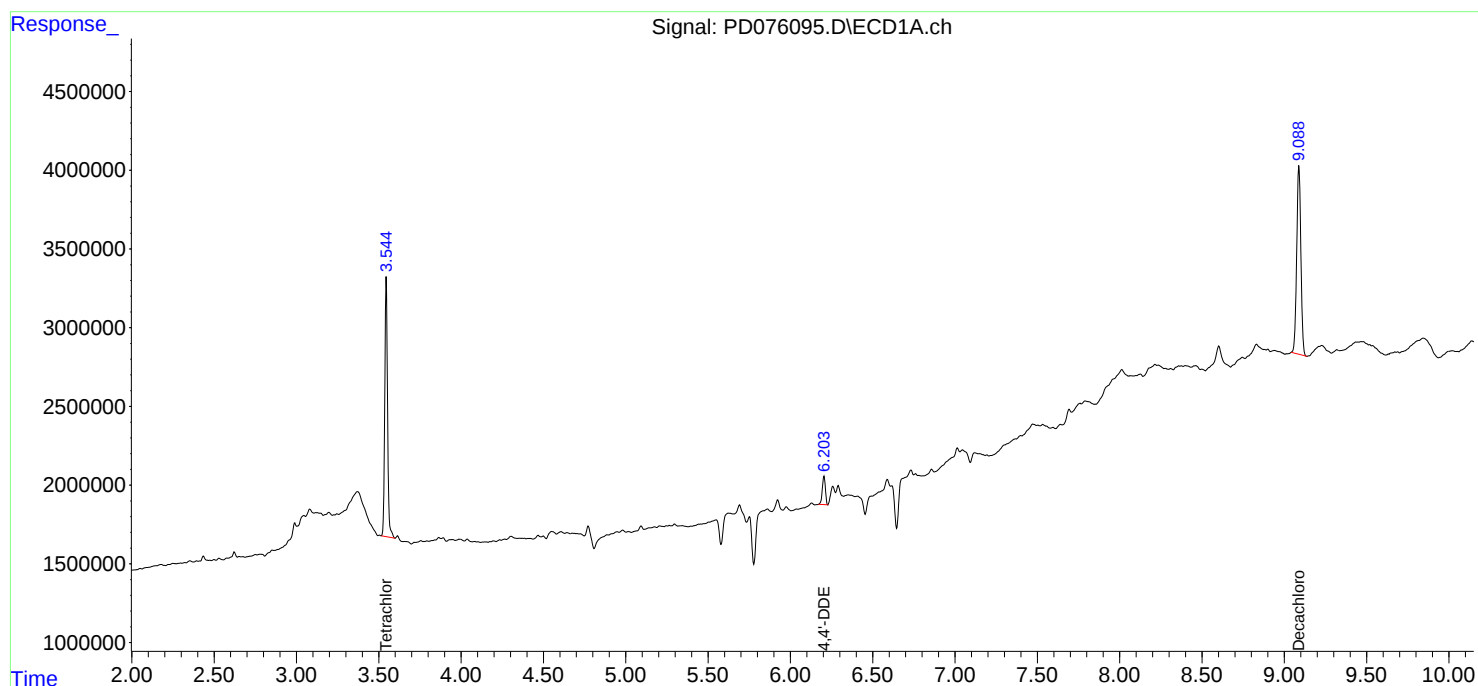

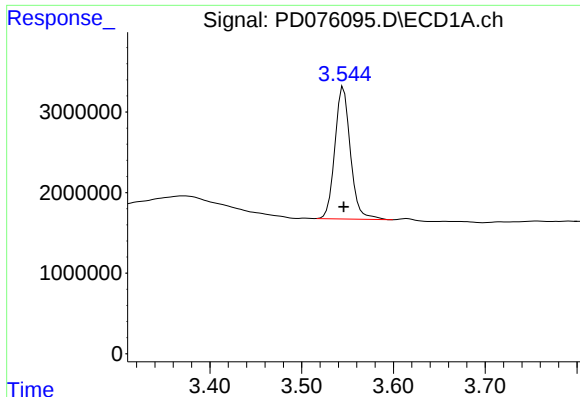


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 19372195
Conc: 9.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
SP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

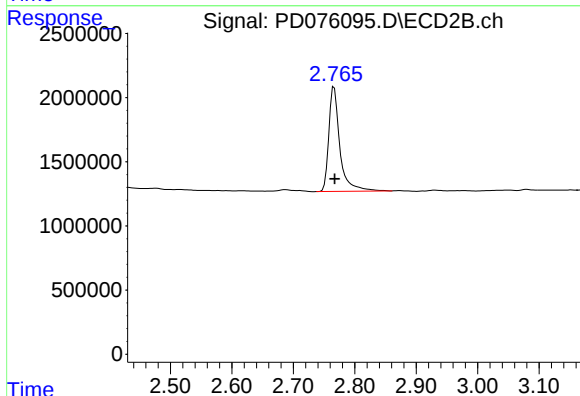


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 10209905
Conc: 9.41 ng/ml

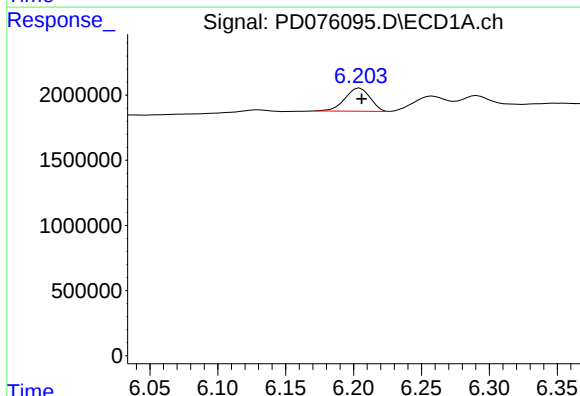


#12 4,4'-DDE

R.T.: 6.205 min
Delta R.T.: -0.001 min
Response: 2293141
Conc: 0.80 ng/ml

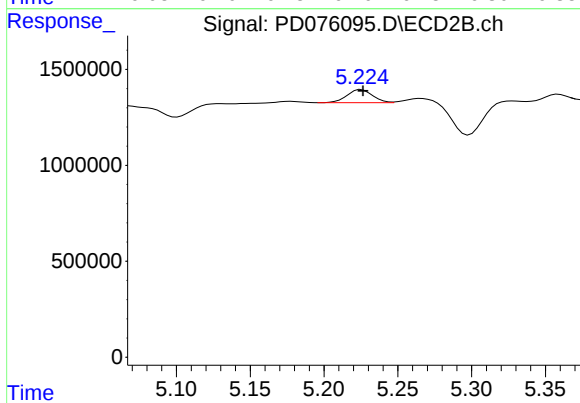

#12 4,4'-DDE

R.T.: 5.224 min
Delta R.T.: -0.003 min
Response: 837932
Conc: 0.75 ng/ml m

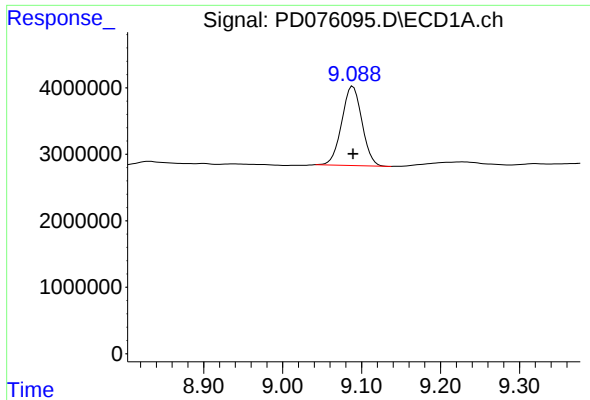


#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 21237851
Conc: 8.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
SP

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

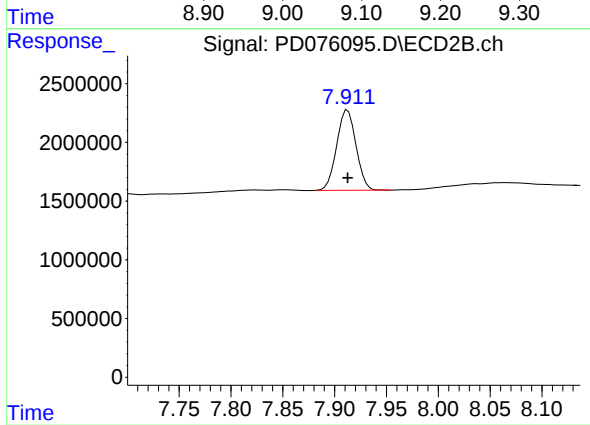

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 8887595
Conc: 9.09 ng/ml