

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
 Data File : PD076101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 11:52
 Operator : AR\AJ
 Sample : 03331-26 (Sig #1); 03331--26 (Sig #2)
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMPOSTIE-SB18-27

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/26/2023
 Supervised By : Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 16:33:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.545	2.767	24235201	11977071	11.377	11.040
2) SA Decachlor...	9.083	7.909	35608816	15991545	14.056m	16.355m
Target Compounds						
11) B alpha-Chl...	6.036	5.033	34780921	8128551	10.758	5.926m#
12) B 4,4'-DDE	6.202	5.223	15886065	6769993	5.558m	6.065m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
Data File : PD076101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 11:52
Operator : AR\AJ
Sample : 03331-26 (Sig #1); 03331--26 (Sig #2)
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMPOSTIE-SB18-27


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/26/2023
Supervised By : Ankita Jodhani 06/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 16:33:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

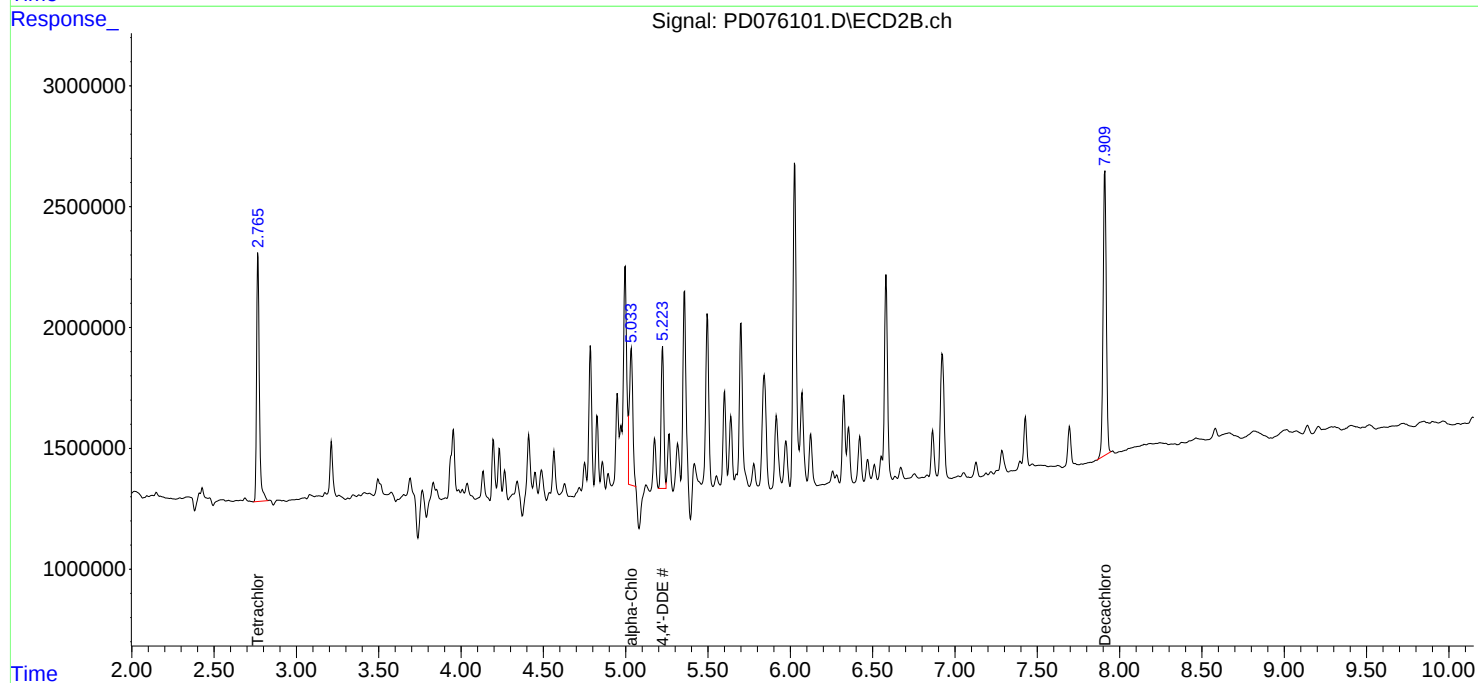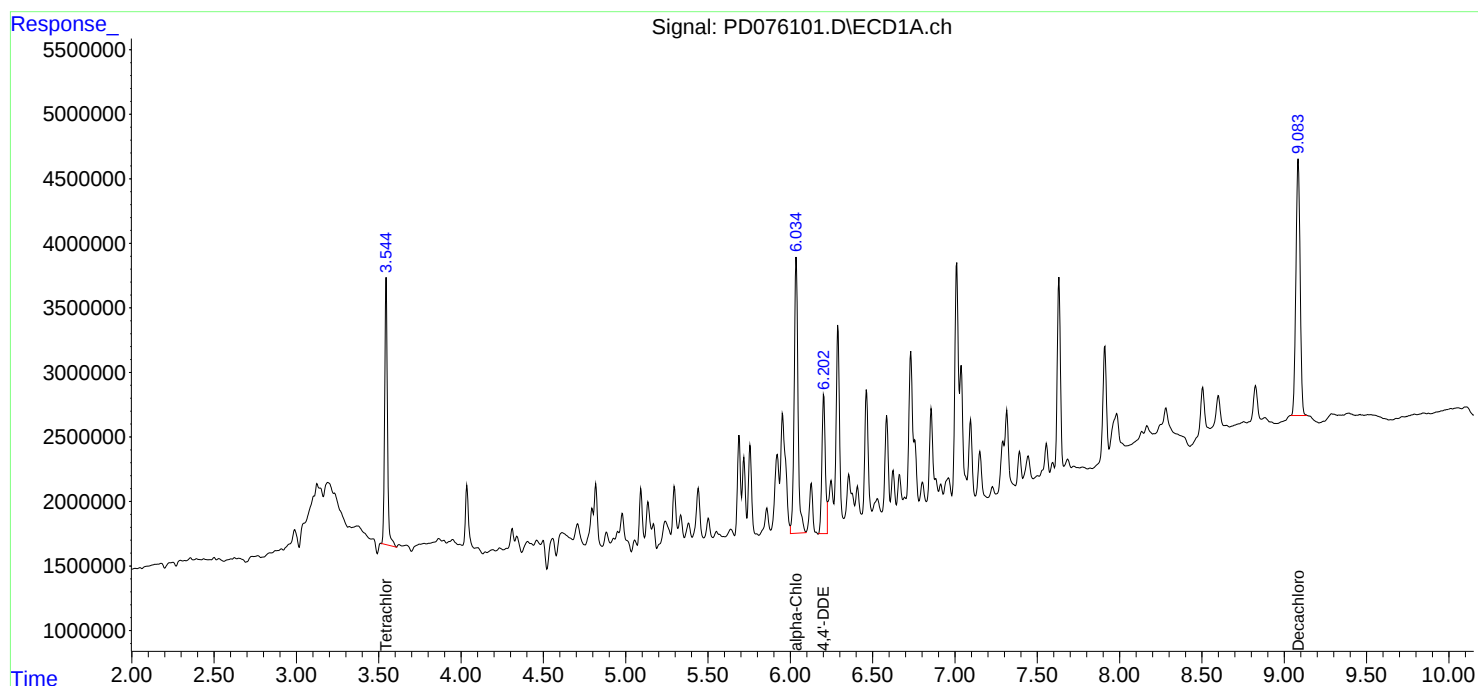

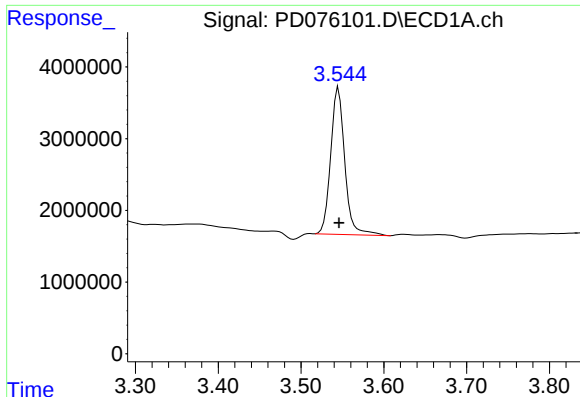


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 24235201
Conc: 11.38 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSTIE-SB18-27


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

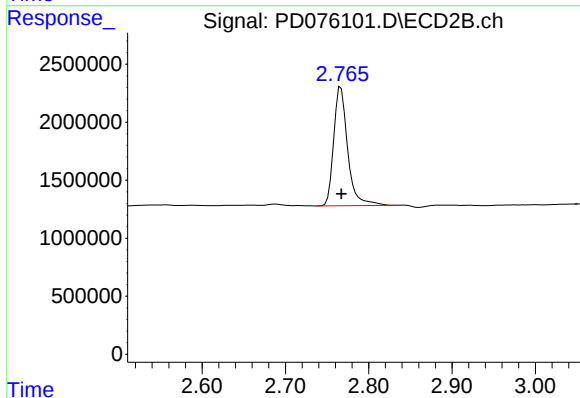


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 11977071
Conc: 11.04 ng/ml

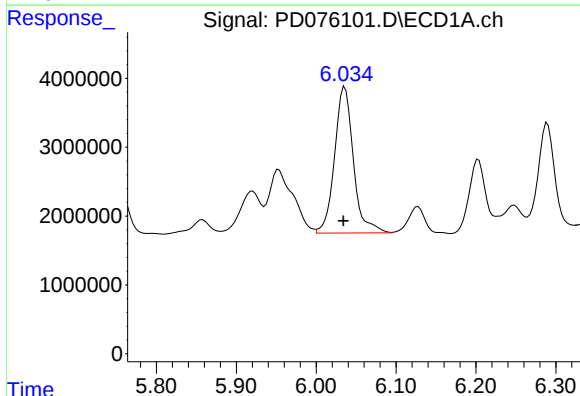


#11 alpha-Chlordane

R.T.: 6.036 min
Delta R.T.: 0.002 min
Response: 34780921
Conc: 10.76 ng/ml

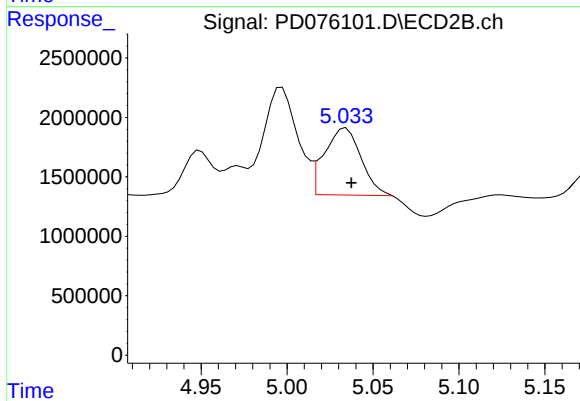

#11 alpha-Chlordane

R.T.: 5.033 min
Delta R.T.: -0.005 min
Response: 8128551
Conc: 5.93 ng/ml m

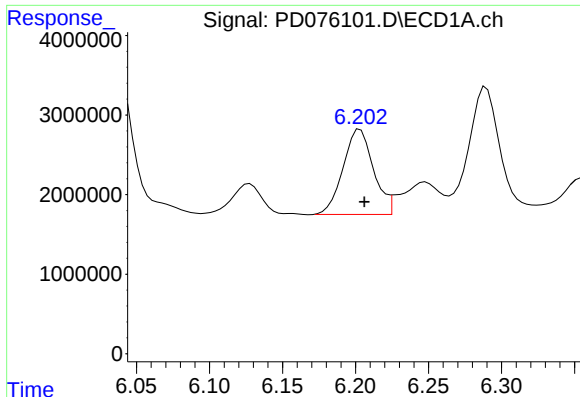


#12 4,4'-DDE

R.T.: 6.202 min
Delta R.T.: -0.004 min
Response: 15886065
Conc: 5.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSTIE-SB18-27


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/26/2023
Supervised By :Ankita Jodhani 06/26/2023

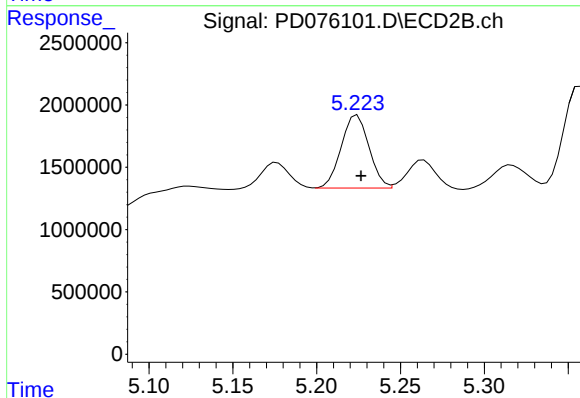


#12 4,4'-DDE

R.T.: 5.223 min
Delta R.T.: -0.004 min
Response: 6769993
Conc: 6.07 ng/ml m

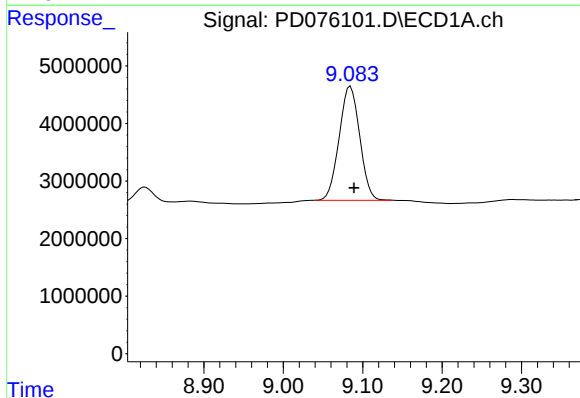

#28 Decachlorobiphenyl

R.T.: 9.083 min
Delta R.T.: -0.006 min
Response: 35608816
Conc: 14.06 ng/ml m

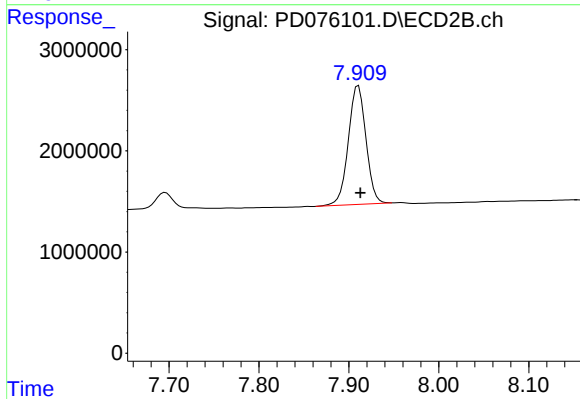

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.004 min
Response: 15991545
Conc: 16.35 ng/ml m