

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
 Data File : PD076108.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 17:08
 Operator : AR\AJ
 Sample : 03365-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 22:48:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.767	34712393	18291989	16.296	16.860
28)	SA Decachlor...	9.085	7.910	34125223	15410982	13.470	15.761
Target Compounds							
12)	B 4,4'-DDE	6.205	5.225	19218600	9104150	6.724	8.157
17)	MA 4,4'-DDT	7.038	6.031	6783818	2963804	2.989	3.649



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
Data File : PD076108.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 17:08
Operator : AR\AJ
Sample : 03365-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 22:48:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

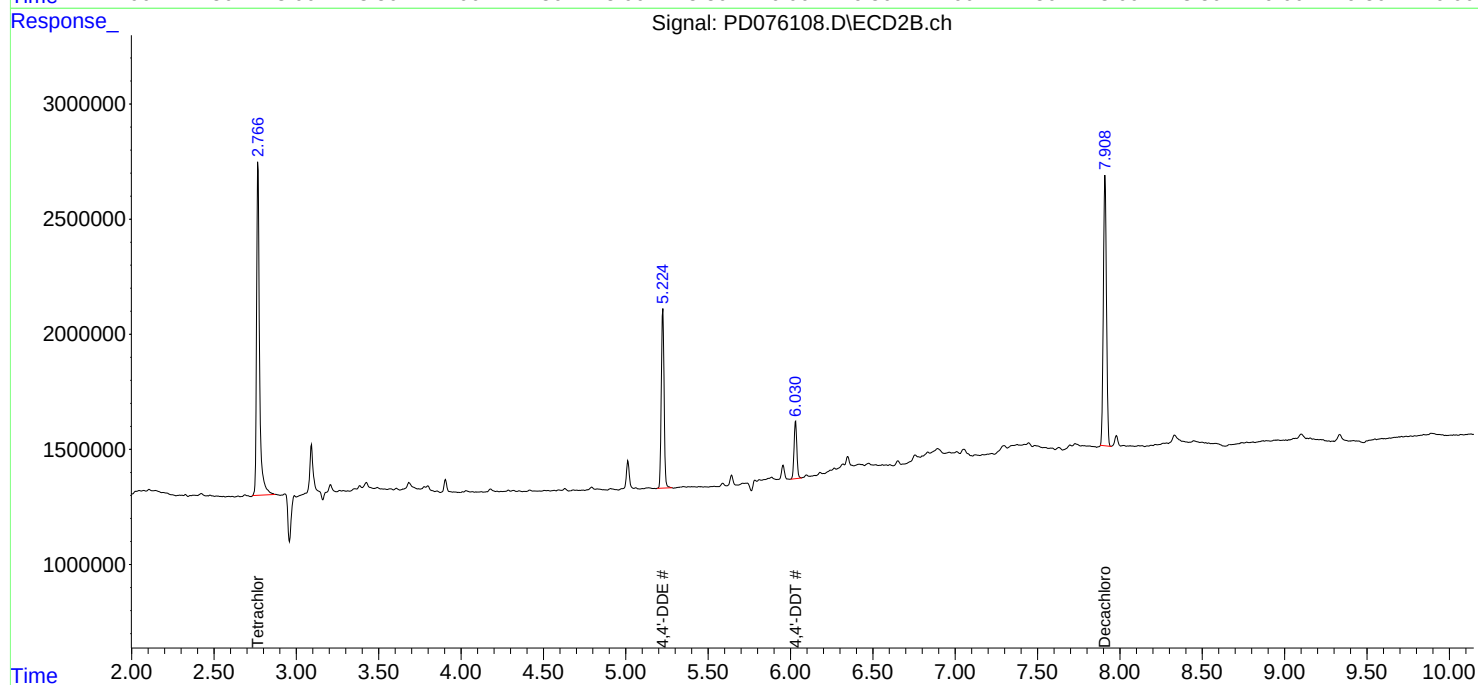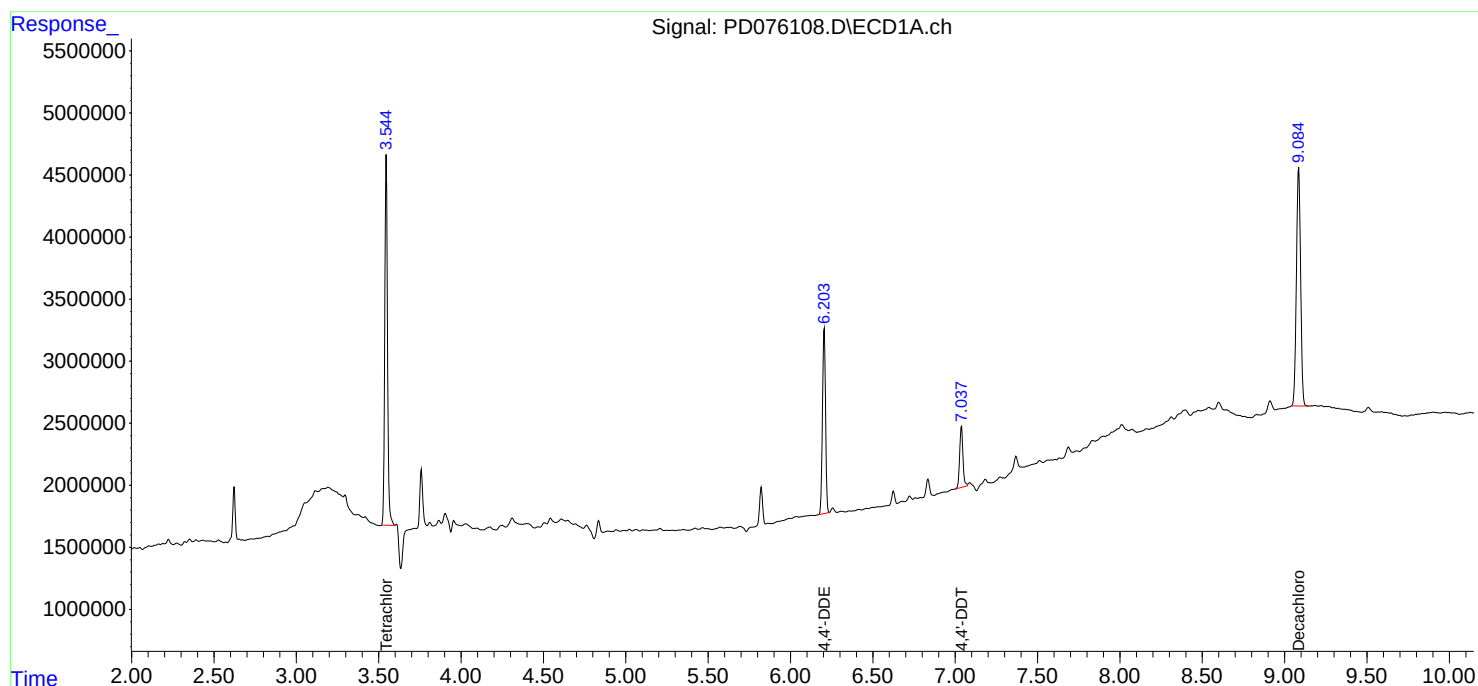


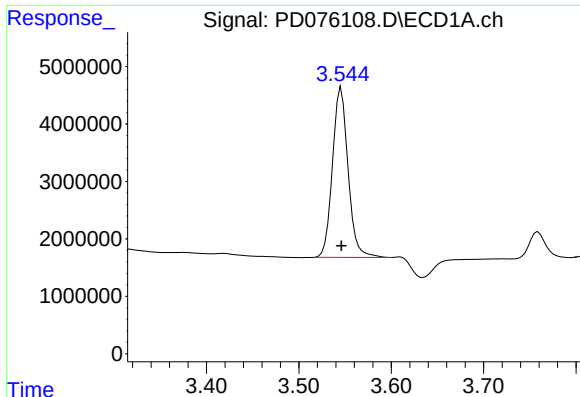

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 34712393
Conc: 16.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP1

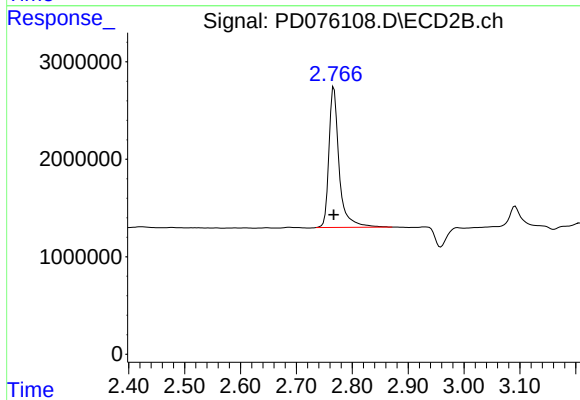


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 18291989
Conc: 16.86 ng/ml

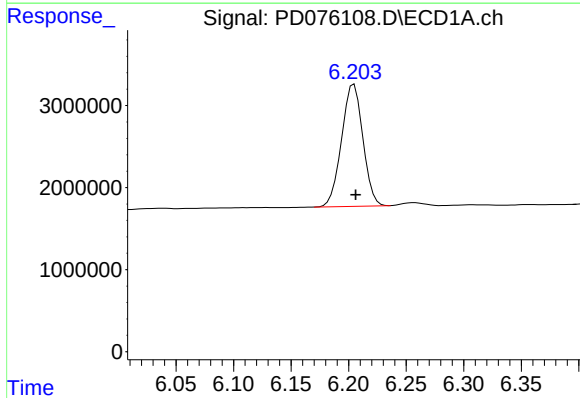


#12 4,4'-DDE

R.T.: 6.205 min
Delta R.T.: -0.001 min
Response: 19218600
Conc: 6.72 ng/ml

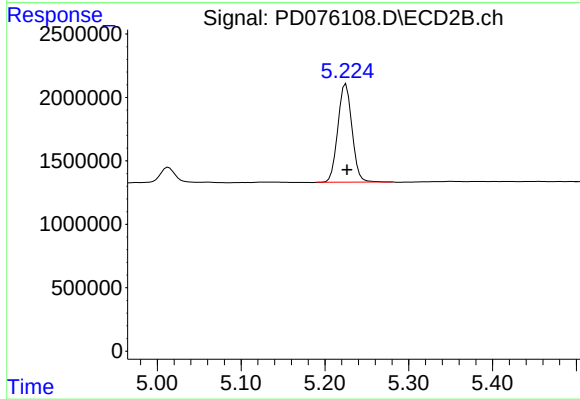

#12 4,4'-DDE


R.T.: 5.225 min
Delta R.T.: -0.001 min
Response: 9104150
Conc: 8.16 ng/ml

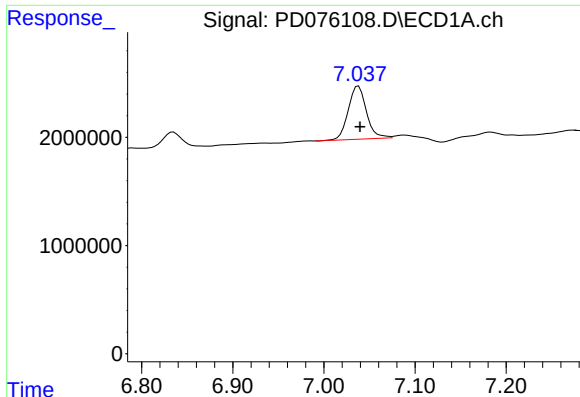

#17 4,4'-DDT


R.T.: 7.038 min
Delta R.T.: -0.002 min
Response: 6783818
Conc: 2.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP1

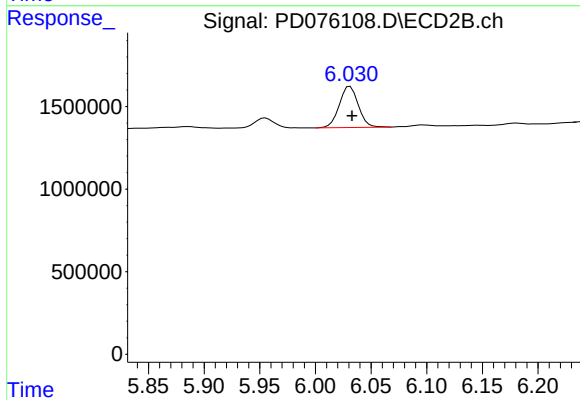


#17 4,4'-DDT

R.T.: 6.031 min
Delta R.T.: -0.002 min
Response: 2963804
Conc: 3.65 ng/ml

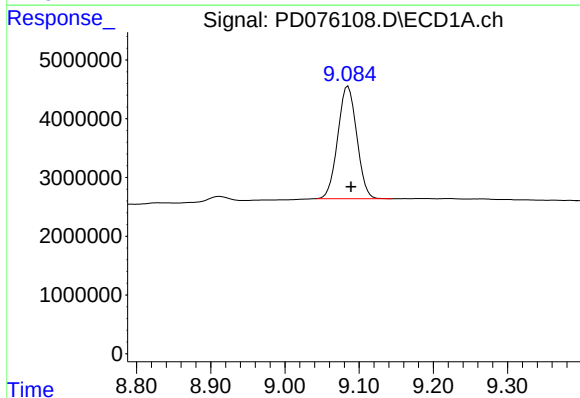

#28 Decachlorobiphenyl

R.T.: 9.085 min
Delta R.T.: -0.004 min
Response: 34125223
Conc: 13.47 ng/ml

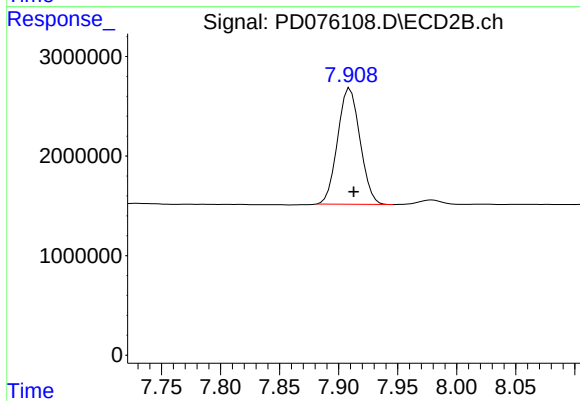

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.003 min
Response: 15410982
Conc: 15.76 ng/ml