

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
 Data File : PD076110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jun 2023 17:35
 Operator : AR\AJ
 Sample : 03365-24MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP1MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 22:50:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.766	32978363	17317195	15.482	15.962
28)	SA Decachlor...	9.086	7.911	33255429	14627308	13.127	14.959
Target Compounds							
12)	B 4,4'-DDE	6.205	5.225	18772287	8590356	6.568	7.696
17)	MA 4,4'-DDT	7.038	6.032	6558560	2683485	2.890	3.304



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062523\
Data File : PD076110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jun 2023 17:35
Operator : AR\AJ
Sample : 03365-24MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
TP1MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 22:50:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

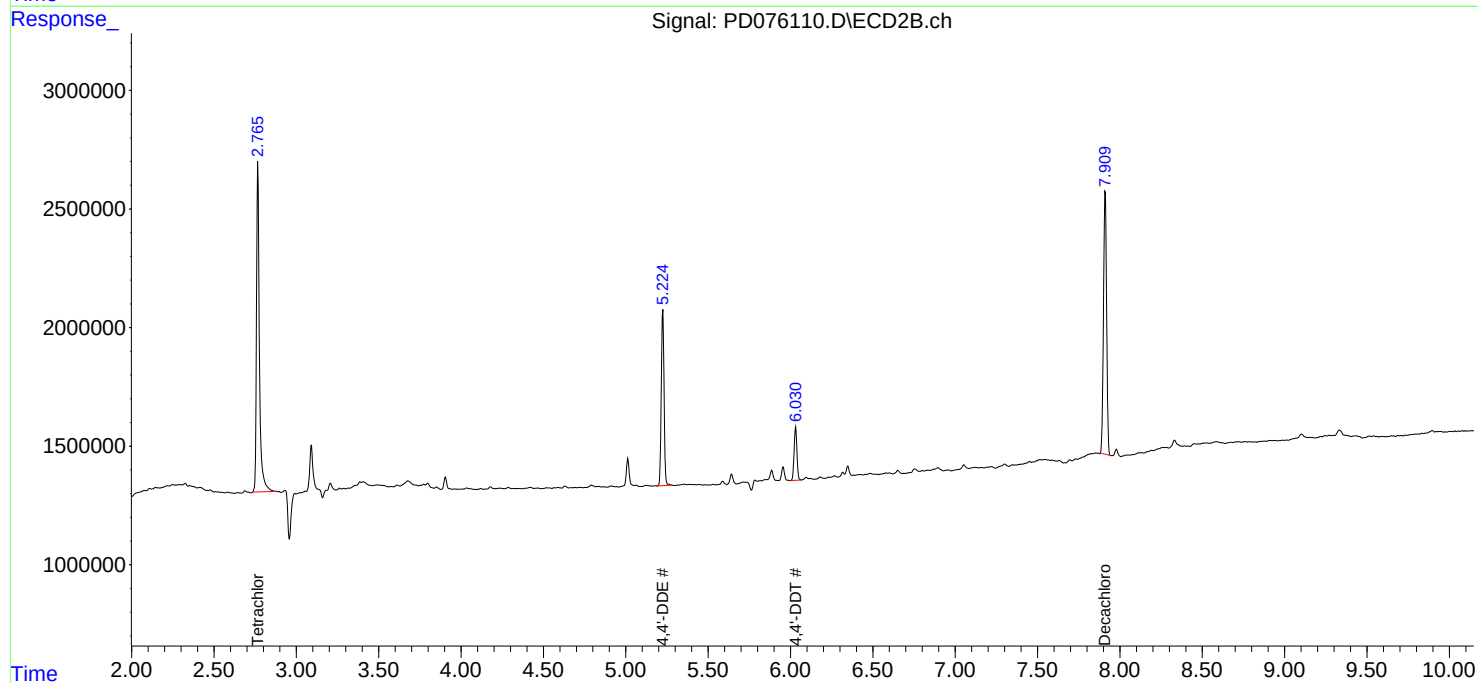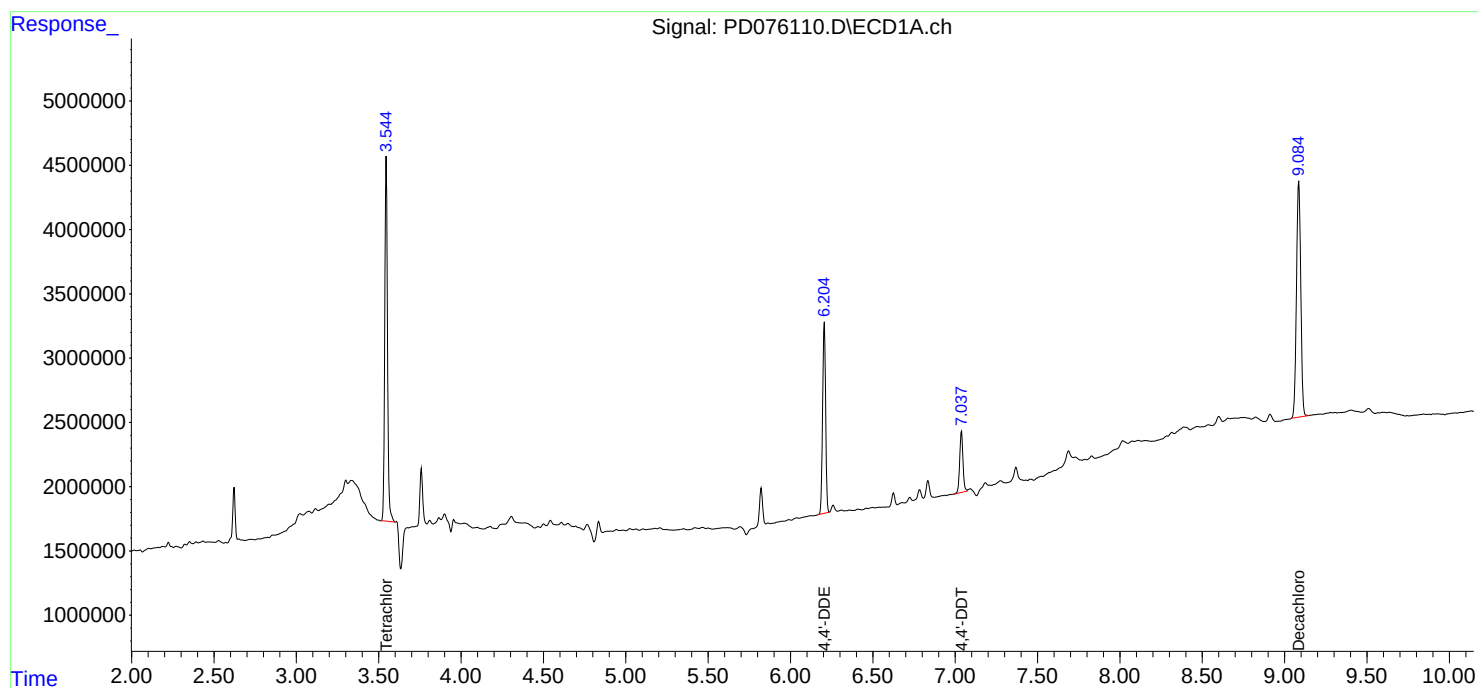


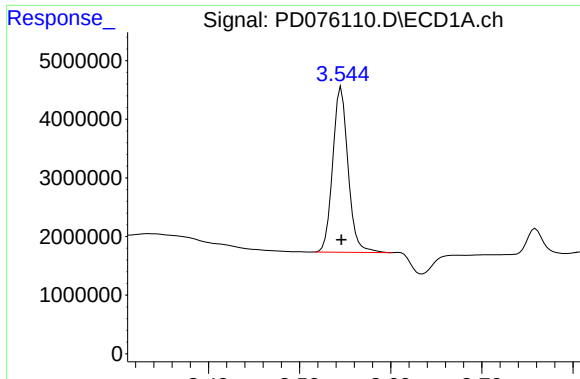

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 32978363
Conc: 15.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP1MSD

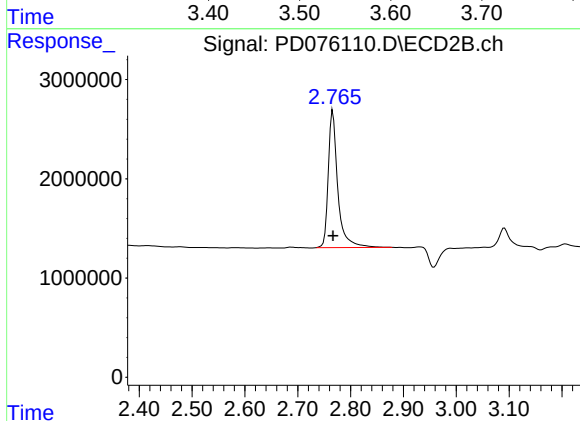


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 17317195
Conc: 15.96 ng/ml

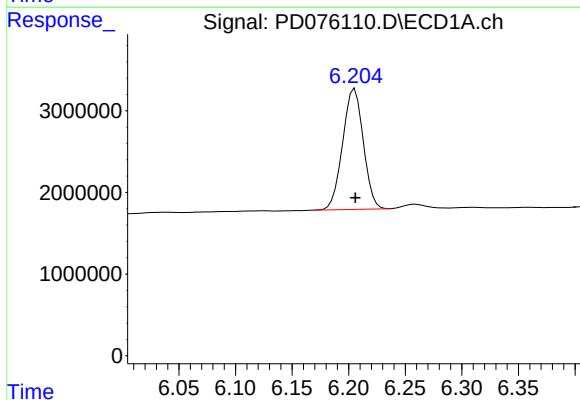


#12 4,4'-DDE

R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 18772287
Conc: 6.57 ng/ml

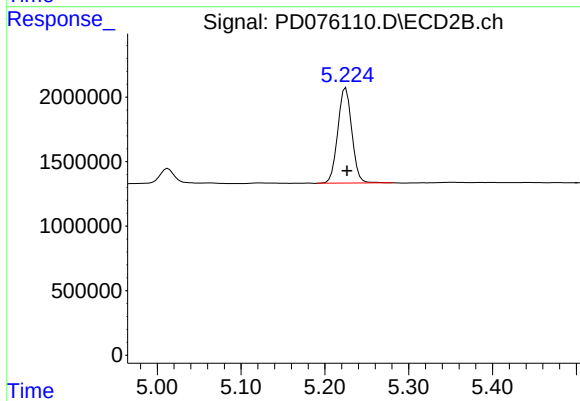

#12 4,4'-DDE


R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 8590356
Conc: 7.70 ng/ml

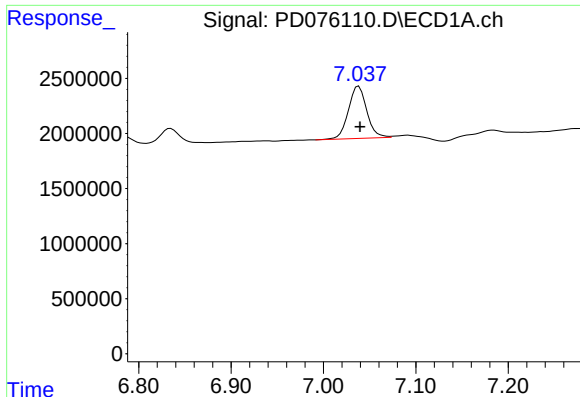

#17 4,4'-DDT


R.T.: 7.038 min
Delta R.T.: -0.001 min
Response: 6558560
Conc: 2.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP1MSD

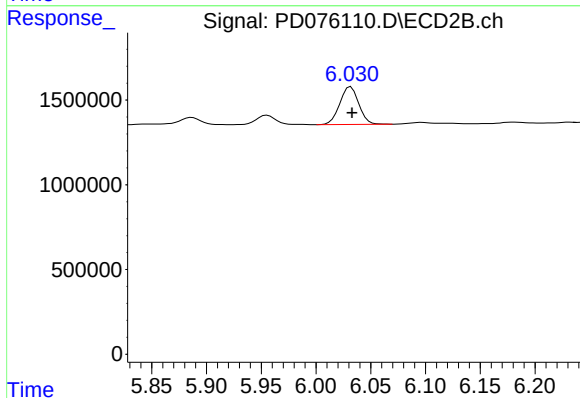


#17 4,4'-DDT

R.T.: 6.032 min
Delta R.T.: -0.001 min
Response: 2683485
Conc: 3.30 ng/ml

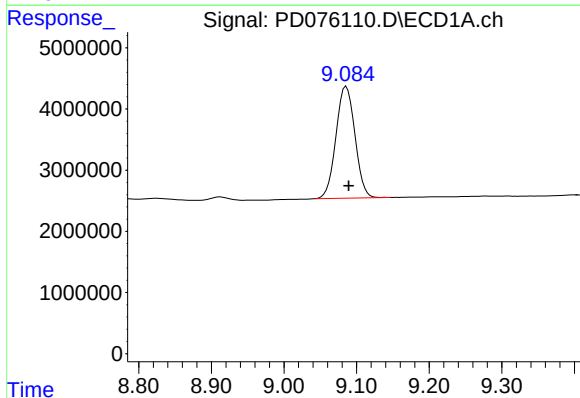

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: -0.003 min
Response: 33255429
Conc: 13.13 ng/ml

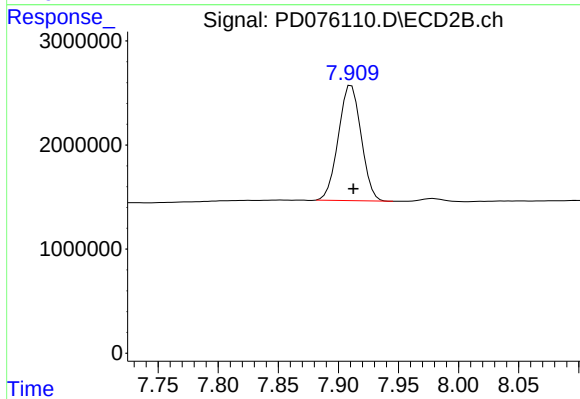

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.002 min
Response: 14627308
Conc: 14.96 ng/ml