

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062623\
 Data File : PD076161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2023 18:48
 Operator : AR\AJ
 Sample : PB153702TB
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB153702TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:24:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.767	43060338	21699021	20.215	20.000
28)	SA Decachlor...	9.087	7.911	49307680	20920034	19.463	21.395
Target Compounds							
7)	B delta-BHC	4.772	0.000	1587712	0	0.478	N.D. #
8)	B Heptachlo...	5.692	0.000	1154182	0	0.358	N.D. #
9)	A Endosulfan I	6.093	0.000	223256	0	0.074	N.D. #
10)	B gamma-Chl...	5.953	0.000	177342	0	0.055	N.D. #
11)	B alpha-Chl...	6.020	0.000	82125	0	0.025	N.D. #
15)	B Endosulfa...	6.837f	0.000	240862	0	0.093	N.D. #
21)	B Endrin ke...	7.690f	0.000	1327423	0	0.476	N.D. #
22)	Mirex	8.164f	0.000	306255	0	0.143	N.D. #
25)	Chlordane-3	5.953	0.000	177342	0	0.341	N.D. #
26)	Chlordane-4	6.020f	0.000	82125	0	0.130	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062623\
Data File : PD076161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2023 18:48
Operator : AR\AJ
Sample : PB153702TB
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB153702TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:24:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

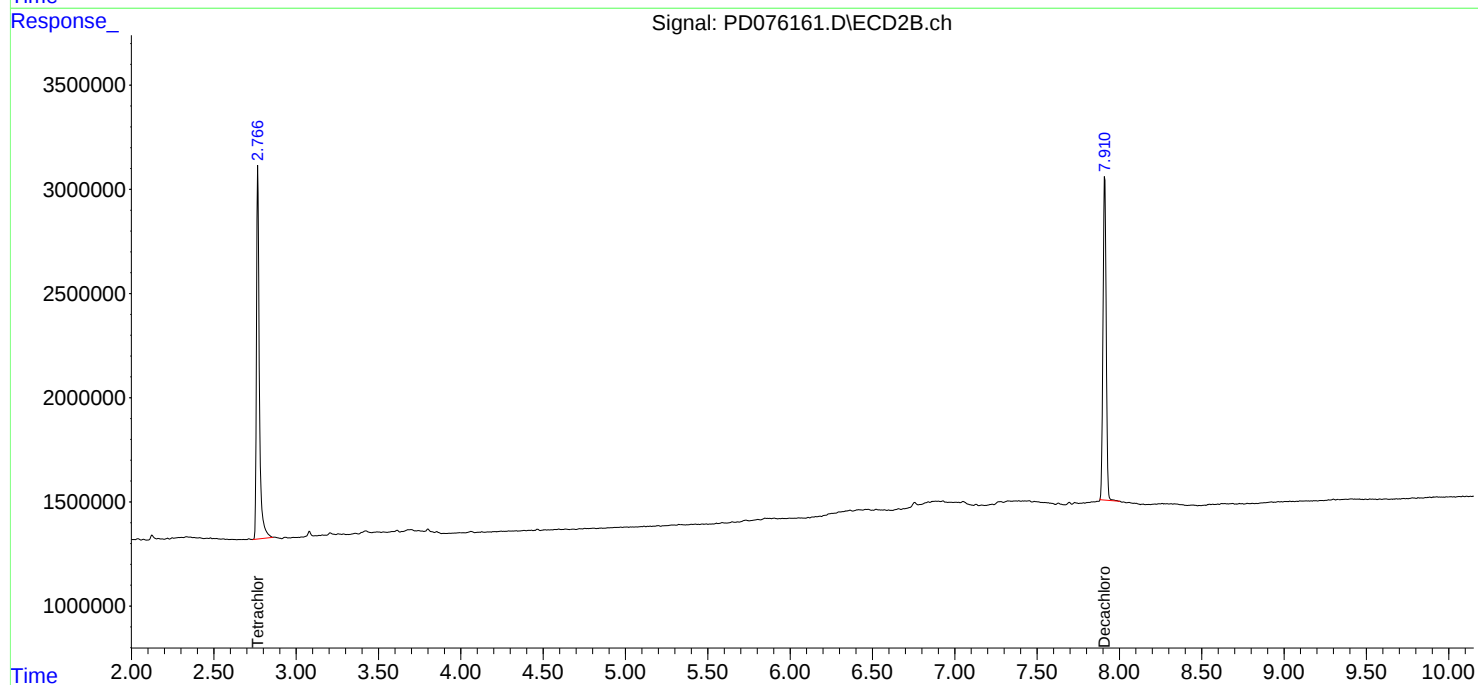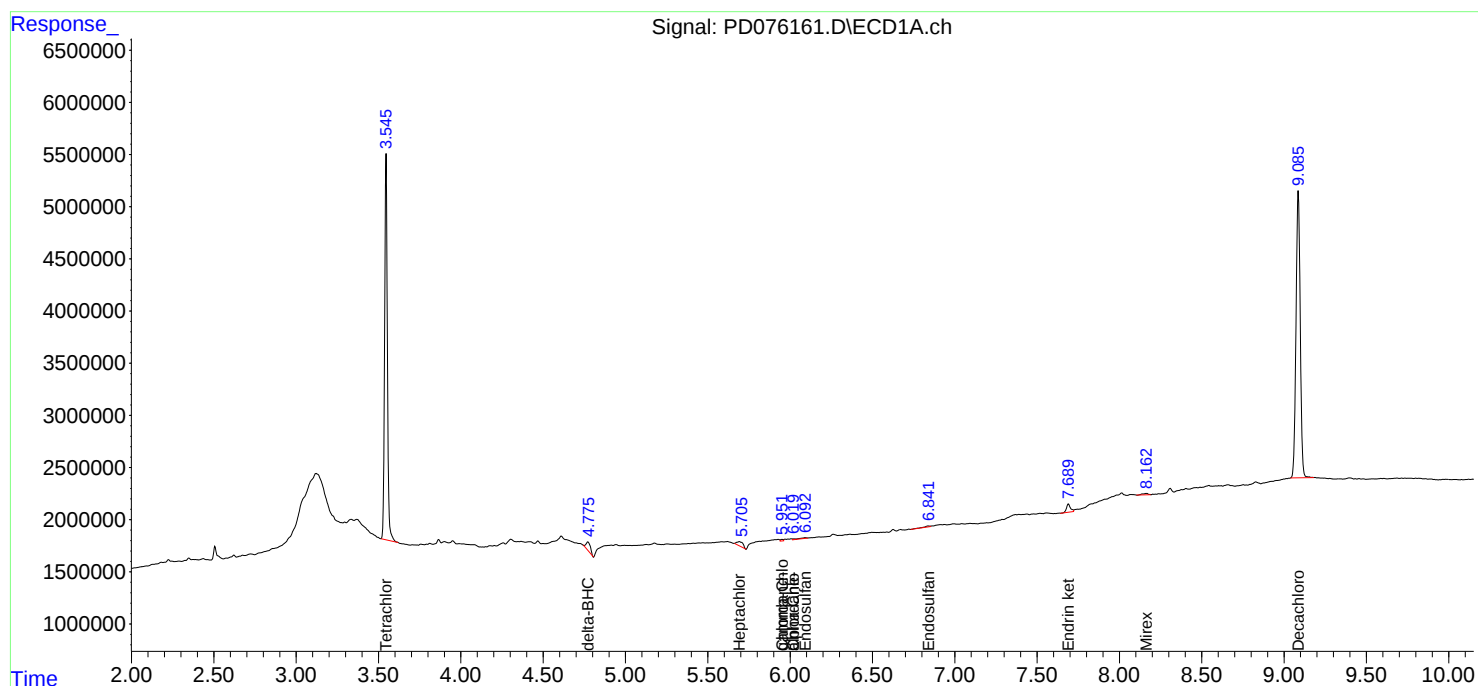


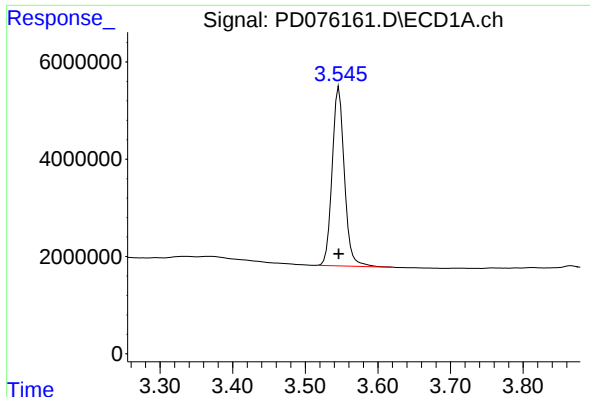

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 43060338
Conc: 20.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153702TB

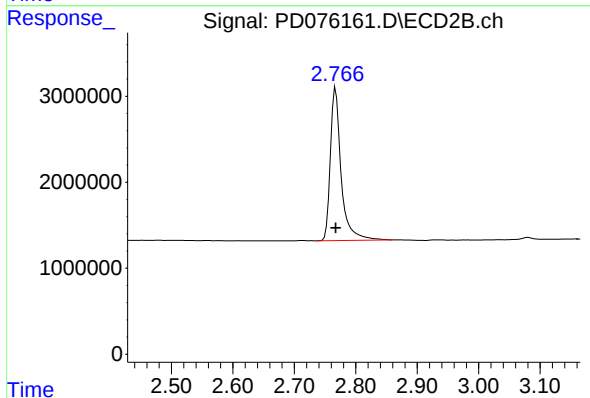


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 21699021
Conc: 20.00 ng/ml

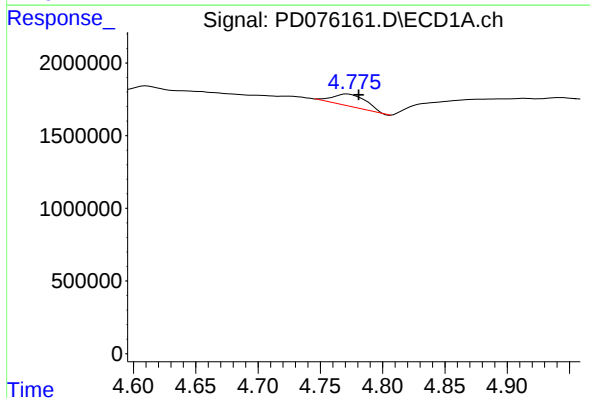


#7 delta-BHC

R.T.: 4.772 min
Delta R.T.: -0.009 min
Response: 1587712
Conc: 0.48 ng/ml

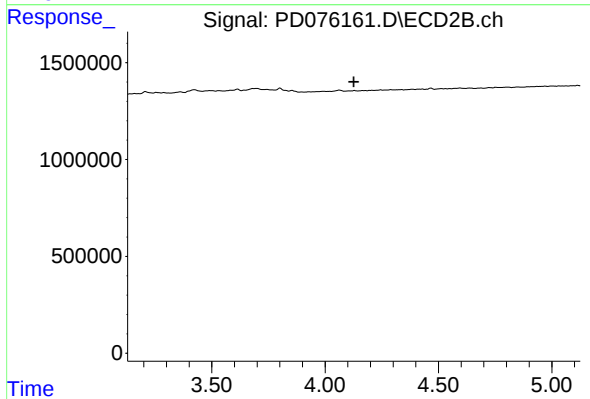

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

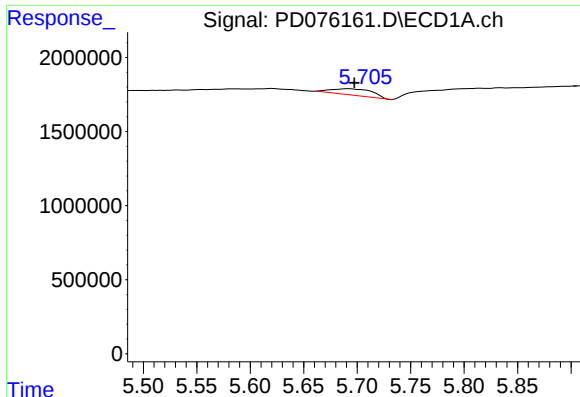

#8 Heptachlor epoxide


R.T.: 5.692 min
Delta R.T.: -0.005 min
Response: 1154182
Conc: 0.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153702TB

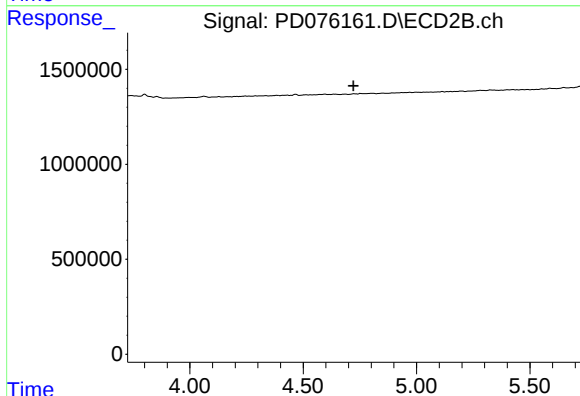


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

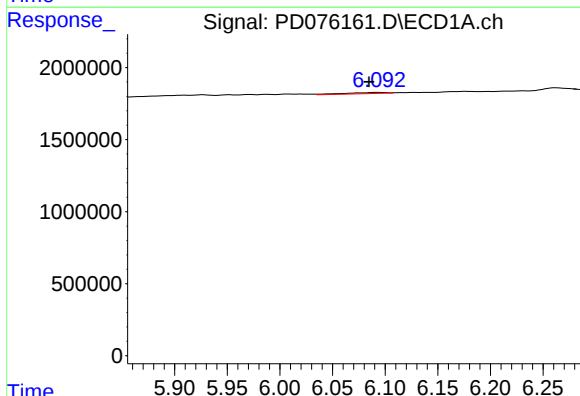


#9 Endosulfan I

R.T.: 6.093 min
Delta R.T.: 0.008 min
Response: 223256
Conc: 0.07 ng/ml

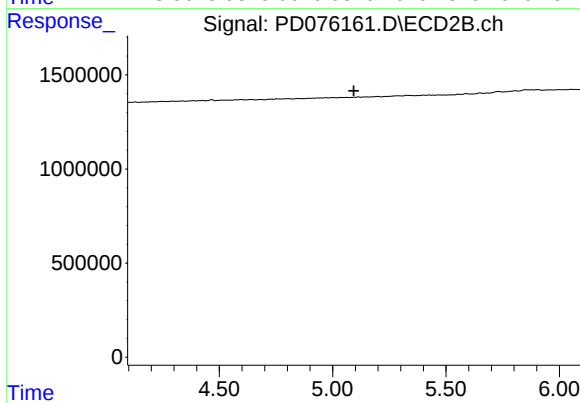

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

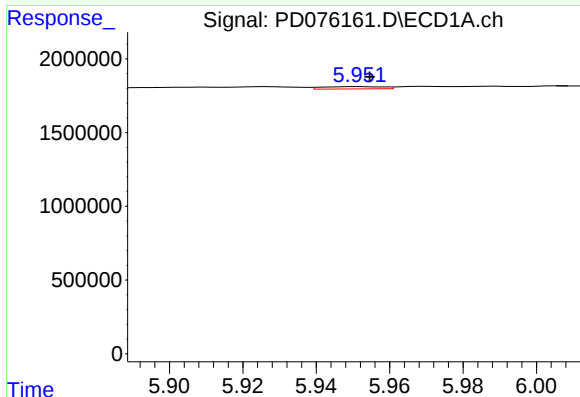

#10 gamma-Chlordane


R.T.: 5.953 min
Delta R.T.: -0.002 min
Response: 177342
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153702TB

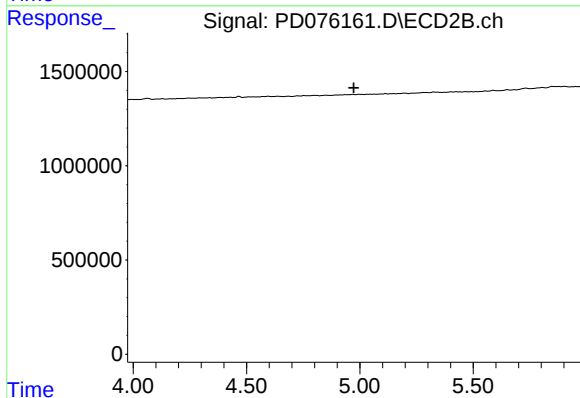


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

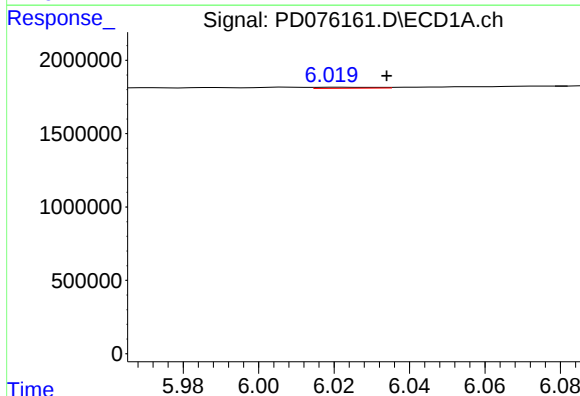


#11 alpha-Chlordane

R.T.: 6.020 min
Delta R.T.: -0.014 min
Response: 82125
Conc: 0.03 ng/ml

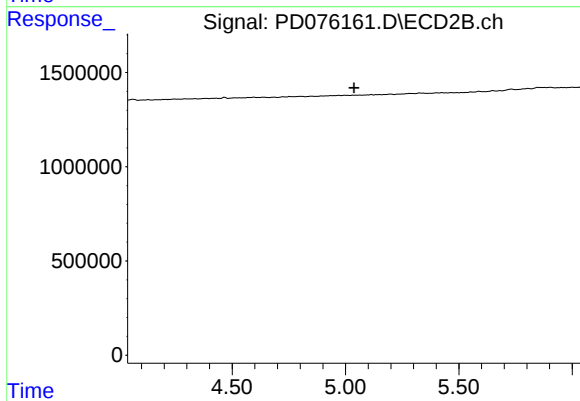

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

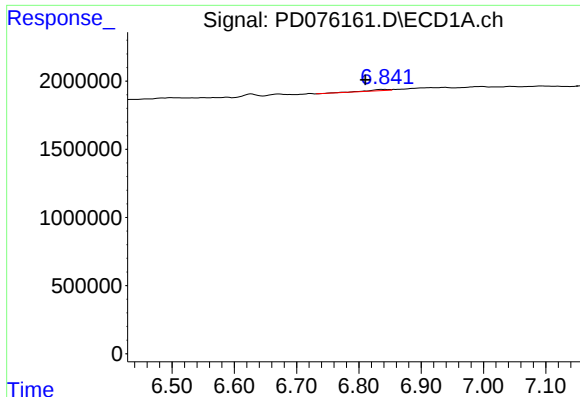

#15 Endosulfan II


R.T.: 6.837 min
Delta R.T.: 0.027 min
Response: 240862
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153702TB

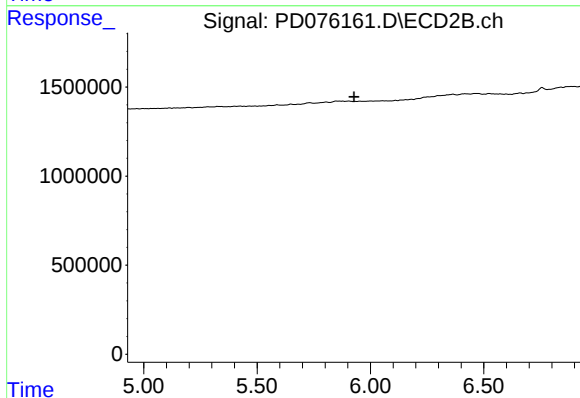


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

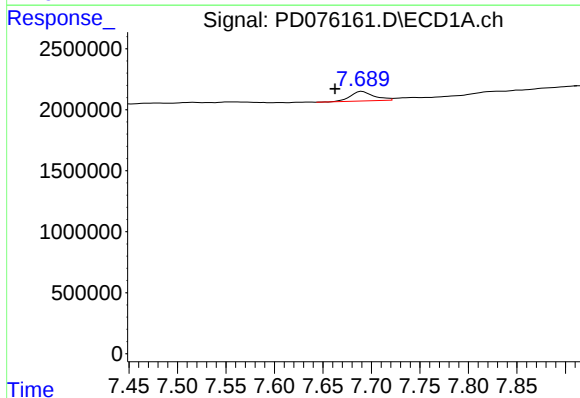


#21 Endrin ketone

R.T.: 7.690 min
Delta R.T.: 0.028 min
Response: 1327423
Conc: 0.48 ng/ml

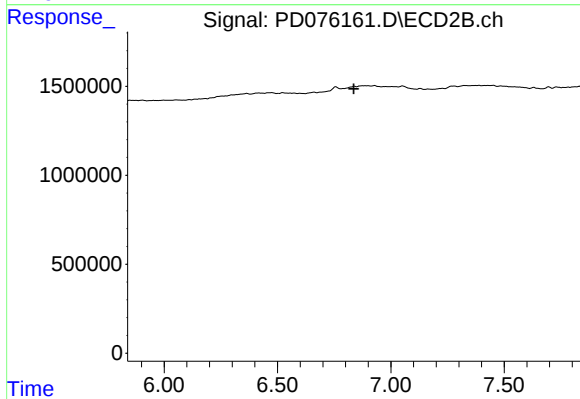

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

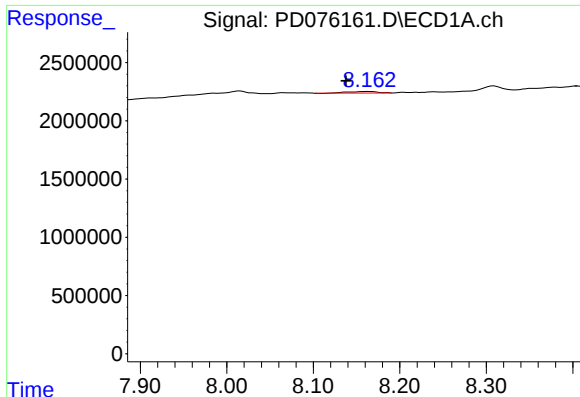

#22 Mirex


R.T.: 8.164 min
Delta R.T.: 0.026 min
Response: 306255
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153702TB

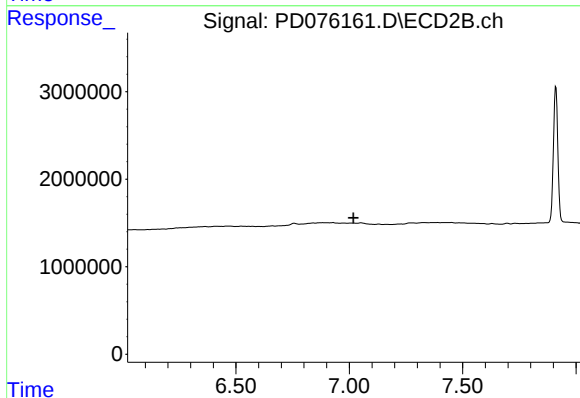


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.019 min
Response: 0
Conc: N.D.

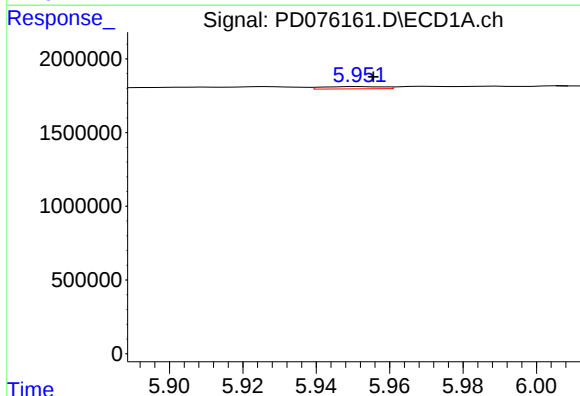


#25 Chlordane-3

R.T.: 5.953 min
Delta R.T.: -0.003 min
Response: 177342
Conc: 0.34 ng/ml

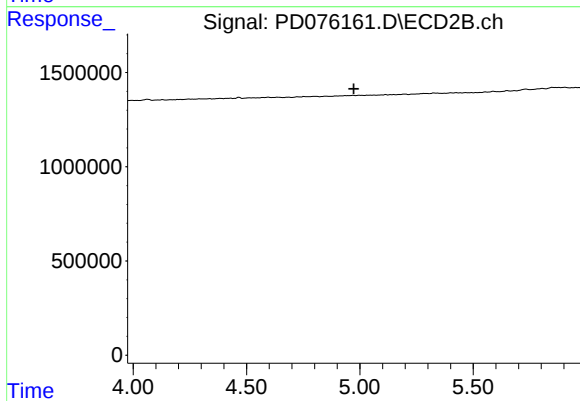

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

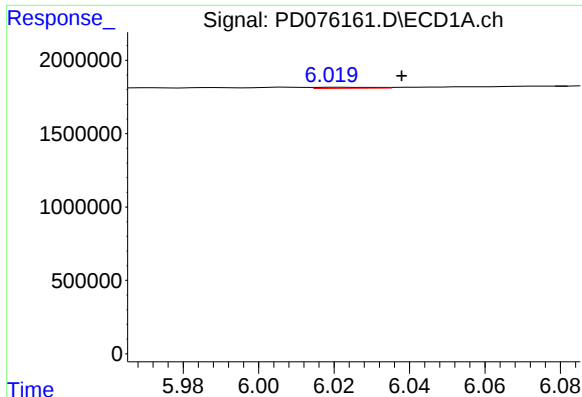

#26 Chlordane-4


R.T.: 6.020 min
Delta R.T.: -0.018 min
Response: 82125
Conc: 0.13 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153702TB

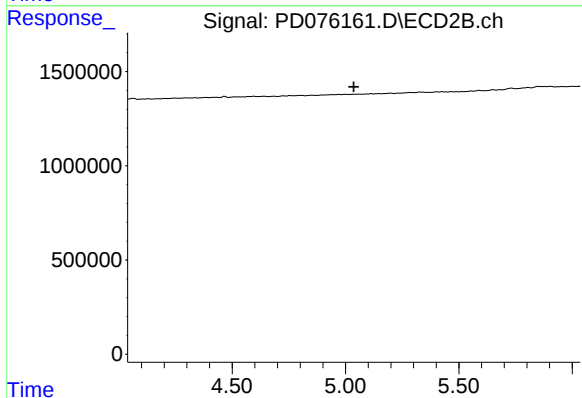


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

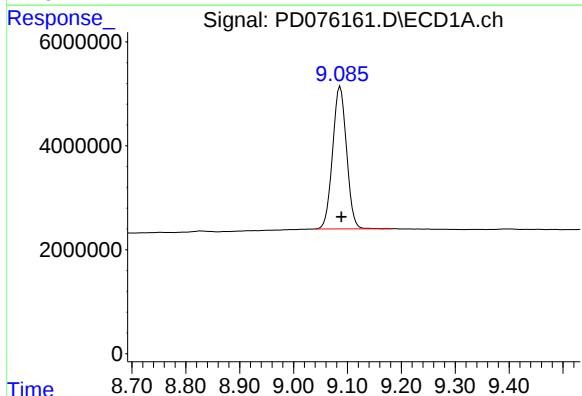

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.002 min
Response: 49307680
Conc: 19.46 ng/ml

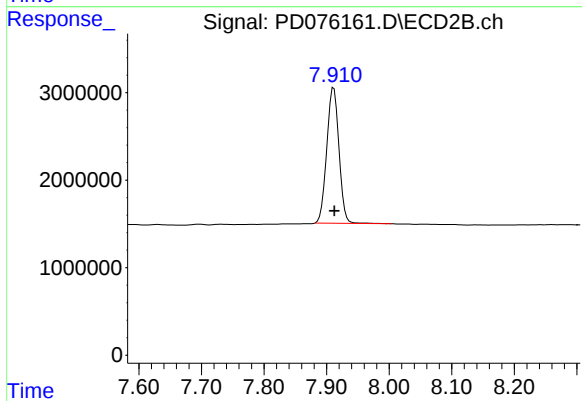

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.001 min
Response: 20920034
Conc: 21.40 ng/ml