

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD062623\  
 Data File : PD076151.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Jun 2023 16:22  
 Operator : AR\AJ  
 Sample : 03357-02  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 WC-SCAN-01

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 26 01:19:51 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD061523.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Jun 16 10:43:19 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.548 | 2.767 | 33949500 | 18467999 | 15.938 | 17.022 |
| 28)                         | SA Decachlor... | 9.090 | 7.912 | 40299565 | 17587946 | 15.908 | 17.987 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD062623\  
Data File : PD076151.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Jun 2023 16:22  
Operator : AR\AJ  
Sample : 03357-02  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
WC-SCAN-01

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 26 01:19:51 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD061523.M  
Quant Title : GC Extractables  
QLast Update : Fri Jun 16 10:43:19 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

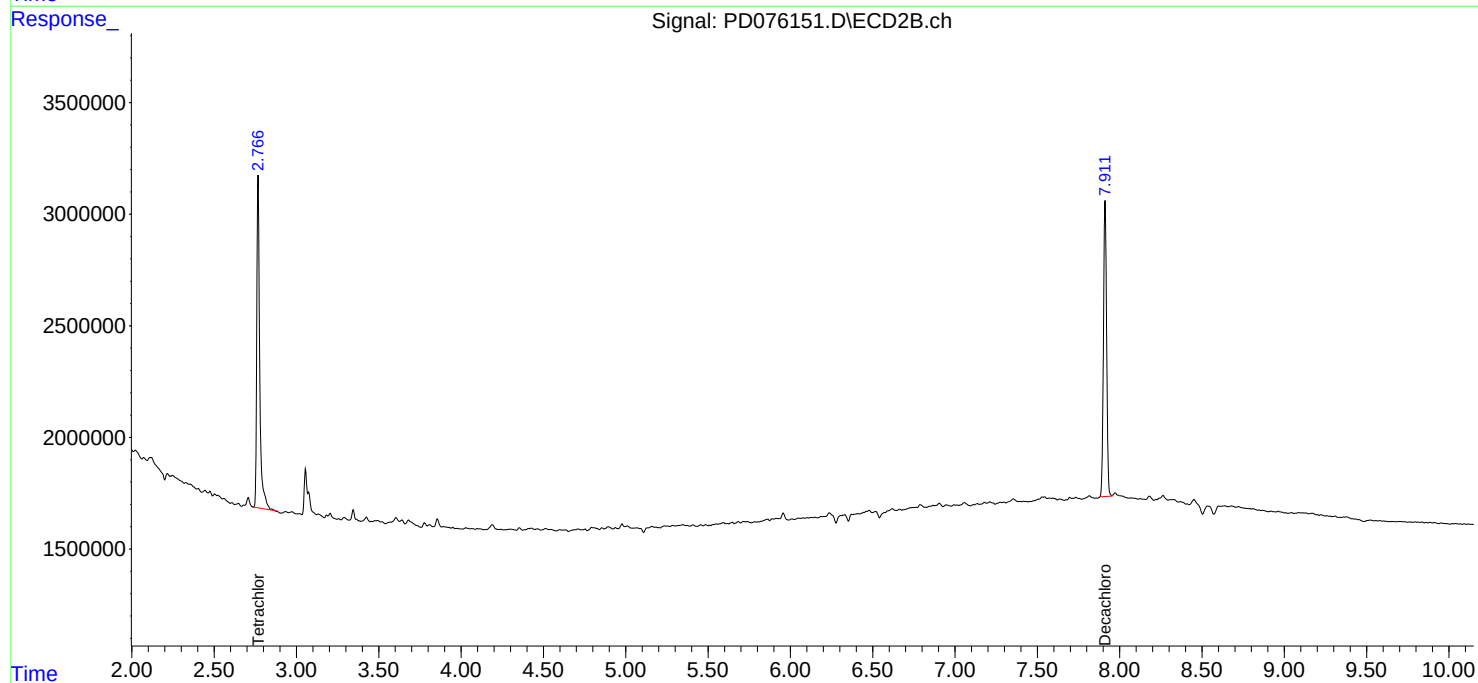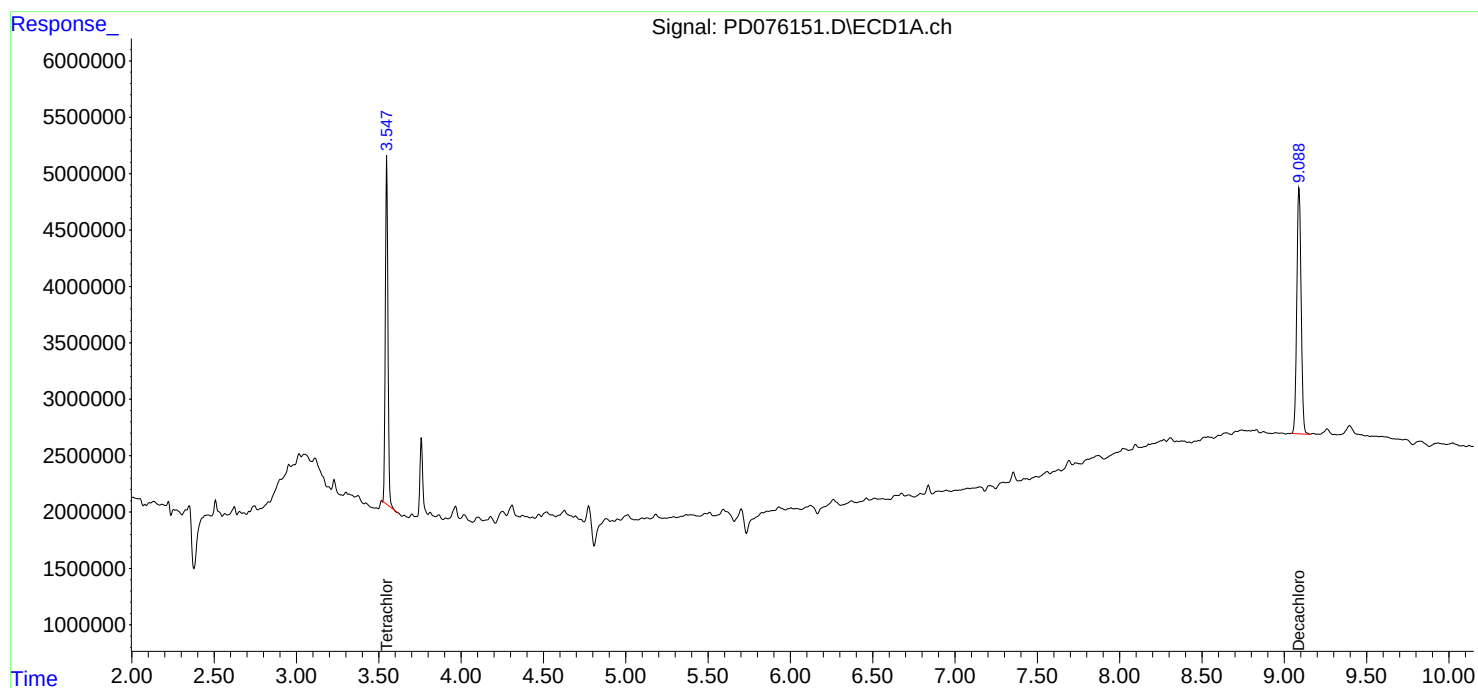


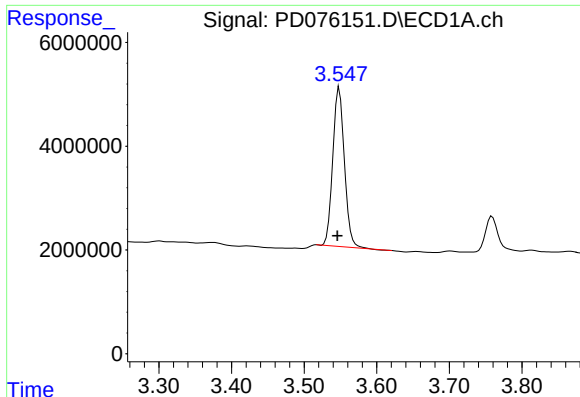

#1 Tetrachloro-m-xylene


R.T.: 3.548 min  
Delta R.T.: 0.002 min  
Response: 33949500  
Conc: 15.94 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
WC-SCAN-01

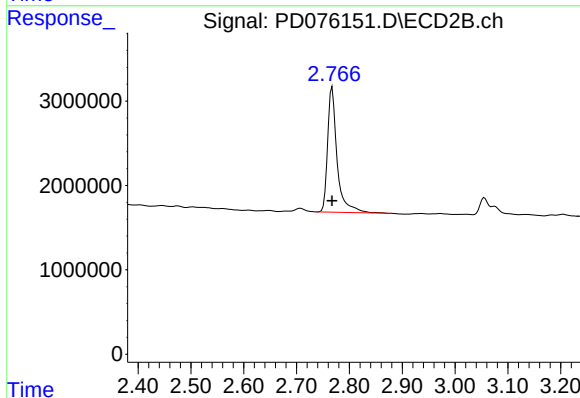


#1 Tetrachloro-m-xylene

R.T.: 2.767 min  
Delta R.T.: 0.000 min  
Response: 18467999  
Conc: 17.02 ng/ml

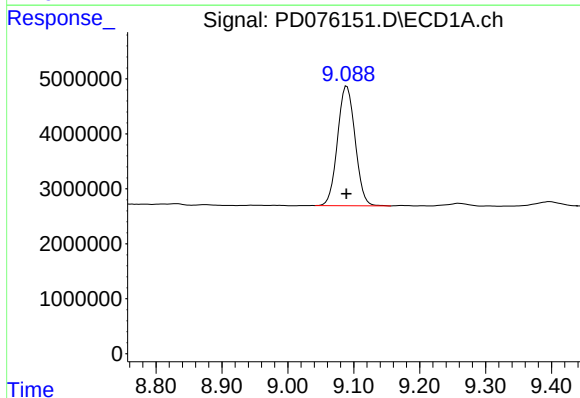

#28 Decachlorobiphenyl

R.T.: 9.090 min  
Delta R.T.: 0.000 min  
Response: 40299565  
Conc: 15.91 ng/ml

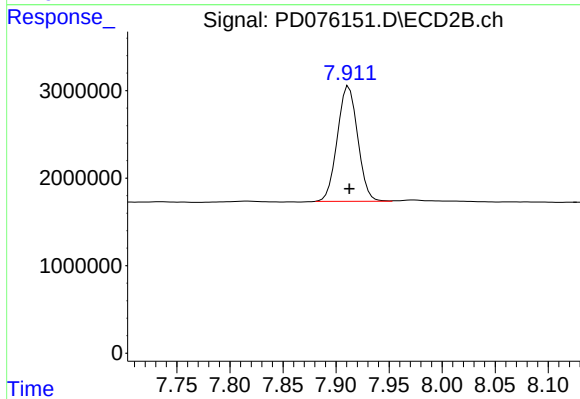

#28 Decachlorobiphenyl

R.T.: 7.912 min  
Delta R.T.: 0.000 min  
Response: 17587946  
Conc: 17.99 ng/ml