

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062623\
 Data File : PD076155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2023 17:27
 Operator : AR\AJ
 Sample : 03357-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-SCAN-03

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/26/2023
 Supervised By : Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:21:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.550	2.766	34804749	18095576	16.339m	16.679
28) SA Decachlor...	9.096	7.913	35377624	15431436	13.965	15.782

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062623\
Data File : PD076155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2023 17:27
Operator : AR\AJ
Sample : 03357-12
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
WC-SCAN-03


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/26/2023
Supervised By : Ankita Jodhani 06/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:21:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

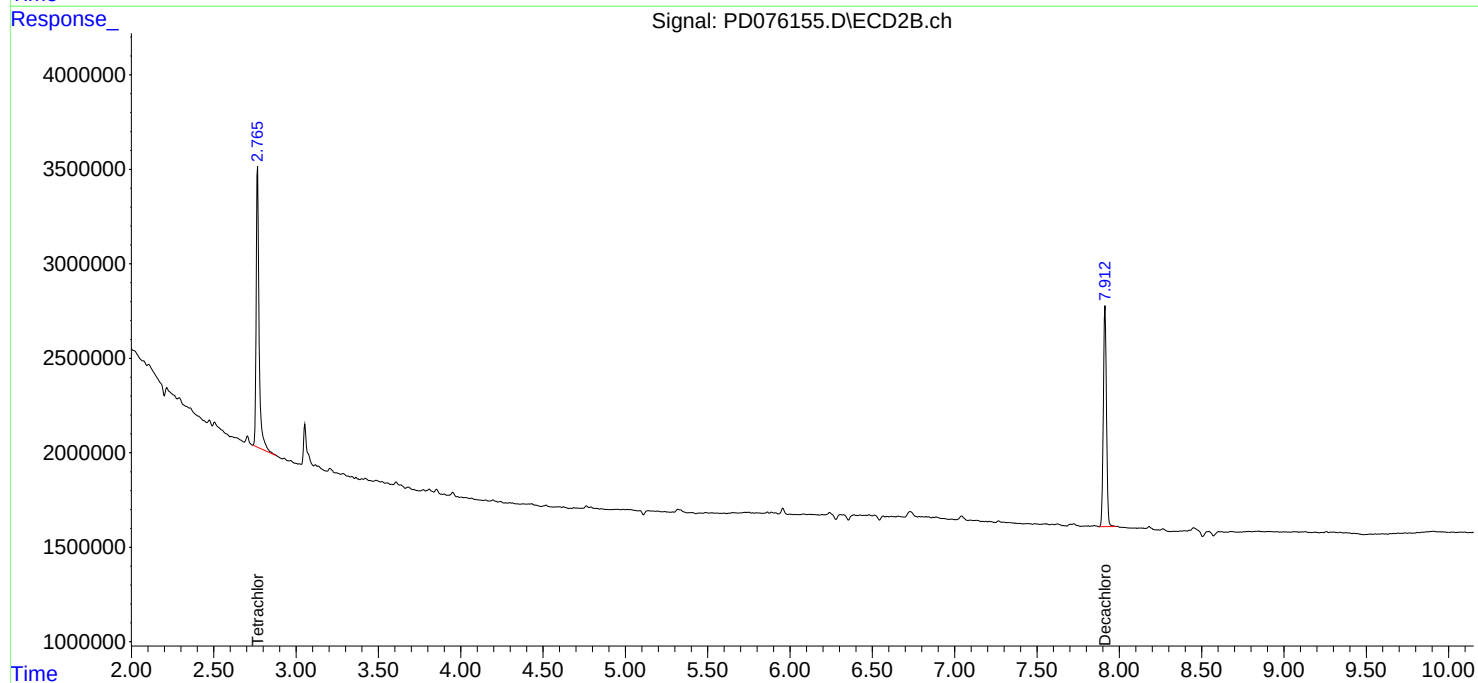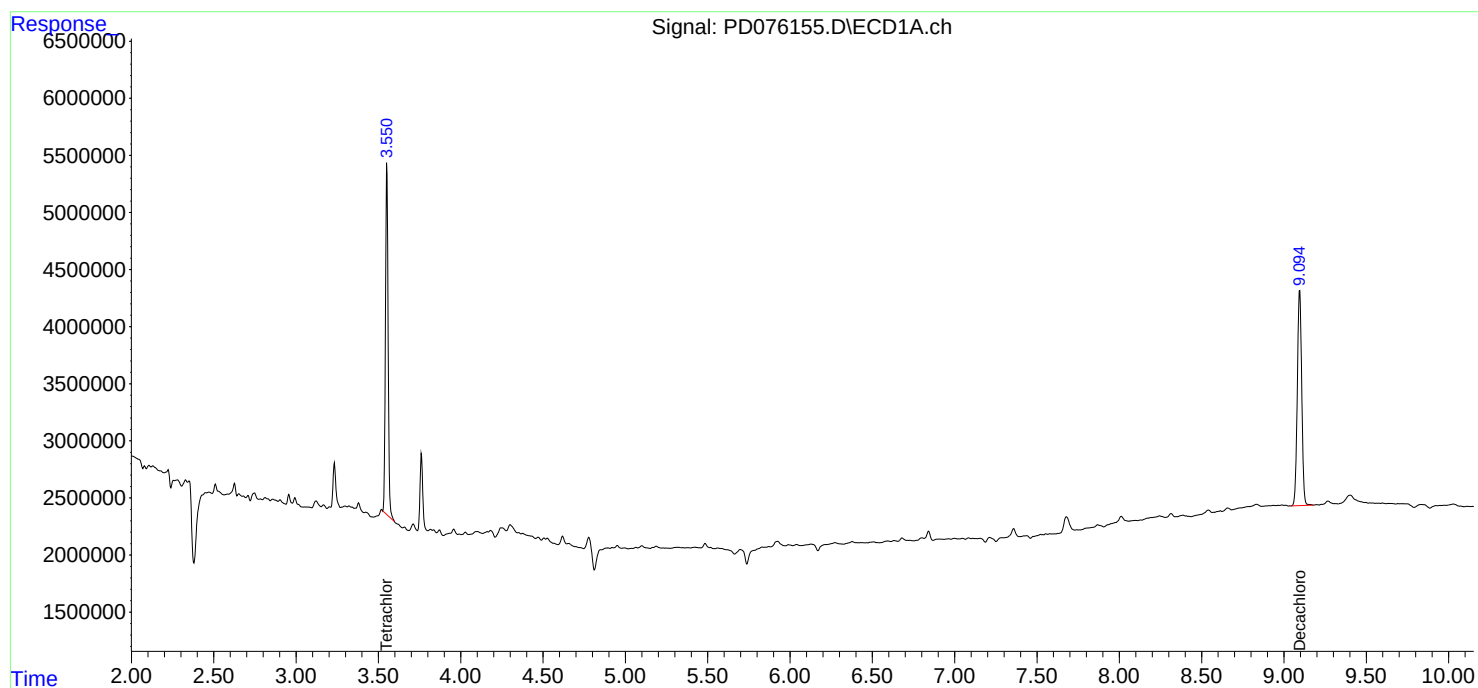

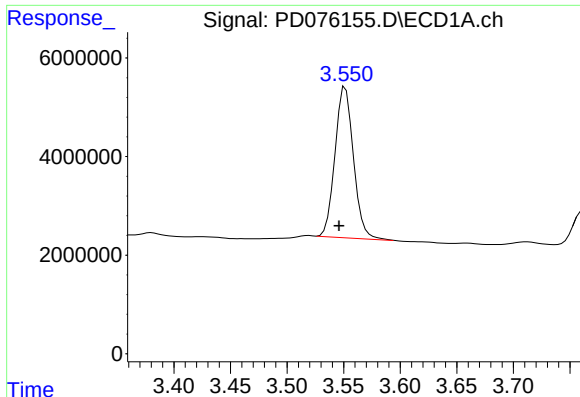

#1 Tetrachloro-m-xylene

R.T.: 3.550 min
Delta R.T.: 0.004 min
Response: 34804749
Conc: 16.34 ng/ml

Instrument :

ECD_D

ClientSampleId :


WC-SCAN-03

Manual Integrations

APPROVED


Reviewed By :Abdul Mirza 06/26/2023

Supervised By :Ankita Jodhani 06/27/2023

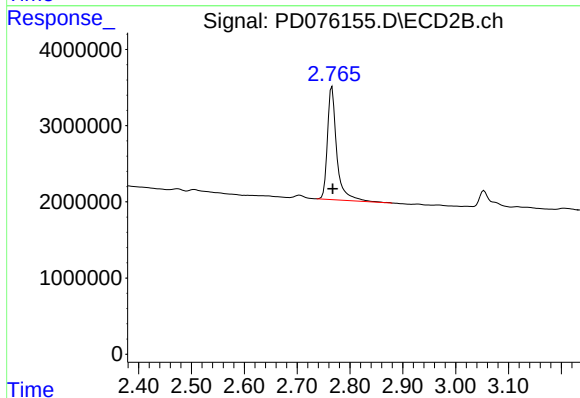


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: -0.001 min
Response: 18095576
Conc: 16.68 ng/ml

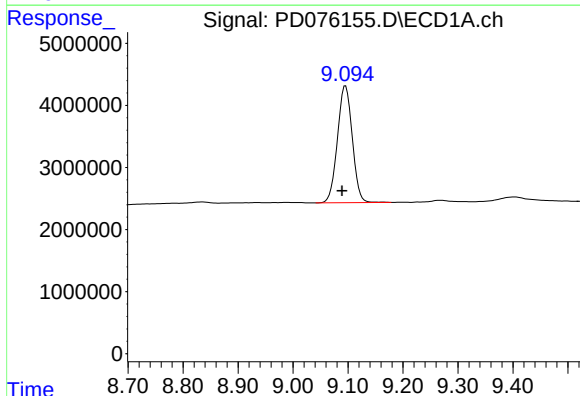

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.006 min
Response: 35377624
Conc: 13.96 ng/ml

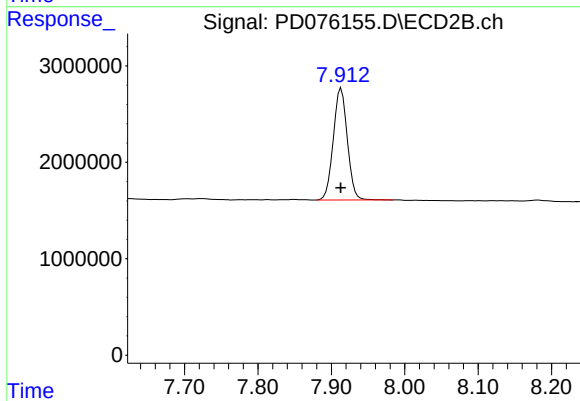

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 15431436
Conc: 15.78 ng/ml