

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062623\
 Data File : PD076182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2023 00:56
 Operator : AR\AJ
 Sample : 03393-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SF-9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 26 01:31:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.767	23021327	11918906	10.807	10.986
28) SA Decachlor...	9.087	7.910	27605687	12504821	10.897	12.789
Target Compounds						
11) B alpha-Chl...	6.037	5.035	13984564	3217555	4.326	2.346 #
12) B 4,4'-DDE	6.204	5.225	4790162	1885410	1.676	1.689



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062623\
Data File : PD076182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2023 00:56
Operator : AR\AJ
Sample : 03393-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SF-9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 01:31:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

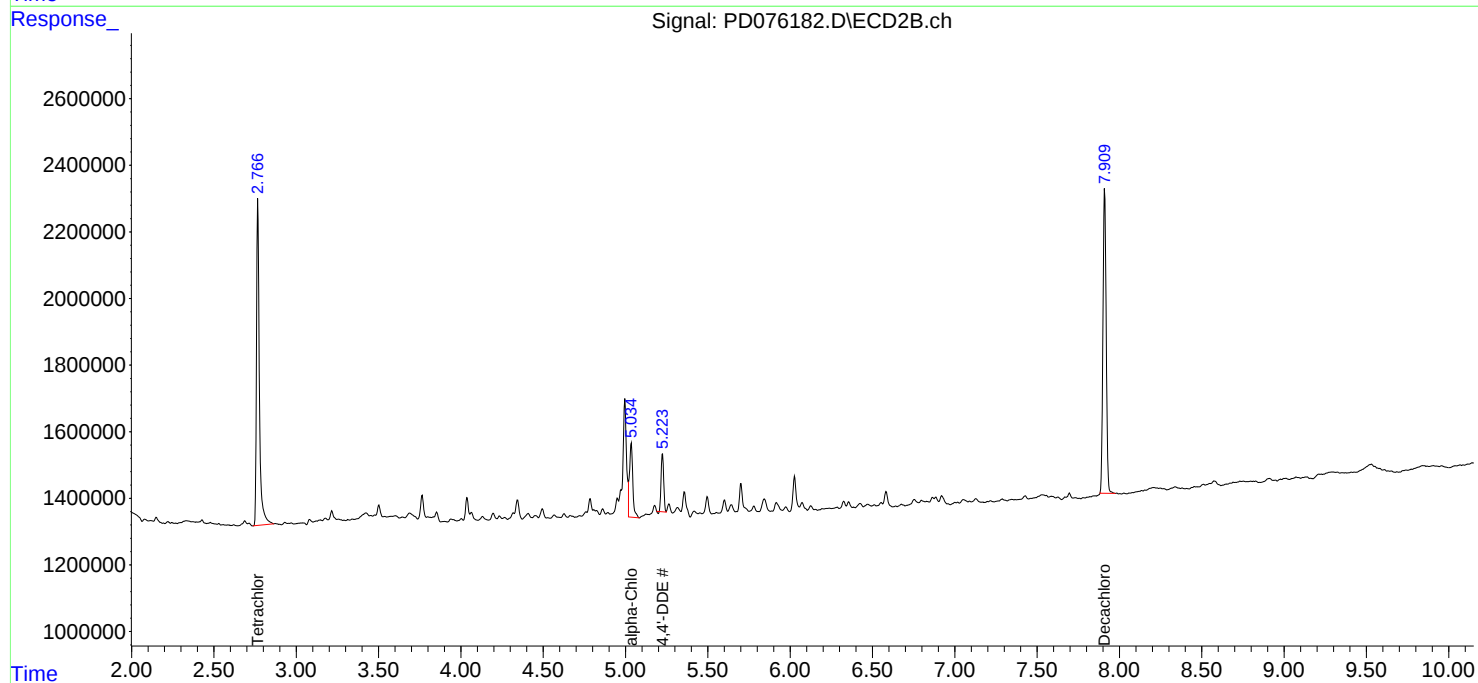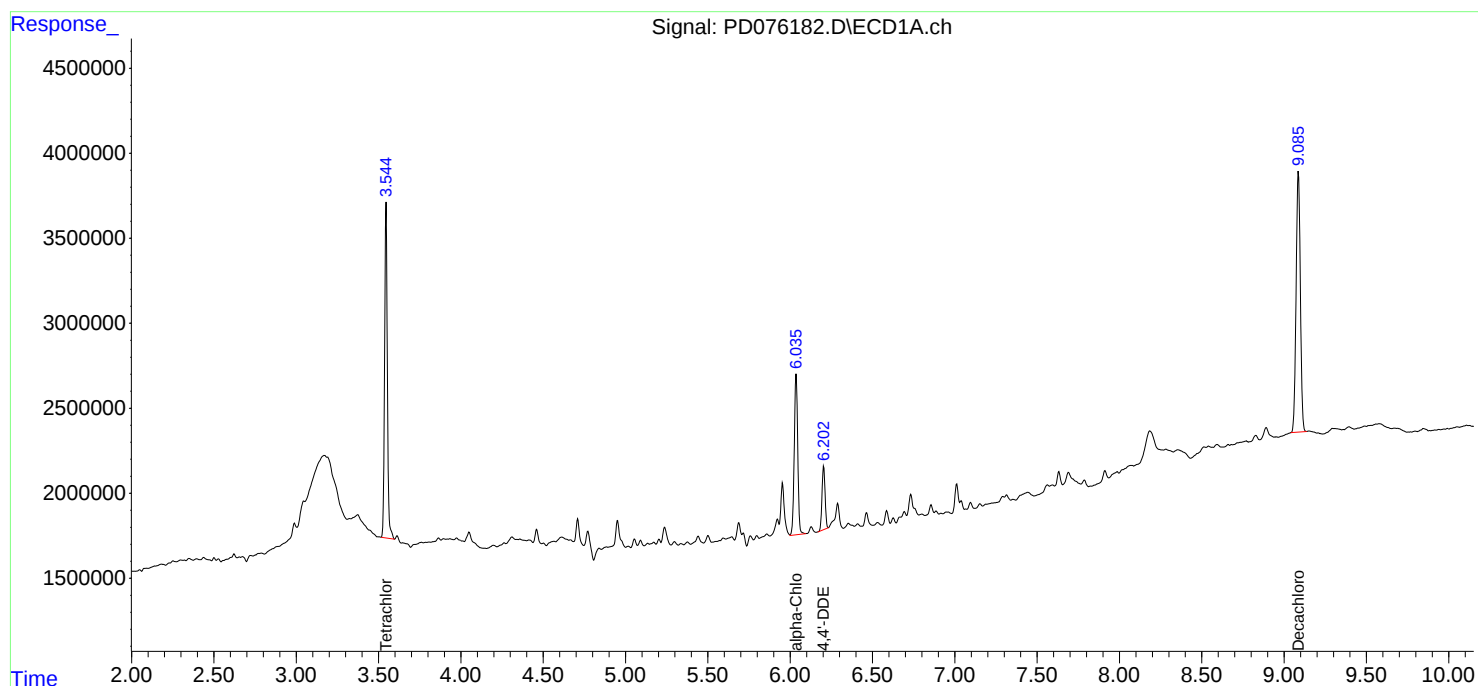


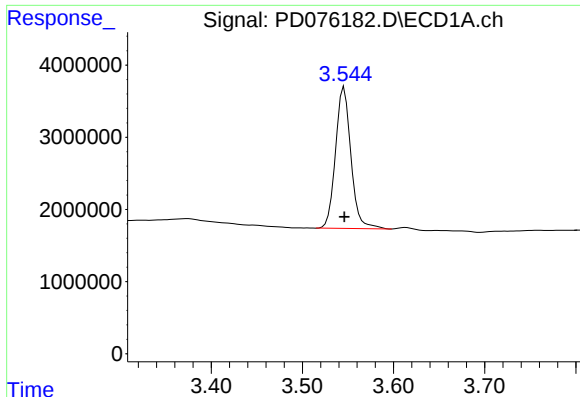

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 23021327
Conc: 10.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
SF-9

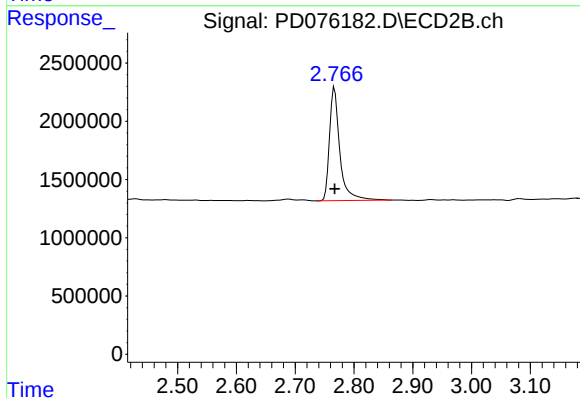


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 11918906
Conc: 10.99 ng/ml

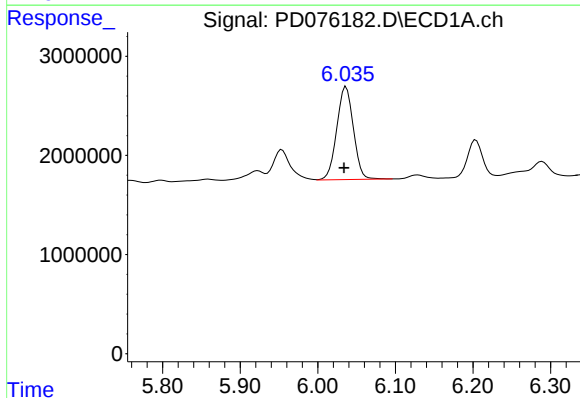


#11 alpha-Chlordane

R.T.: 6.037 min
Delta R.T.: 0.003 min
Response: 13984564
Conc: 4.33 ng/ml

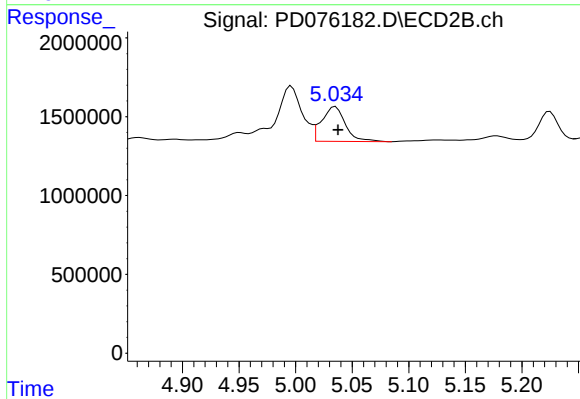

#11 alpha-Chlordane


R.T.: 5.035 min
Delta R.T.: -0.002 min
Response: 3217555
Conc: 2.35 ng/ml

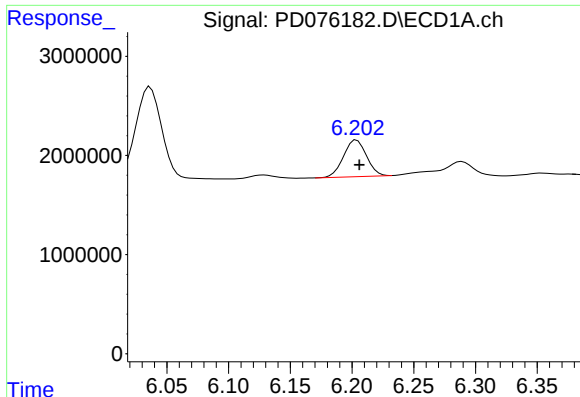

#12 4,4'-DDE


R.T.: 6.204 min
Delta R.T.: -0.002 min
Response: 4790162
Conc: 1.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
SF-9

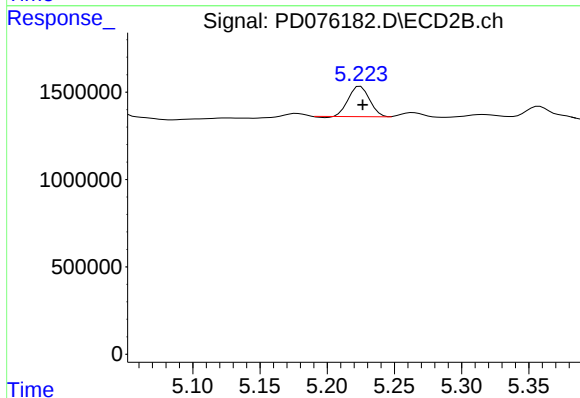


#12 4,4'-DDE

R.T.: 5.225 min
Delta R.T.: -0.002 min
Response: 1885410
Conc: 1.69 ng/ml

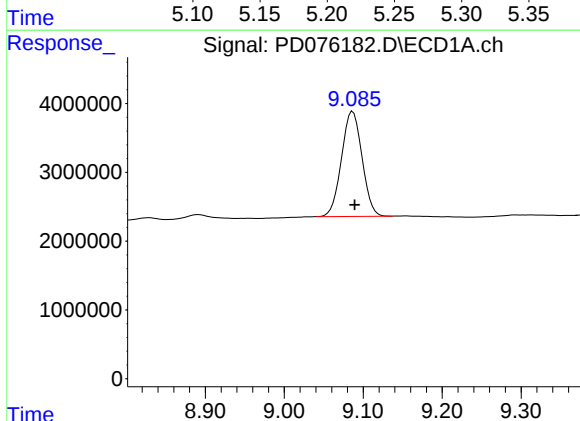

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.002 min
Response: 27605687
Conc: 10.90 ng/ml

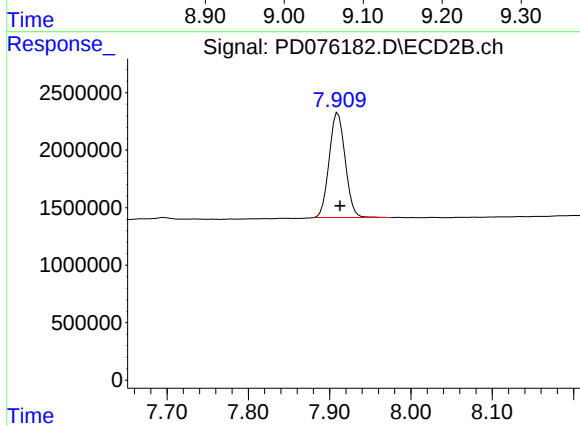

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.002 min
Response: 12504821
Conc: 12.79 ng/ml