

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062624\
 Data File : PD083812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jun 2024 13:55
 Operator : AR\AJ
 Sample : RESC034
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC036

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 04:40:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 04:33:52 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	20577261	109.0E6	20.267	20.105
2)	SA Decachlor...	9.116	7.897	86256301	270.6E6	40.482	40.498
Target Compounds							
2)	A alpha-BHC	4.019	3.270	18127635	88707529	9.582	9.840
3)	MA gamma-BHC...	4.353	3.599	17735229	85756079	9.610	10.018
4)	MA Heptachlor	4.945	3.936	19751818	83159836	9.853	9.876
5)	MB Aldrin	5.289	4.216	20397328	85261506	10.042	10.106
6)	B beta-BHC	4.550	3.895	8469994	37035197	10.084	9.768
7)	B delta-BHC	4.799	4.124	20454494	87386556	9.650	9.574
8)	B Heptachlo...	5.717	4.717	18129791	77767070	9.312	9.901
9)	A Endosulfan I	6.104	5.086	18694080	72222046	10.093	10.394
10)	B trans-Chl...	5.974	4.966	18749893	75926594	9.848	9.826
11)	B cis-Chlor...	6.053	5.030	19394908	77153223	9.908	9.802
12)	B 4,4'-DDE	6.225	5.217	38726192	148.9E6	19.551	19.882
13)	MA Dieldrin	6.380	5.350	38806203	155.7E6	19.380	20.116
14)	MA Endrin	6.611	5.625	32437660	135.1E6	19.612	20.407
15)	B Endosulfa...	6.831	5.919	36097436	132.9E6	19.800	19.914
16)	A 4,4'-DDD	6.744	5.772	27888000	119.6E6	19.330	20.076
17)	MA 4,4'-DDT	7.060	6.022	30078846	114.8E6	19.891	19.637
18)	B Endrin al...	6.961	6.098	27037674	101.6E6	19.771	20.267
19)	B Endosulfa...	7.197	6.321	35127892	131.3E6	19.821	20.212
20)	A Methoxychlor	7.536	6.598	90860181	319.3E6	102.124	108.055
21)	B Endrin ke...	7.684	6.827	39604686	148.5E6	20.285	21.145

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062624\
Data File : PD083812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2024 13:55
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 04:40:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 04:33:52 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

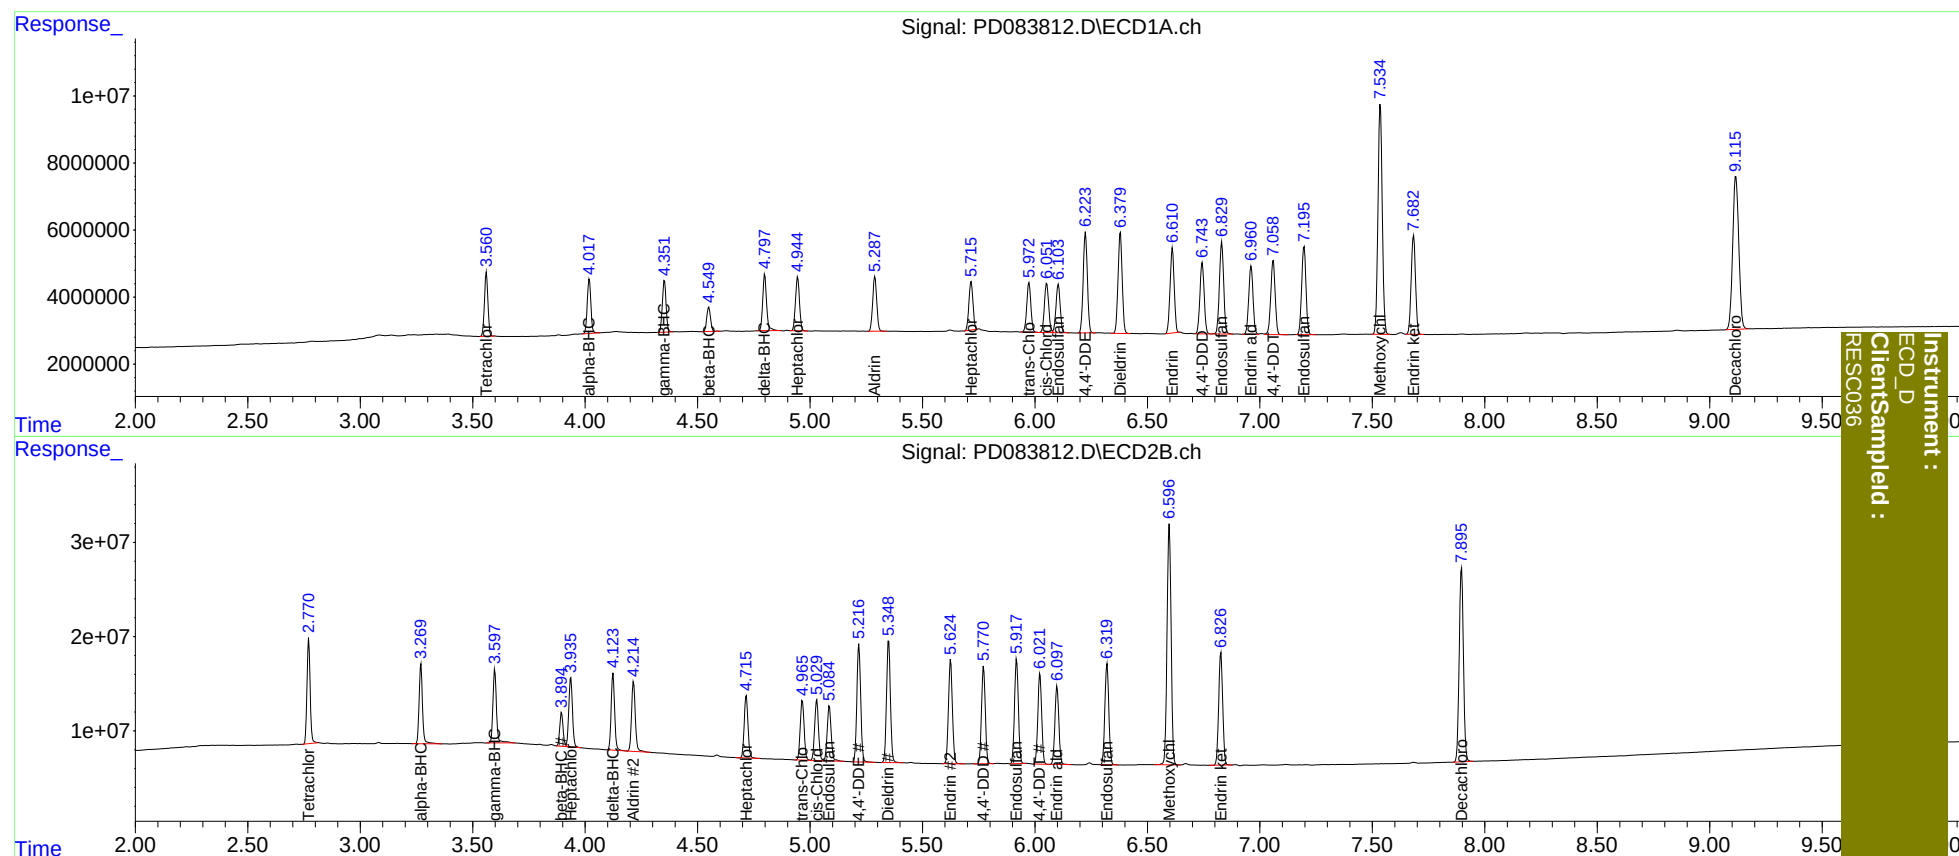

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062624\
Data File : PD083812.D
Acq On : 26 Jun 2024 13:55
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Title : GC Extractables
Last Update : Thu Jun 27 04:33:52 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.561	4.019	100.00%
4.019	4.353	100.00%
4.353	4.550	100.00%
4.550	4.799	100.00%
4.799	4.945	100.00%
4.945	5.289	100.00%
5.289	5.717	100.00%
5.717	5.974	100.00%
5.974	6.053	100.00%
6.053	6.104	97.49%
6.104	6.225	100.00%
6.225	6.380	100.00%
6.380	6.611	100.00%
6.611	6.744	100.00%
6.744	6.831	100.00%
6.831	6.961	100.00%
6.961	7.060	100.00%
7.060	7.197	100.00%
7.197	7.536	100.00%
7.536	7.684	100.00%
7.684	9.116	100.00%

Signal #2


2.771	3.270	100.00%
3.270	3.599	100.00%
3.599	3.895	100.00%
3.895	3.936	96.07%
3.936	4.124	100.00%
4.124	4.216	100.00%
4.216	4.717	100.00%
4.717	4.966	100.00%
4.966	5.030	100.00%
5.030	5.086	98.64%
5.086	5.217	100.00%
5.217	5.350	100.00%
5.350	5.625	100.00%
5.625	5.772	100.00%
5.772	5.919	100.00%
5.919	6.022	100.00%
6.022	6.098	100.00%
6.098	6.321	100.00%
6.321	6.598	100.00%
6.598	6.827	100.00%
6.827	7.897	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062624\
Data File : PD083812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2024 13:55
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 17:55:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 26 17:50:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

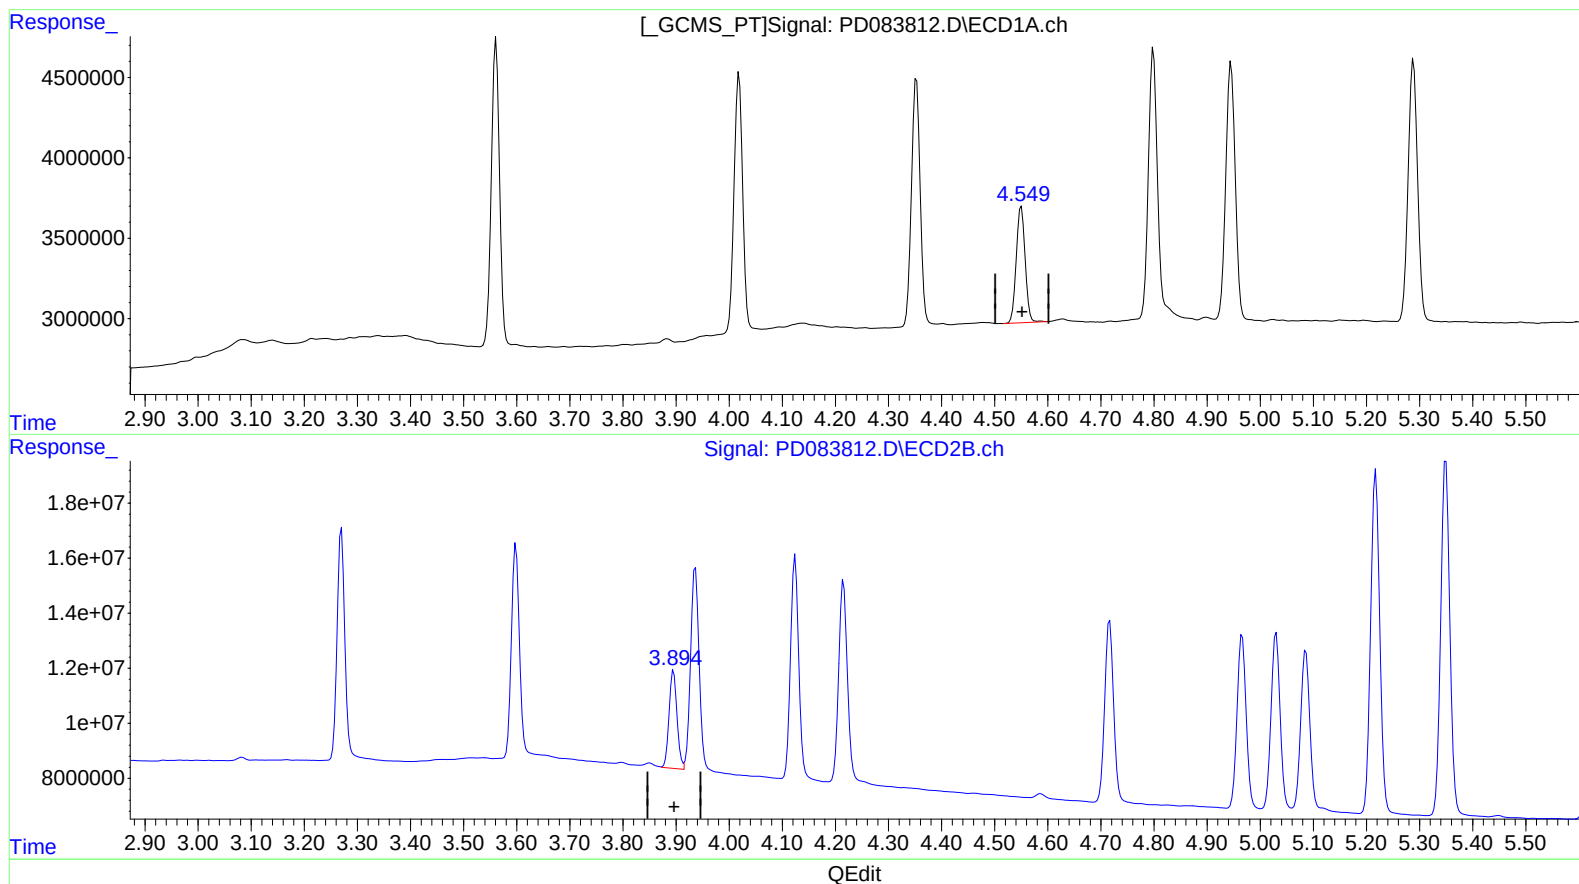

(6) beta-BHC (B)
4.550min 10.084 ng/ml
response 8469994


(6) beta-BHC #2 (B)
3.895min 9.768 ng/ml
response 37035197

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062624\
Data File : PD083812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jun 2024 13:55
Operator : AR\AJ
Sample : RESC034
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 26 17:55:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062624CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 26 17:50:15 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

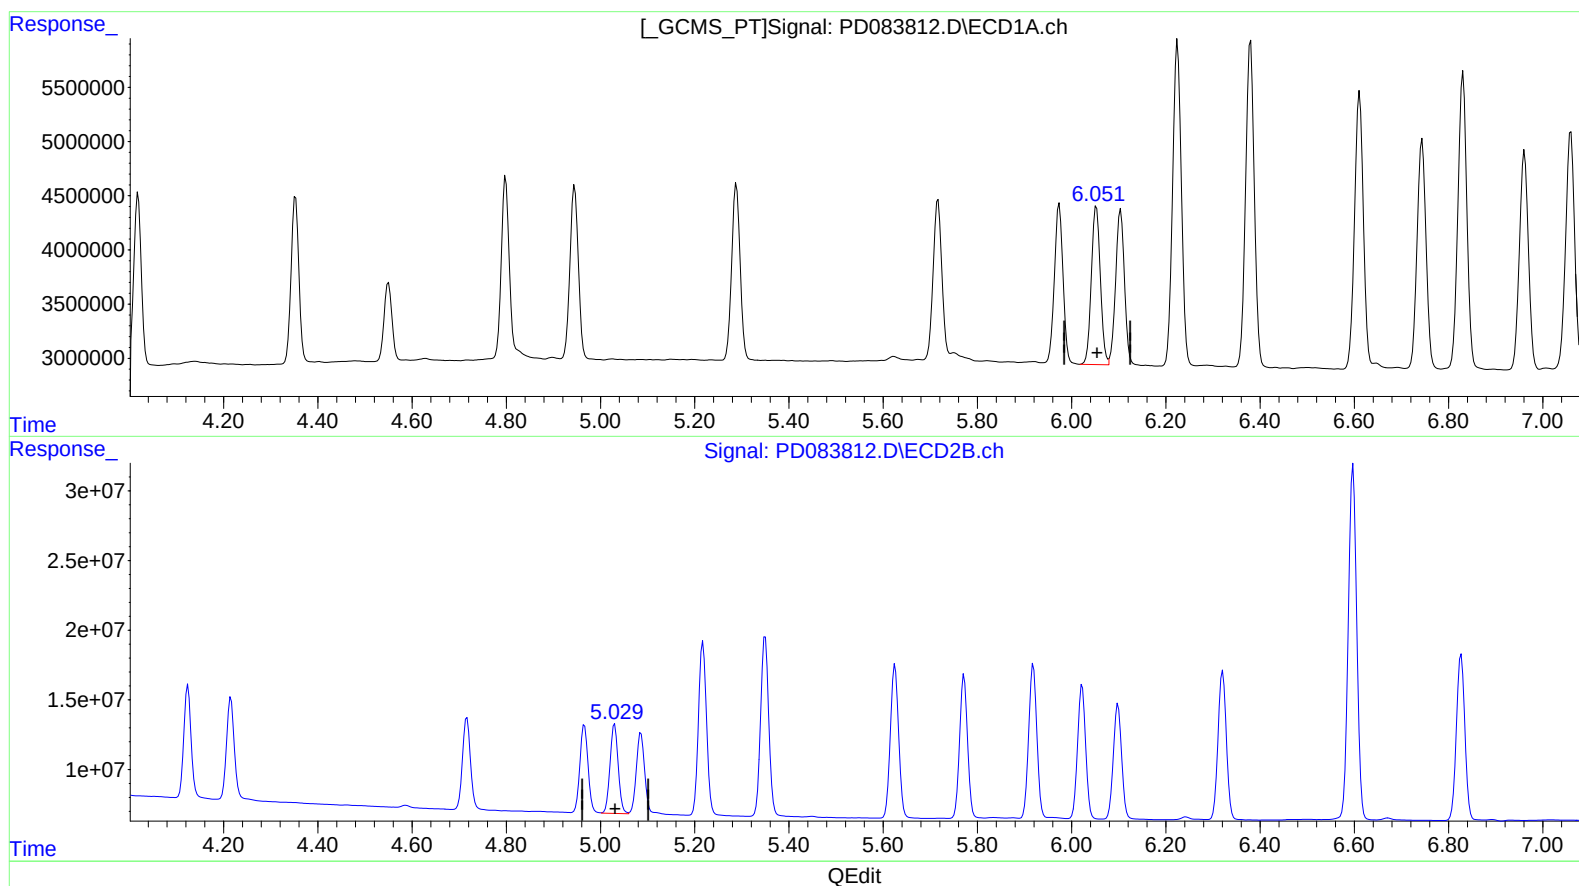

(11) cis-Chlordane (B)

6.053min 9.908 ng/ml

response 19394908

(11) cis-Chlordane #2 (B)

5.030min 9.802 ng/ml

response 77153223