

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062719\
 Data File : PD053734.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jun 2019 9:54
 Operator : SM\AJ
 Sample : PIBLK02
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 07:41:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062019CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 08:58:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.983	15331556	24274525	21.138	21.524
27)	SA Decachlor...	8.012	9.027	27790518	40431736	44.159	41.375


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062719\
Data File : PD053734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jun 2019 9:54
Operator : SM\AJ
Sample : PIBLK02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 07:41:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062019CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 08:58:58 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

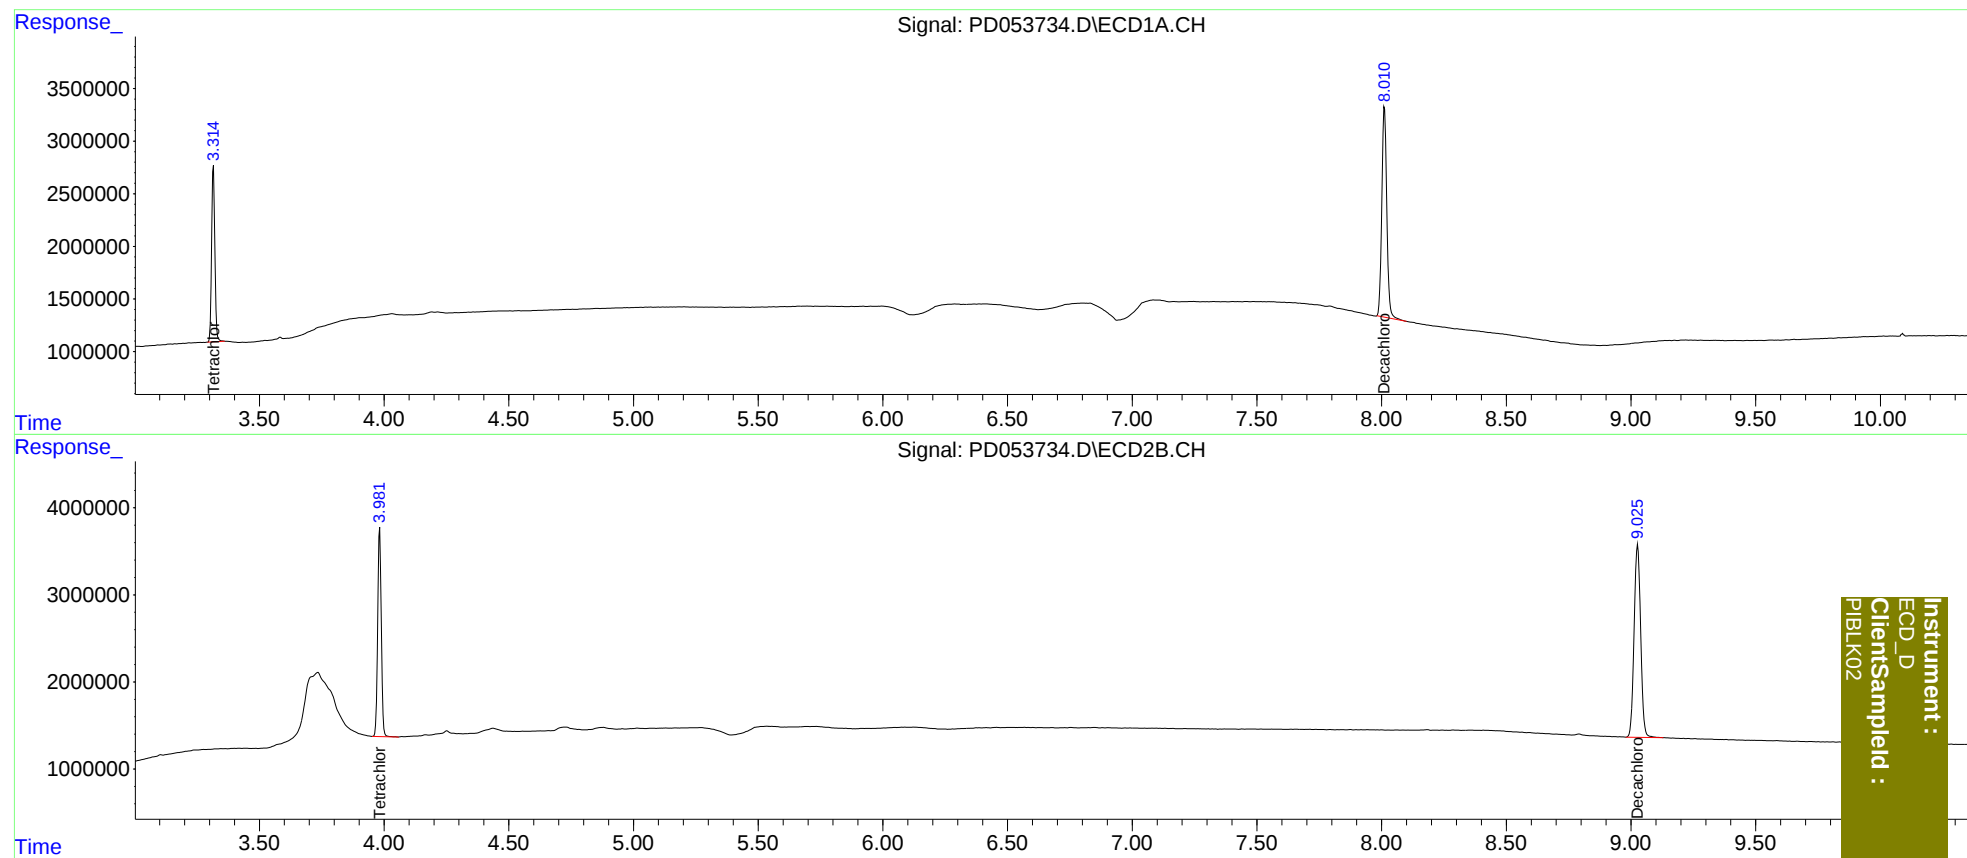


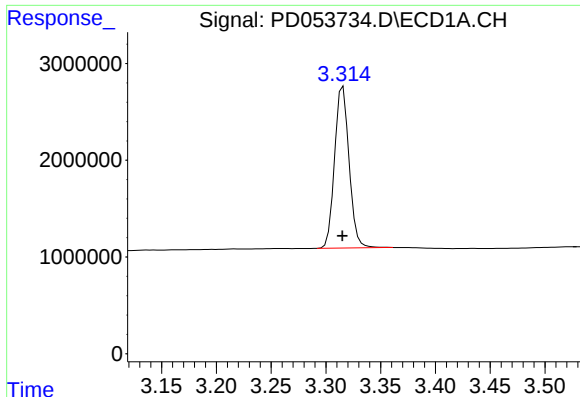

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: 0.000 min
Response: 15331556
Conc: 21.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK02

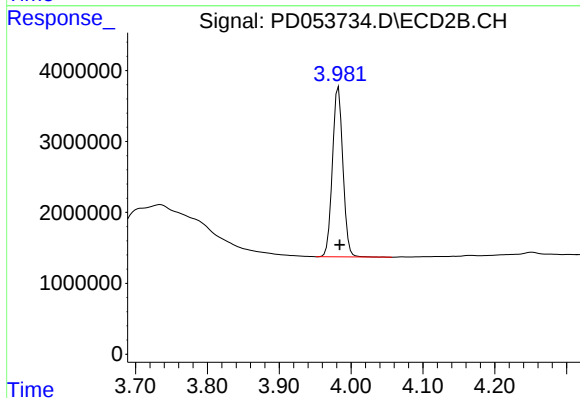


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.002 min
Response: 24274525
Conc: 21.52 ng/ml

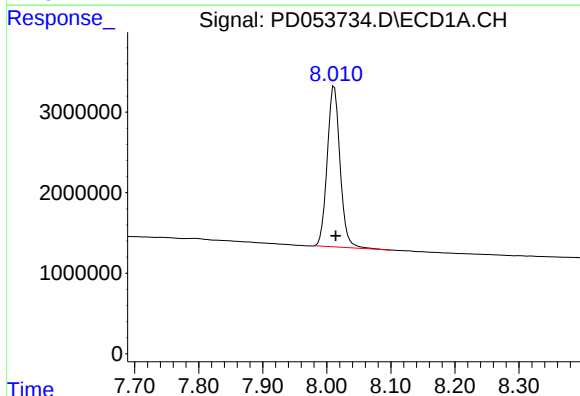

#27 Decachlorobiphenyl

R.T.: 8.012 min
Delta R.T.: -0.002 min
Response: 27790518
Conc: 44.16 ng/ml

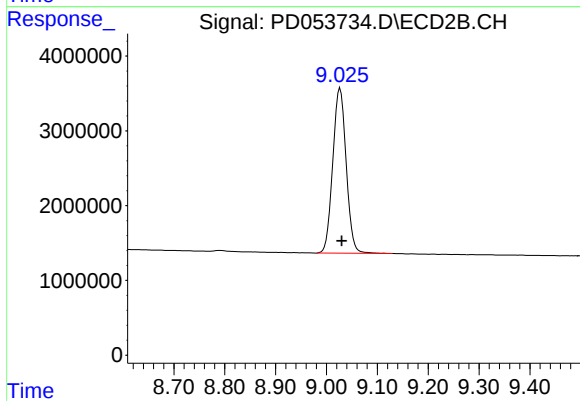

#27 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.003 min
Response: 40431736
Conc: 41.38 ng/ml