

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
 Data File : PD083832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2024 13:50
 Operator : AR\AJ
 Sample : RESC035
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC037

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 19:06:19 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 19:01:18 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	20647895	115.3E6	20.808	20.834
27)	SA Decachlor...	9.119	7.897	85456054	269.8E6	41.375	41.523
Target Compounds							
2)	A alpha-BHC	4.018	3.270	18000563	92023982	9.427	10.188
3)	MA gamma-BHC...	4.353	3.599	17868131	86346600	9.573	10.206
4)	MA Heptachlor	4.945	3.937	19390968	87126276	9.833	10.389
5)	MB Aldrin	5.288	4.215	19992807	87461147	10.097	10.441
6)	B beta-BHC	4.550	3.896	8209001	39233564	10.335	10.255
7)	B delta-BHC	4.799	4.125	20345372	90556362	9.863	10.061
8)	B Heptachlo...	5.716	4.717	18791009	79024511	9.996	10.333
9)	A Endosulfan I	6.104	5.086	18581960	72754879	10.188	10.518
10)	B trans-Chl...	5.974	4.966	18339114	76508871	9.911	10.141
11)	B cis-Chlor...	6.053	5.030	18907277	77166754	9.938	10.120
12)	B 4,4'-DDE	6.225	5.218	37381383	149.0E6	19.403	20.442
13)	MA Dieldrin	6.379	5.350	38874578	160.8E6	19.402	20.978
14)	MA Endrin	6.612	5.625	30511492	130.9E6	19.649	21.119
15)	B Endosulfa...	6.831	5.919	35000431	132.8E6	19.869	20.788
16)	A 4,4'-DDD	6.745	5.772	27902314	124.9E6	19.044	20.827
17)	MA 4,4'-DDT	7.060	6.022	28365807	112.8E6	19.159	19.747
18)	B Endrin al...	6.961	6.098	27471422	106.3E6	20.908	22.083
19)	B Endosulfa...	7.198	6.321	34246469	131.4E6	20.092	21.058
20)	A Methoxychlor	7.537	6.597	86131200	308.7E6	102.494	113.022
21)	B Endrin ke...	7.685	6.826	39478955	151.4E6	20.912	22.603

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
Data File : PD083832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 13:50
Operator : AR\AJ
Sample : RESC035
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 19:06:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 19:01:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

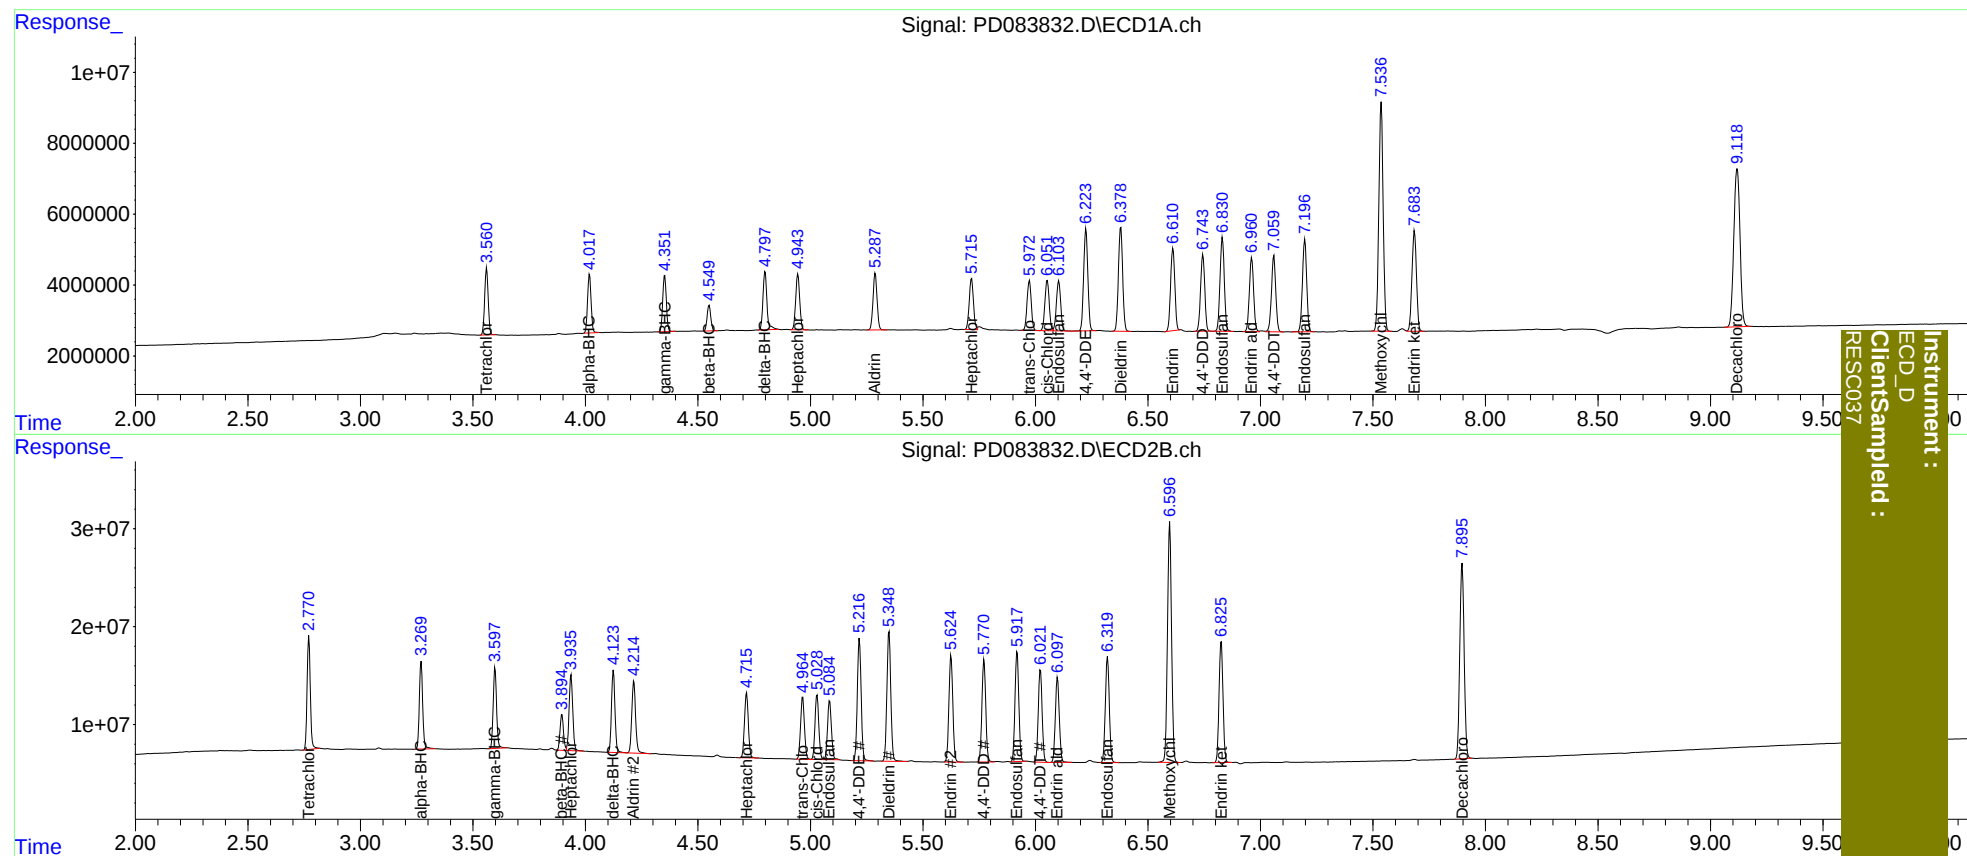

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
Data File : PD083832.D
Acq On : 27 Jun 2024 13:50
Operator : AR\AJ
Sample : RESC035
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC037

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Title : GC Extractables
Last Update : Thu Jun 27 19:01:18 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.561	4.018	100.00%
4.018	4.353	100.00%
4.353	4.550	100.00%
4.550	4.799	100.00%
4.799	4.945	100.00%
4.945	5.288	100.00%
5.288	5.716	100.00%
5.716	5.974	100.00%
5.974	6.053	100.00%
6.053	6.104	97.36%
6.104	6.225	100.00%
6.225	6.379	100.00%
6.379	6.612	100.00%
6.612	6.745	100.00%
6.745	6.831	100.00%
6.831	6.961	100.00%
6.961	7.060	100.00%
7.060	7.198	100.00%
7.198	7.537	100.00%
7.537	7.685	100.00%
7.685	9.119	100.00%

Signal #2


2.771	3.270	100.00%
3.270	3.599	100.00%
3.599	3.896	100.00%
3.896	3.937	92.24%
3.937	4.125	100.00%
4.125	4.215	99.64%
4.215	4.717	100.00%
4.717	4.966	100.00%
4.966	5.030	99.33%
5.030	5.086	99.40%
5.086	5.218	100.00%
5.218	5.350	100.00%
5.350	5.625	100.00%
5.625	5.772	100.00%
5.772	5.919	100.00%
5.919	6.022	100.00%
6.022	6.098	100.00%
6.098	6.321	100.00%
6.321	6.597	100.00%
6.597	6.826	100.00%
6.826	7.897	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
Data File : PD083832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 13:50
Operator : AR\AJ
Sample : RESC035
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC037

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 19:06:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 19:01:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

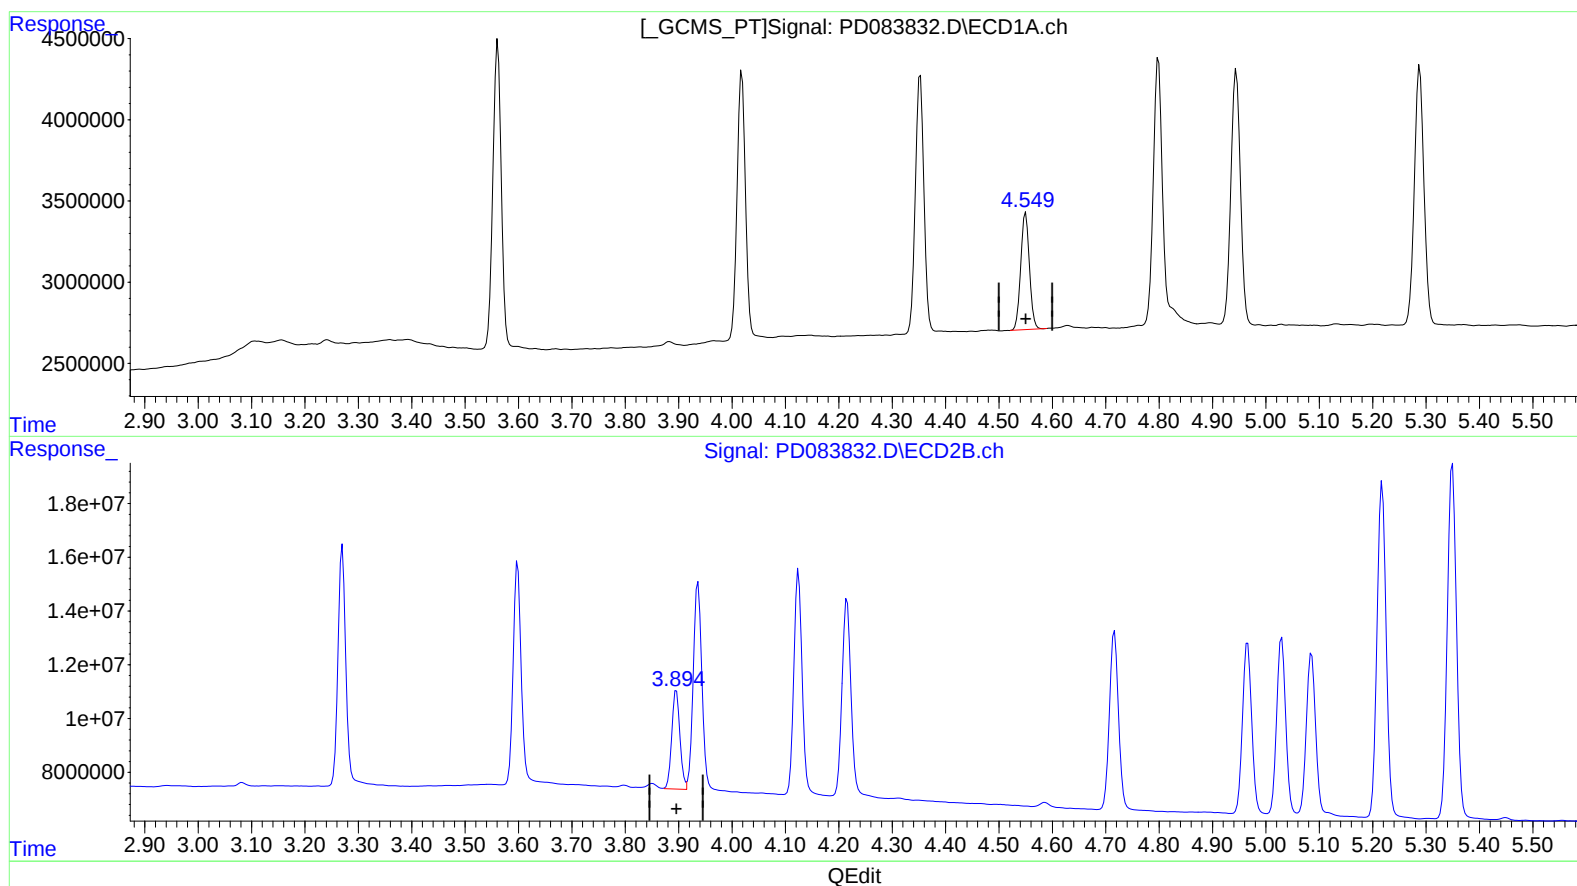

(6) beta-BHC (B)

4.550min 10.335 ng/ml

response 8209001

(6) beta-BHC #2 (B)

3.896min 10.255 ng/ml


response 39233564

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
Data File : PD083832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 13:50
Operator : AR\AJ
Sample : RESC035
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC037

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 19:06:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 19:01:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

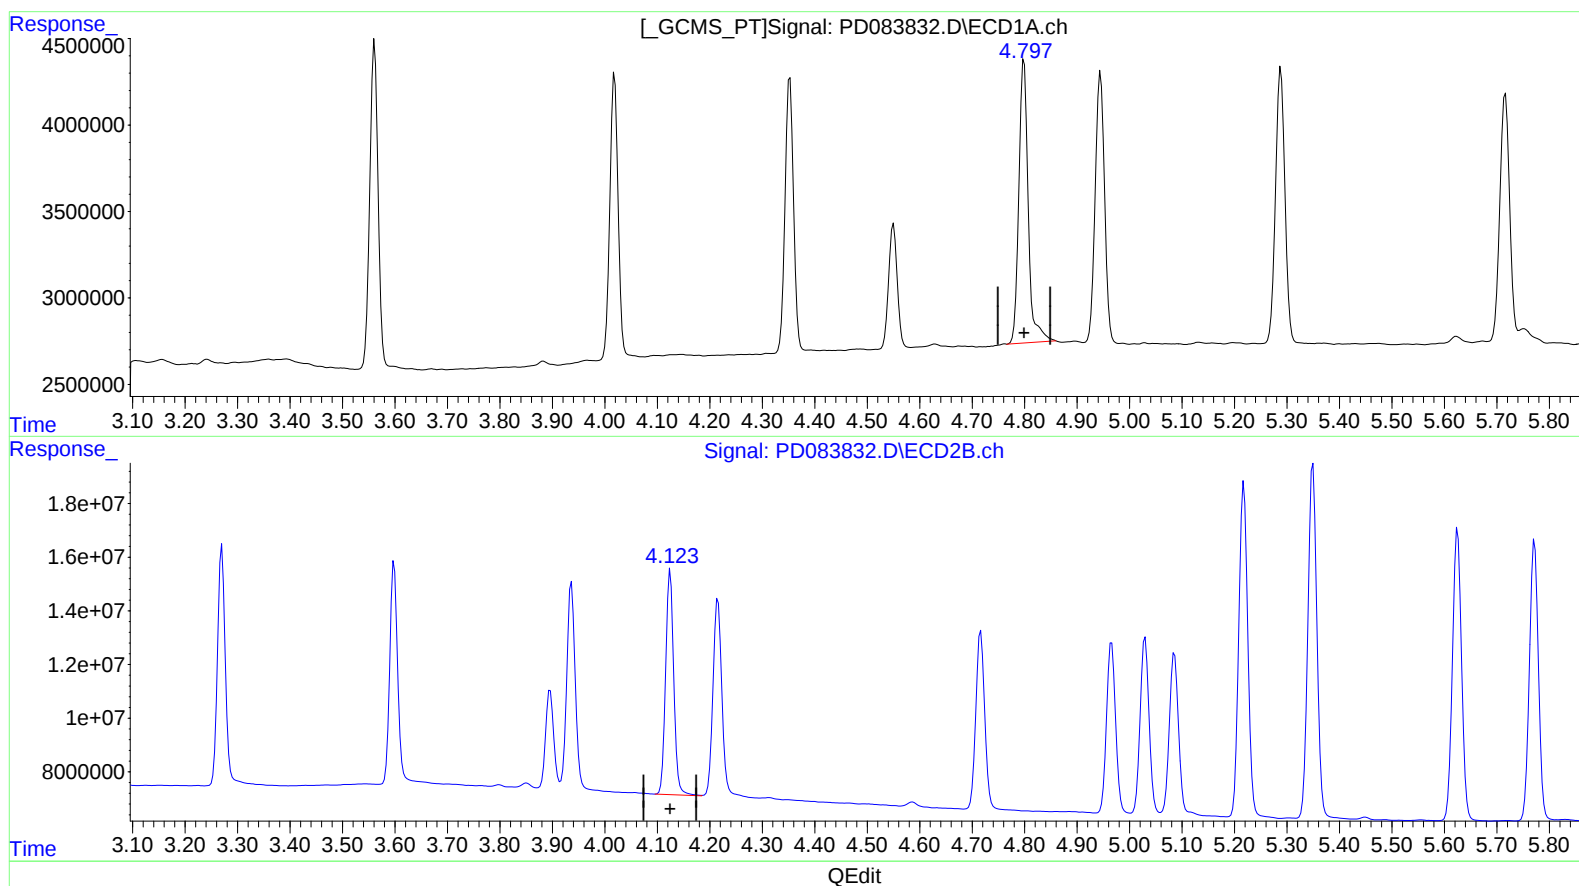

(7) delta-BHC (B)

4.799min 9.863 ng/ml

response 20345372

(7) delta-BHC #2 (B)

4.125min 10.061 ng/ml


response 90556362

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
Data File : PD083832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 13:50
Operator : AR\AJ
Sample : RESC035
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC037

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 19:06:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 19:01:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

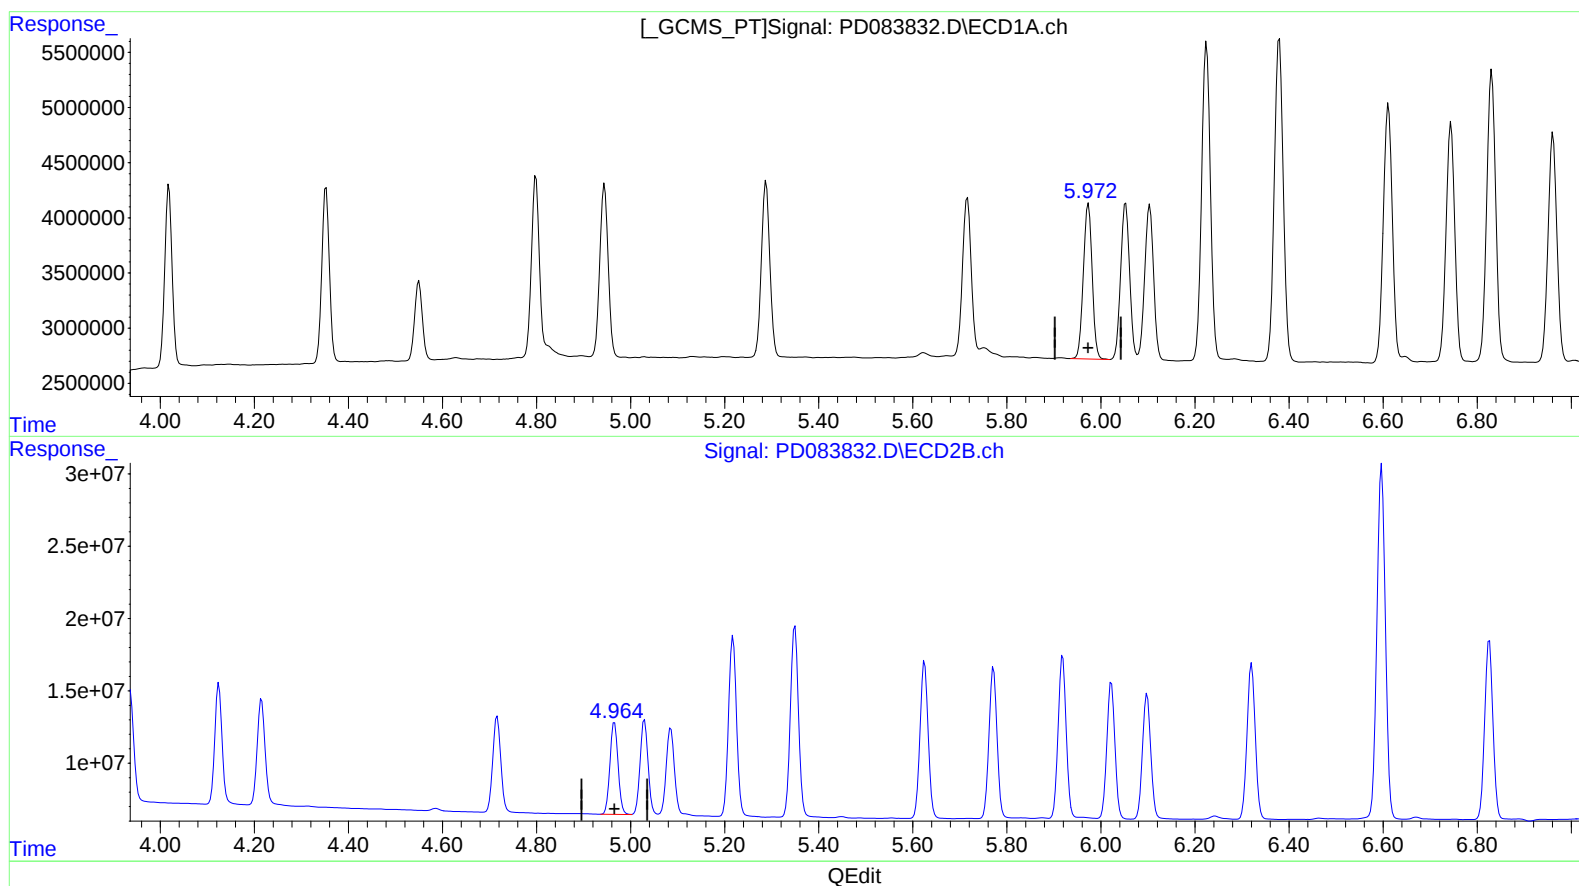

(10) trans-Chlordane (B)

5.974min 9.911 ng/ml

response 18339114

(10) trans-Chlordane #2 (B)

4.966min 10.141 ng/ml


response 76508871

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
Data File : PD083832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 13:50
Operator : AR\AJ
Sample : RESC035
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC037

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 19:06:19 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 19:01:18 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

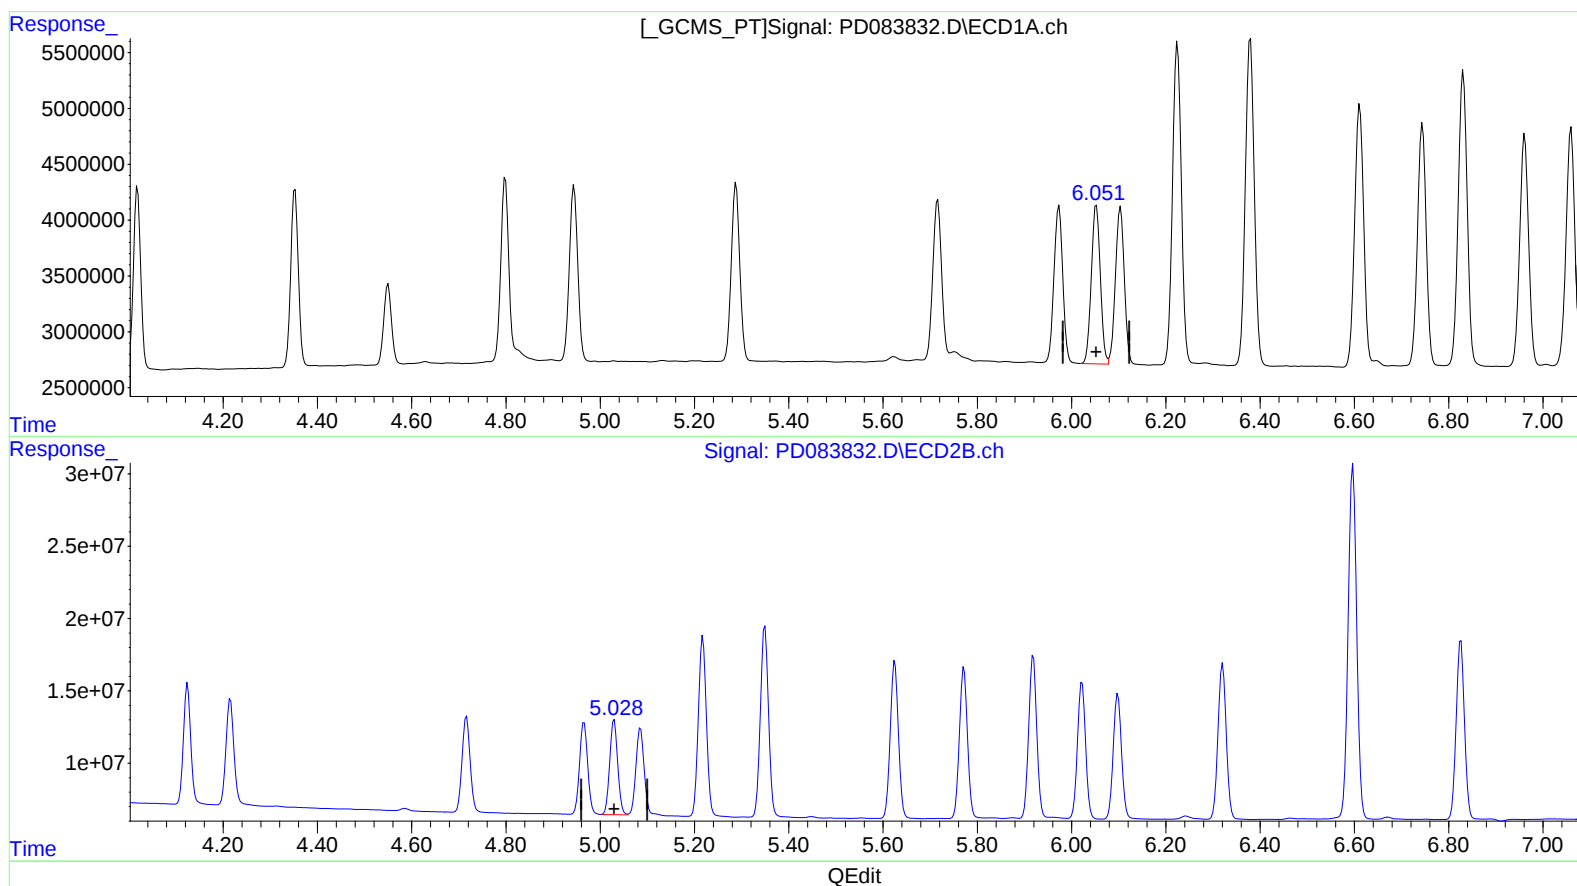

(11) cis-Chlordane (B)

6.053min 9.938 ng/ml

response 18907277

(11) cis-Chlordane #2 (B)

5.030min 10.120 ng/ml

response 77166754