

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
 Data File : PD083842.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jun 2024 16:03
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2026

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 18:18:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 27 18:05:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	9998020	57242524	9.999	10.240
27)	SA Decachlor...	9.116	7.896	41922958	136.9E6	20.273	21.035
Target Compounds							
2)	A alpha-BHC	4.018	3.270	17376147	88710956	9.188	9.716
3)	MA gamma-BHC...	4.353	3.599	17391294	84468463	9.376	9.860
4)	MA Heptachlor	4.944	3.936	18839924	84048482	9.601	9.912
9)	A Endosulfan I	6.104	5.085	17903225	70583568	9.800	10.106
13)	MA Dieldrin	6.379	5.350	37592857	154.7E6	18.794	19.884
14)	MA Endrin	6.610	5.625	29302341	124.6E6	18.820	19.703
16)	A 4,4'-DDD	6.744	5.772	27379622	120.3E6	18.740	19.826
17)	MA 4,4'-DDT	7.060	6.022	26568488	108.7E6	17.971	18.650
20)	A Methoxychlor	7.536	6.597	82874003	297.3E6	97.755	106.215

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062724\
Data File : PD083842.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jun 2024 16:03
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 18:18:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062724CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 27 18:05:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

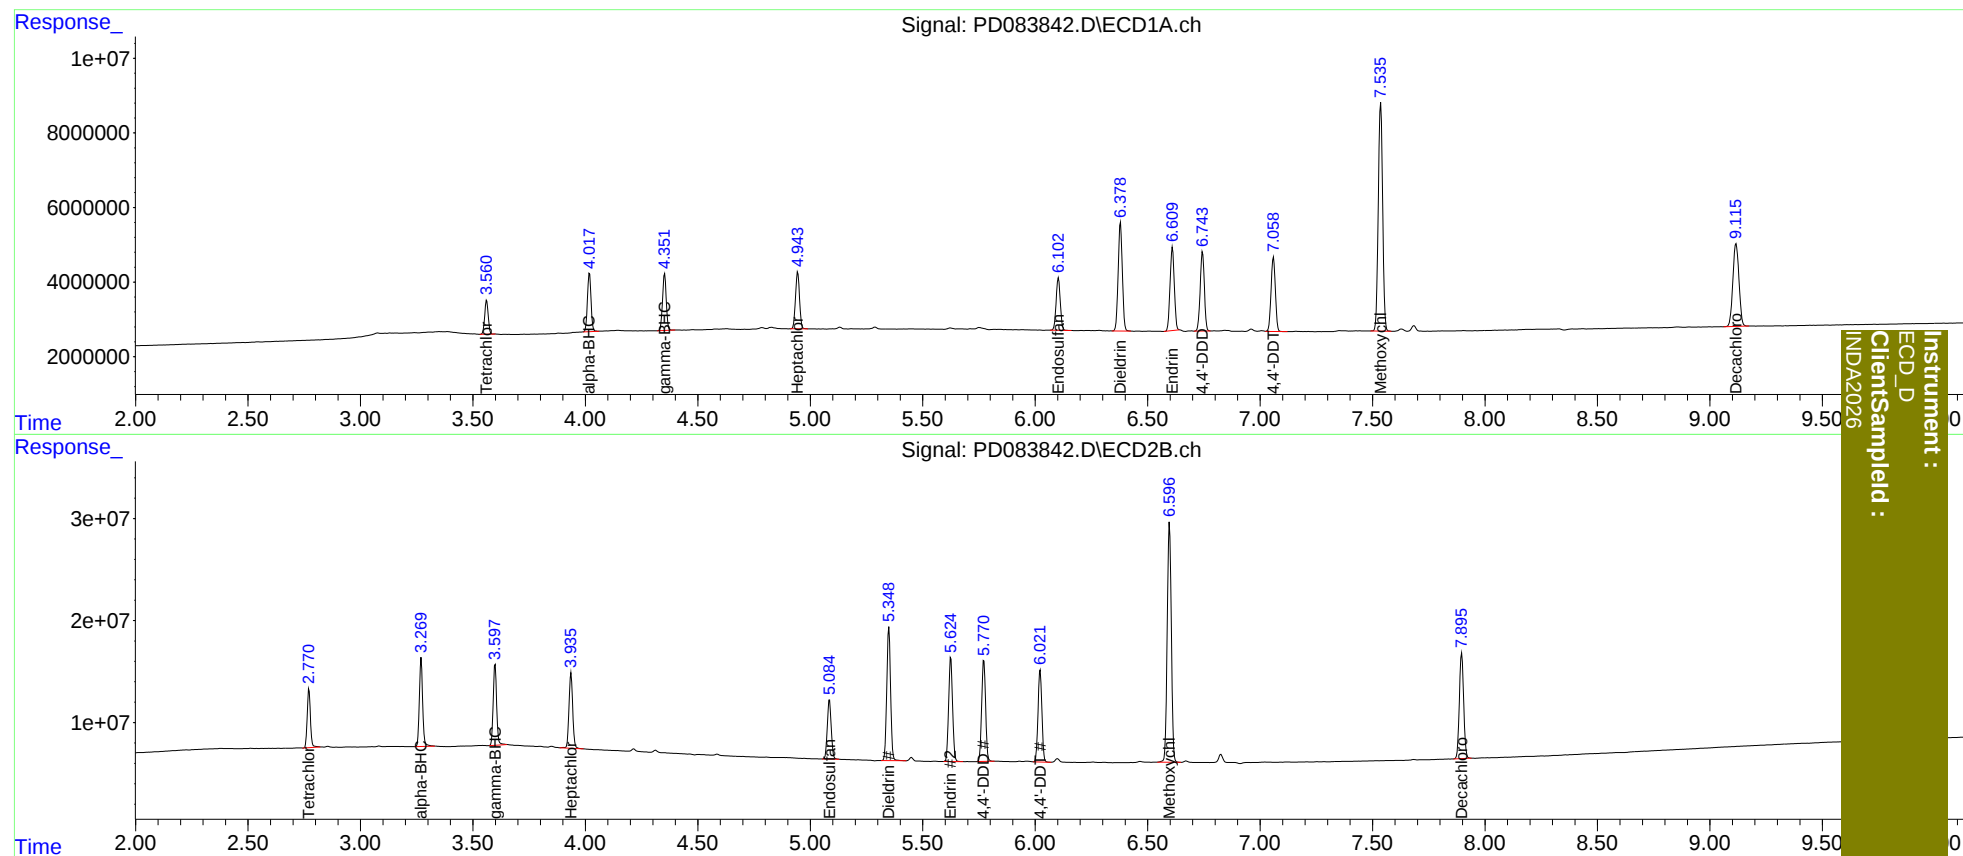

Instrument :
ECD_D
ClientSampled :
INDA2026