

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062822\
 Data File : PD070566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 22:23
 Operator : AR\AJ
 Sample : PB145738BS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS738

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/29/2022
 Supervised By :Ankita Jodhani 06/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 02:43:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062822CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 29 02:34:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.990	29247912	216.9E6	18.292	20.409
27)	SA Decachlor...	8.094	9.047	64825035	307.5E6	39.655	41.342
Target Compounds							
2)	A alpha-BHC	3.794	4.375	9853235	79604114	4.123	4.940
3)	MA gamma-BHC...	4.074	4.658	9872511	78873453	4.378	5.156
4)	MA Heptachlor	4.365	5.172	9916968	77627211	4.607m	5.415
5)	MB Aldrin	4.609	5.477	10636420	80569150	4.754	5.446
6)	B beta-BHC	4.324	4.823	4609076	35134541	4.435	5.264
7)	B delta-BHC	4.524	5.037	7648072	53254540	3.262	3.653m
8)	B Heptachlo...	5.051	5.858	9792170	70932142	4.749	5.488m
9)	A Endosulfan I	5.387	6.217	8517421	67733022	4.506	5.507
10)	B trans-Chl...	5.276	6.095	9848498	71813227	4.602	5.244
11)	B cis-Chlor...	5.334	6.168	9770040	71673738	4.674	5.417
12)	B 4,4'-DDE	5.500	6.323	17857712	140.2E6	8.769m	10.838
13)	MA Dieldrin	5.628	6.471	19317826	144.9E6	9.091	10.885m
14)	MA Endrin	5.885	6.689	16973261	129.3E6	9.389	11.957 #
15)	B Endosulfa...	6.160	6.894	16868459	119.2E6	9.627	10.987
16)	A 4,4'-DDD	6.018	6.807	15262130	112.3E6	9.034	10.592m
17)	MA 4,4'-DDT	6.257	7.109	13217290	105.2E6	8.179	10.411 #
18)	B Endrin al...	6.330	7.018	15320643	99987448	10.107	10.938
19)	B Endosulfa...	6.543	7.241	15001410	94958084	8.419	9.255
20)	A Methoxychlor	6.811	7.564	44601404	263.8E6	50.429	54.591
21)	B Endrin ke...	7.033	7.708	19497914	123.7E6	9.939	10.850

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062822\
Data File : PD070566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 22:23
Operator : AR\AJ
Sample : PB145738BS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 02:43:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062822CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 29 02:34:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

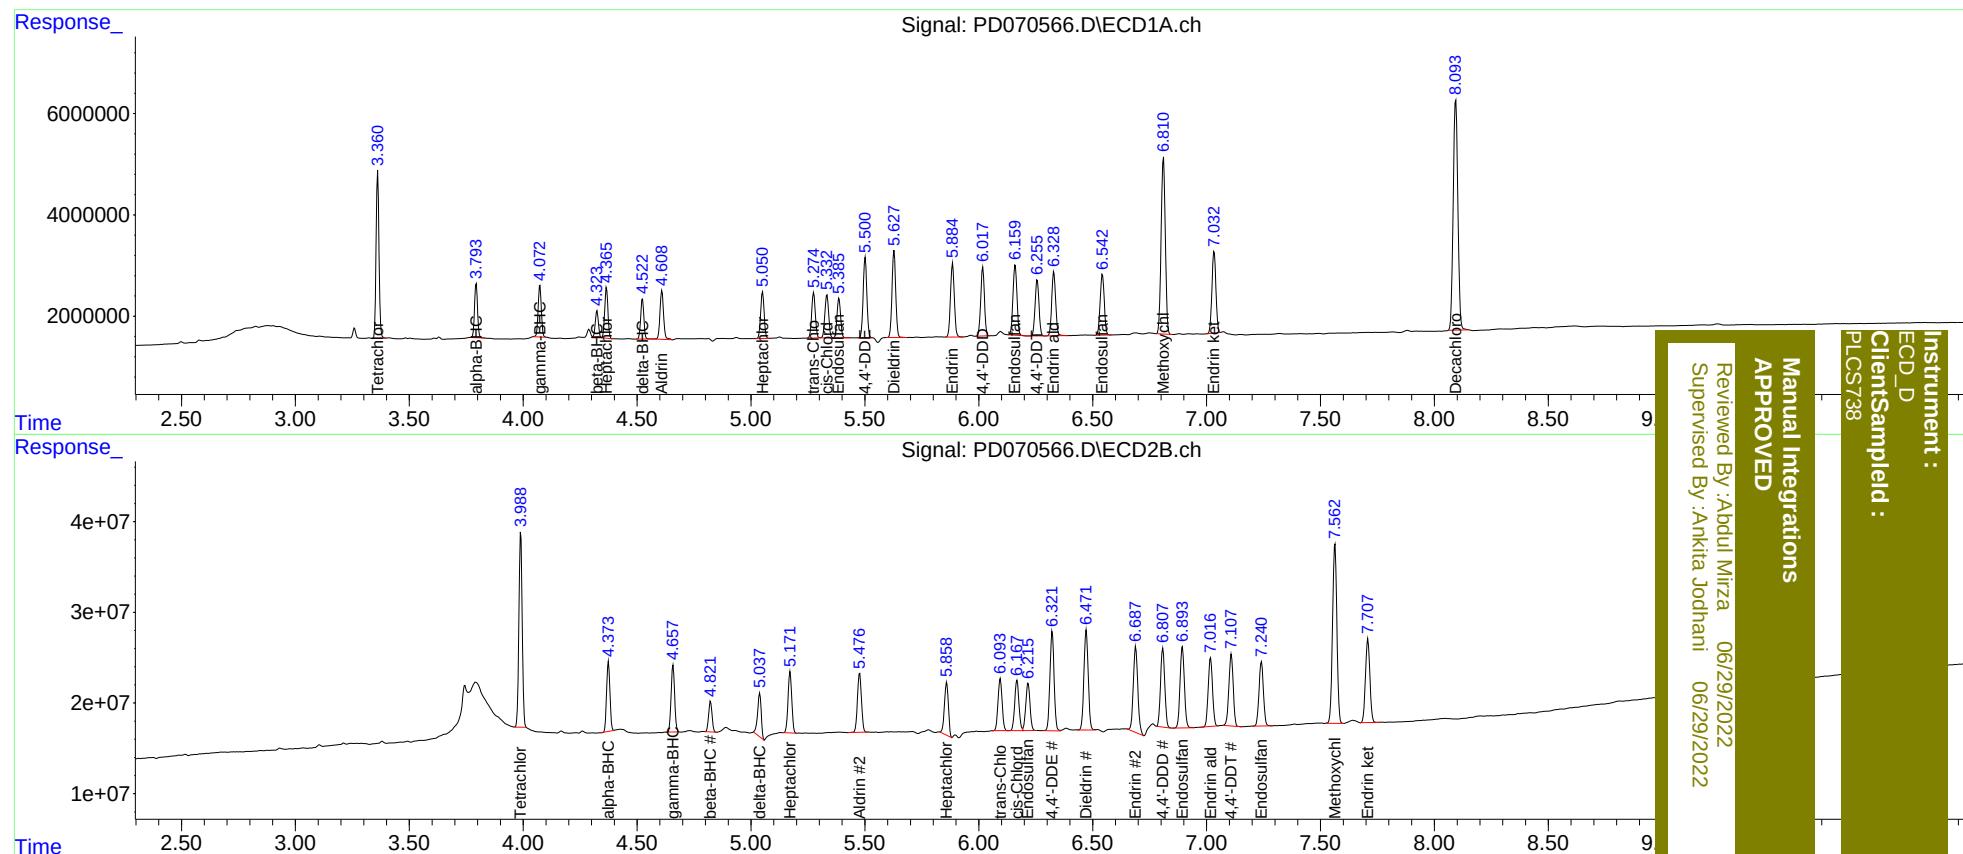

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/29/2022
Supervised By: Ankita Jodhani 06/29/2022

Instrument :
ECD_D
ClientSampled :
PLCS738