

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062822\
 Data File : PD070570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 23:19
 Operator : AR\AJ
 Sample : N3392-03 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXEX8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/29/2022
 Supervised By : Ankita Jodhani 06/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 02:45:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062822CLP-TCLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 29 02:34:55 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.377	3.990	32537089	234.0E6	20.349m	22.014
2)	SA Decachlor...	8.109	9.047	66147217	321.4E6	40.464	43.214
Target Compounds							
12)	B 4,4'-DDE	5.517	6.322	2850544	23783907	1.400m	1.839 #
14)	MA Endrin	5.907	6.713	1277834	7828000	0.707m	0.724m
16)	A 4,4'-DDD	6.034	6.808	1330082	11370139	0.787	1.073 #
17)	MA 4,4'-DDT	6.273	7.106	1719388	18438868	1.064	1.825m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062822\
Data File : PD070570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 23:19
Operator : AR\AJ
Sample : N3392-03 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 02:45:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062822CLP-TCLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 29 02:34:55 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

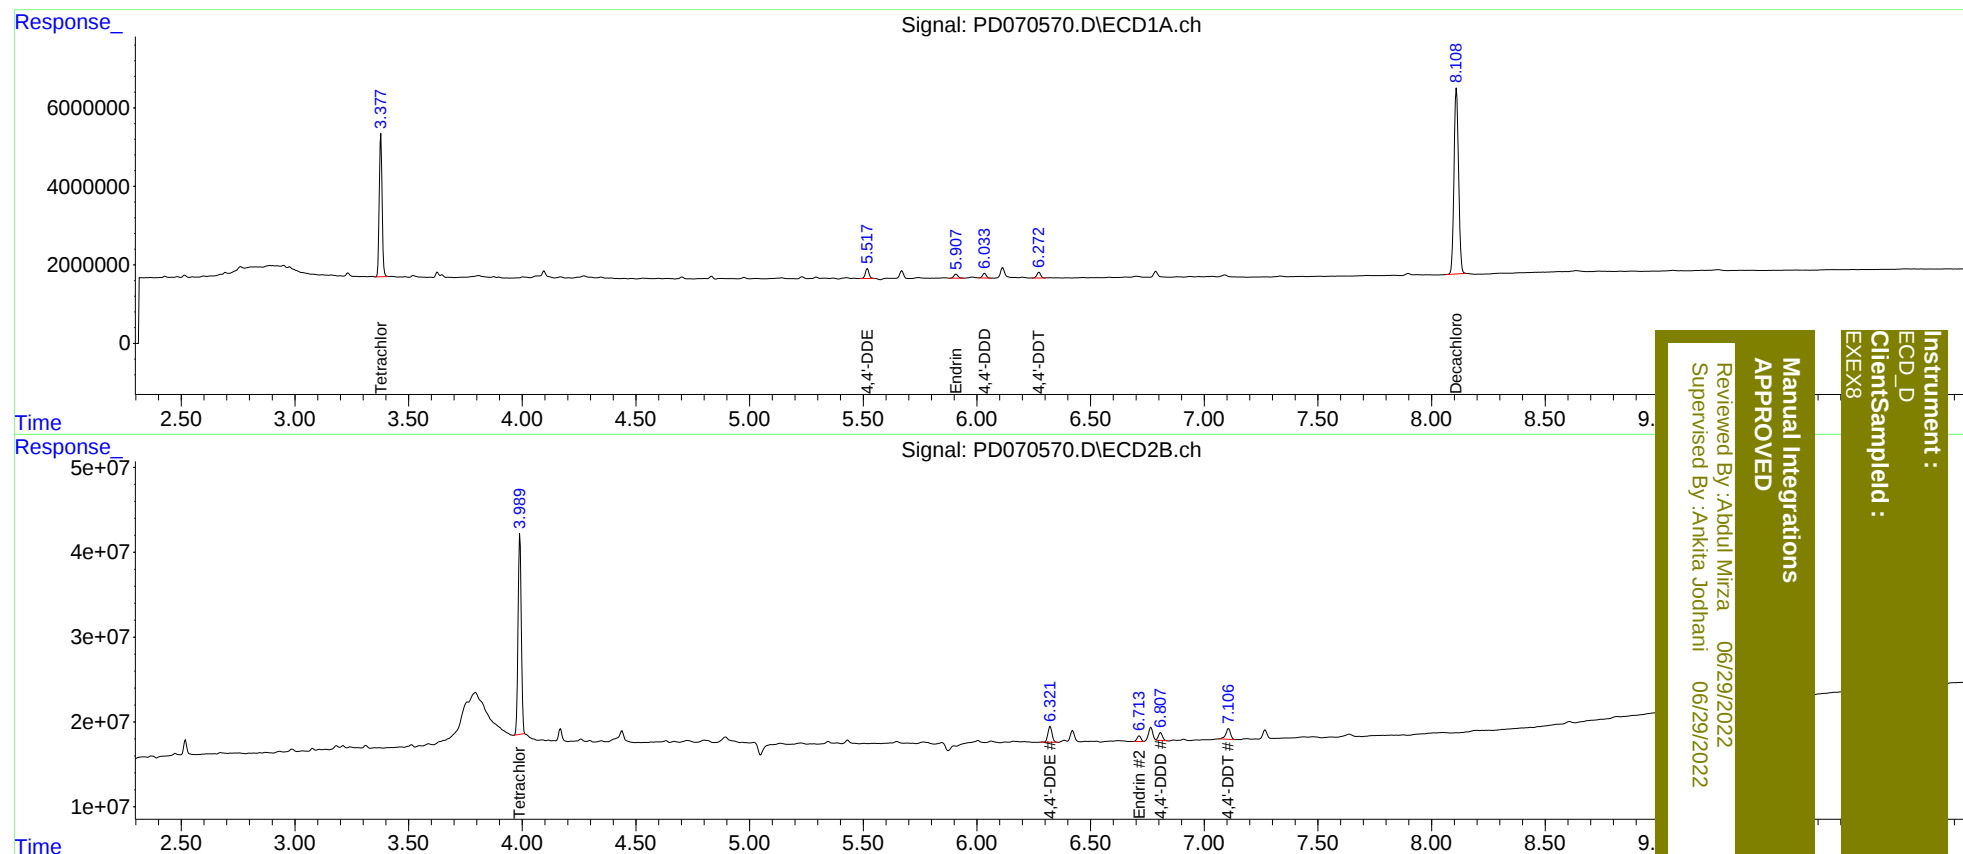

Reviewed By: Abdul Mirza 06/29/2022
Supervised By: Ankita Jodhani 06/29/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EXEX8